

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
Data File : FF012575.D
Signal(s) : FID2B.ch
Acq On : 03 May 2023 11:24
Operator : YP\AJ
Sample : 02500-15 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PT-DIES-SOIL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

Integration File: autoint1.e
Quant Time: May 04 01:23:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.001	211326	1.758 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050323\
Data File : FF012575.D
Signal(s) : FID2B.ch
Acq On : 03 May 2023 11:24
Operator : YP\AJ
Sample : 02500-15 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
PT-DIES-SOIL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2023
Supervised By :Ankita Jodhani 05/04/2023

Integration File: autoint1.e
Quant Time: May 04 01:23:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

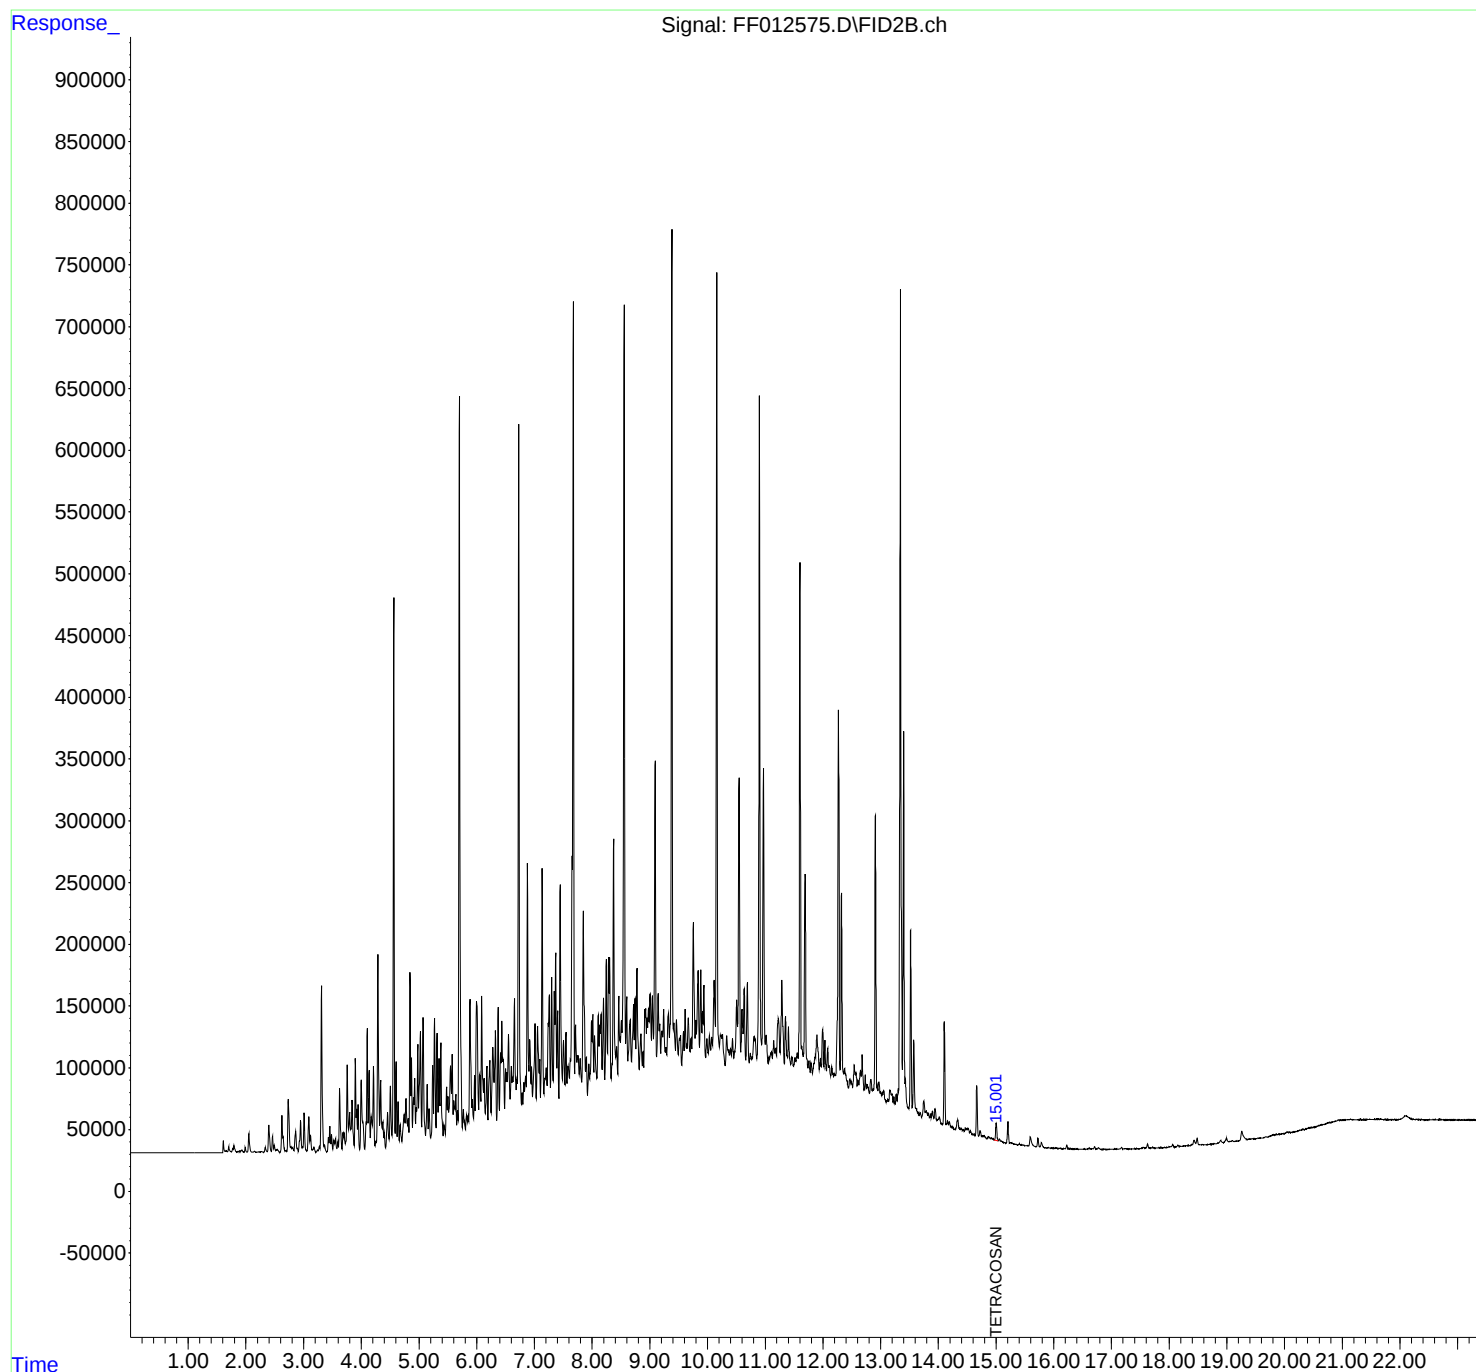

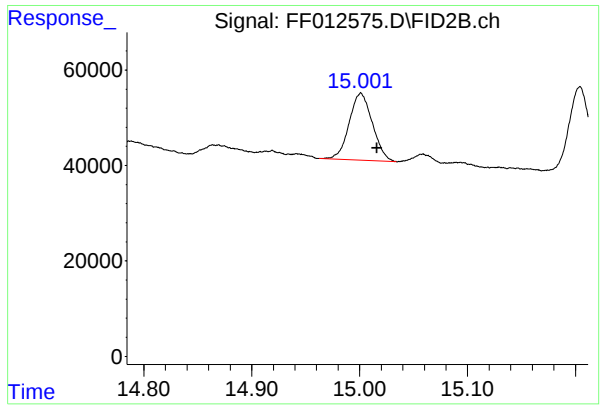

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.001 min
Delta R.T.: -0.015 min
Response: 211326
Conc: 1.76 ug/ml

Instrument :

FID_F

ClientSampleId :

PT-DIES-SOIL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2023

Supervised By :Ankita Jodhani 05/04/2023