

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF050422AL\  
 Data File : FF010516.D  
 Signal(s) : FID2B.ch  
 Acq On : 04 May 2022 12:48  
 Operator : AJ\MA  
 Sample : N2637-09DL 5X  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: May 04 15:42:32 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH -FF050322.M  
 Quant Title : GC Extractables  
 QLast Update : Tue May 03 13:18:42 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 12.287 | 1127735    | 10.370 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 20.74%       |
|                                |        |            |              |
| Target Compounds               |        |            |              |
| 4) T n-Dodecane (C12)          | 5.706  | 42969      | 0.358 ug/ml  |
| 10) T n-Eicosane (C20)         | 11.843 | 26995      | 0.215 ug/ml  |
| 11) T n-Heneicosane (C21)      | 12.454 | 28979      | 0.230 ug/ml  |
| 13) T n-Docosane (C22)         | 13.039 | 95125      | 0.760 ug/ml  |
| 14) T n-Tetracosane (C24)      | 14.142 | 245881     | 1.997 ug/ml  |
| 15) T n-Hexacosane (C26)       | 15.161 | 308091     | 2.589 ug/ml  |
| 16) T n-Octacosane (C28)       | 16.110 | 449776     | 3.941 ug/ml  |
| 17) T n-Tricontane (C30)       | 16.996 | 357932     | 3.282 ug/ml  |
| 18) T n-Dotriacontane (C32)    | 17.826 | 247240     | 2.413 ug/ml  |
| 19) T n-Tetratriacontane (C34) | 18.609 | 184810     | 2.003 ug/ml  |
| 20) T n-Hexatriacontane (C36)  | 19.344 | 64910      | 0.778 ug/ml  |
| 21) T n-Octatriacontane (C38)  | 20.062 | 34650      | 0.465 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF050422AL\  
Data File : FF010516.D  
Signal(s) : FID2B.ch  
Acq On : 04 May 2022 12:48  
Operator : AJ\MA  
Sample : N2637-09DL 5X  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 04 15:42:32 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\Aliphatic EPH -FF050322.M  
Quant Title : GC Extractables  
QLast Update : Tue May 03 13:18:42 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

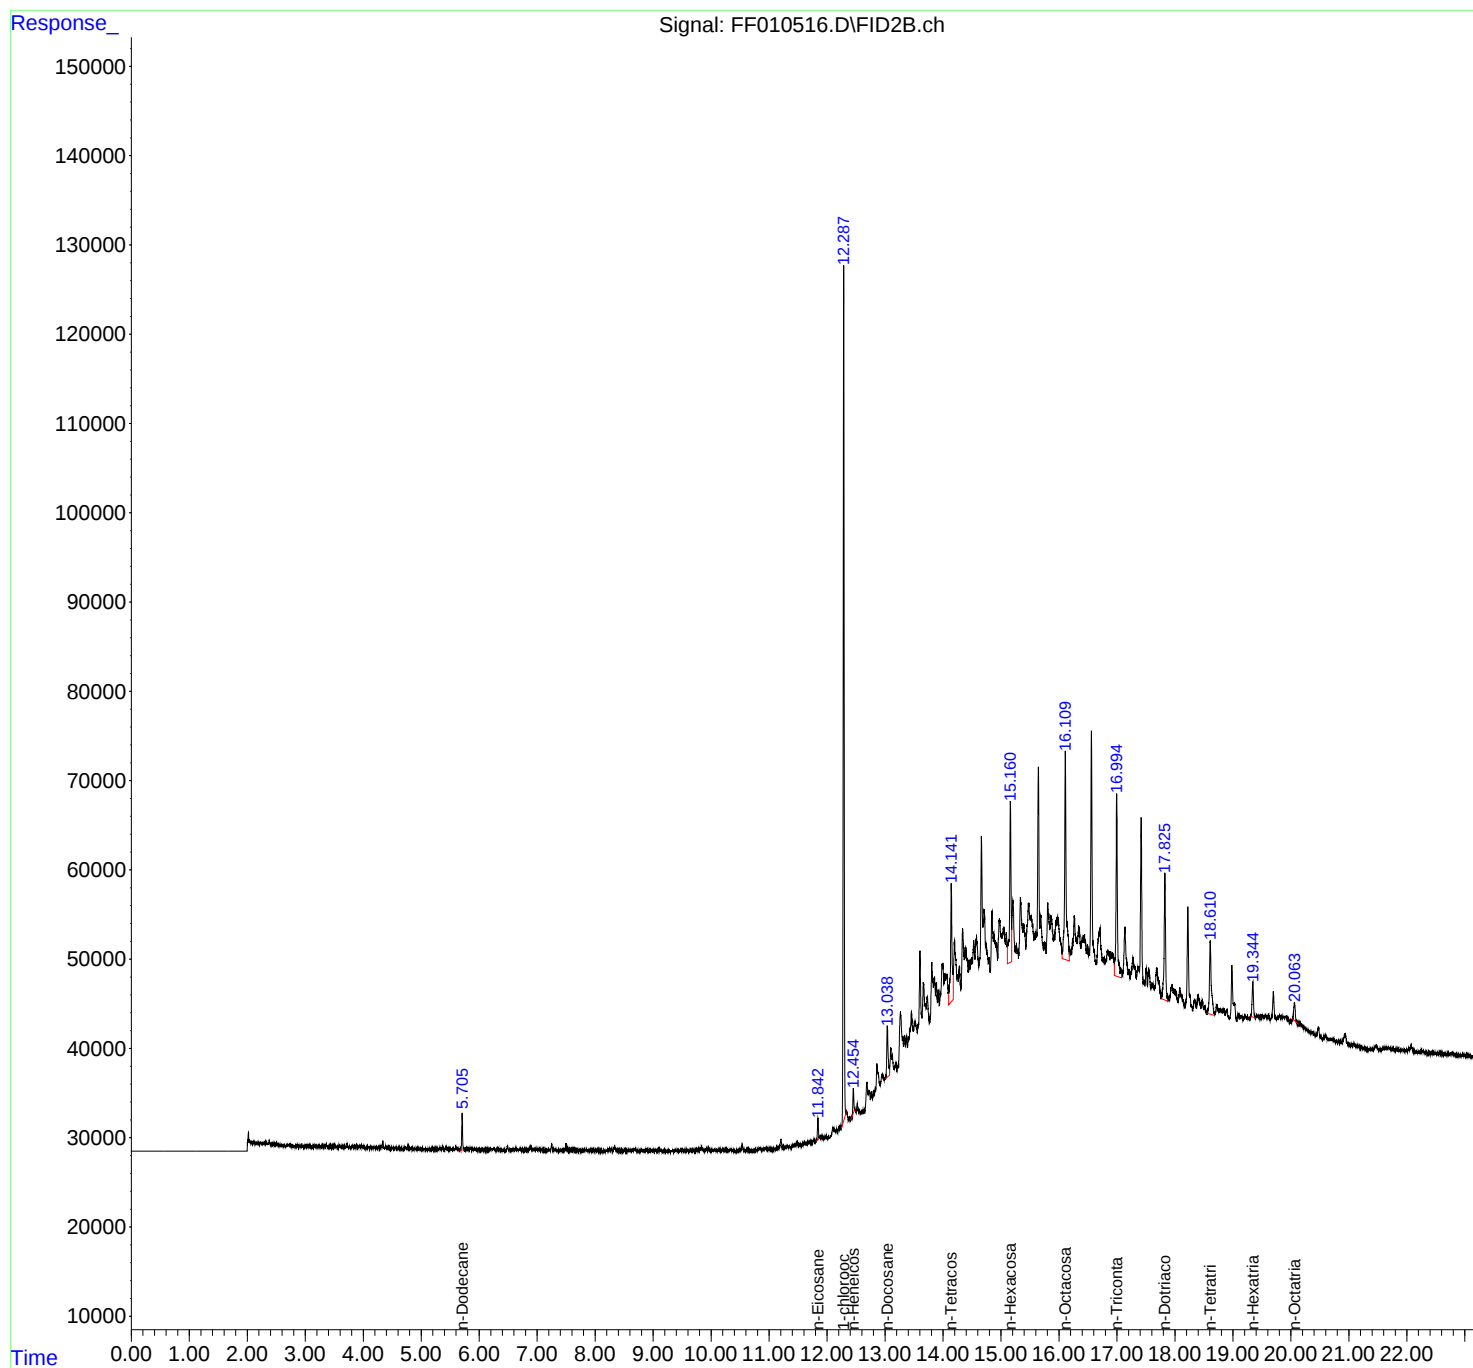


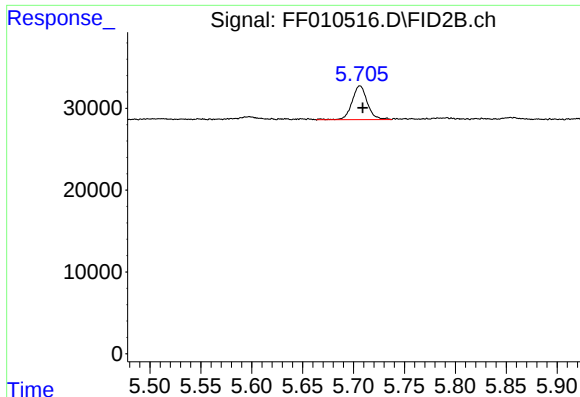

#4 n-Dodecane (C12)


R.T.: 5.706 min  
Delta R.T.: -0.003 min  
Response: 42969  
Conc: 0.36 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

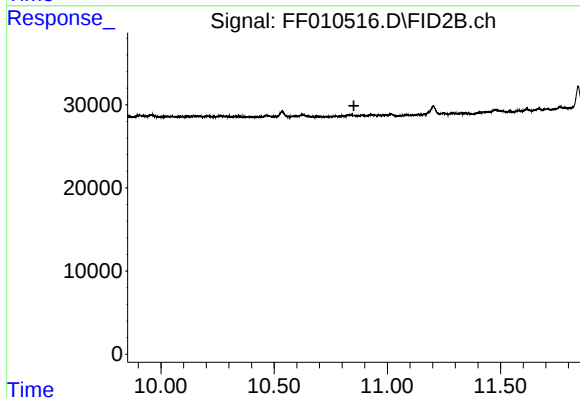


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 10.852 min  
Response: 0  
Conc: N.D.

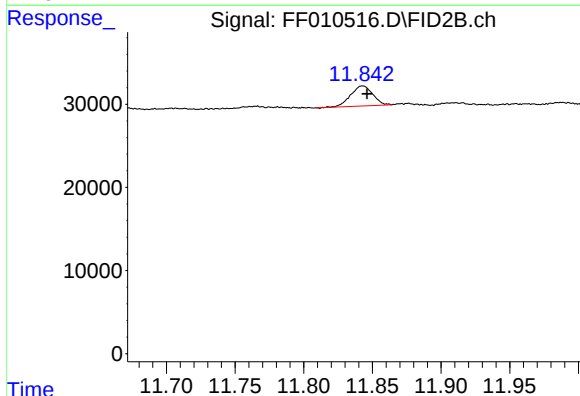


#10 n-Eicosane (C20)

R.T.: 11.843 min  
Delta R.T.: -0.003 min  
Response: 26995  
Conc: 0.22 ug/ml

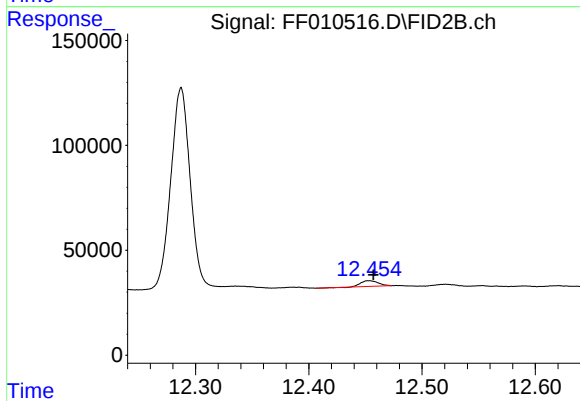

#11 n-Heneicosane (C21)


R.T.: 12.454 min  
Delta R.T.: -0.003 min  
Response: 28979  
Conc: 0.23 ug/ml

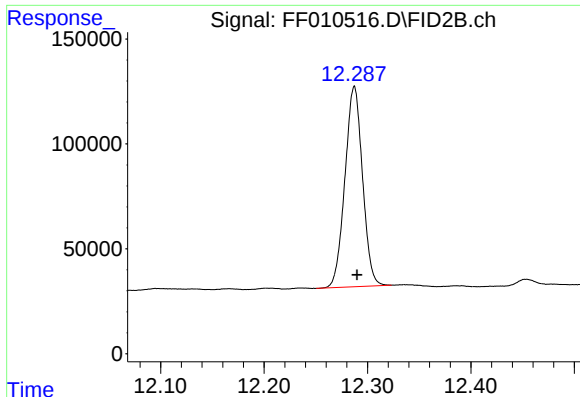

#12 1-chlorooctadecane (SURR)


R.T.: 12.287 min  
Delta R.T.: -0.003 min  
Response: 1127735  
Conc: 10.37 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

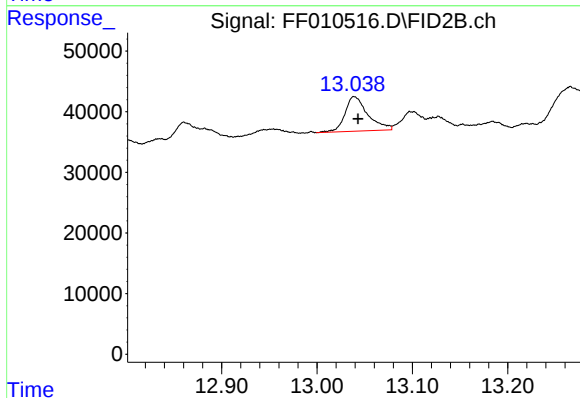


#13 n-Docosane (C22)

R.T.: 13.039 min  
Delta R.T.: -0.005 min  
Response: 95125  
Conc: 0.76 ug/ml

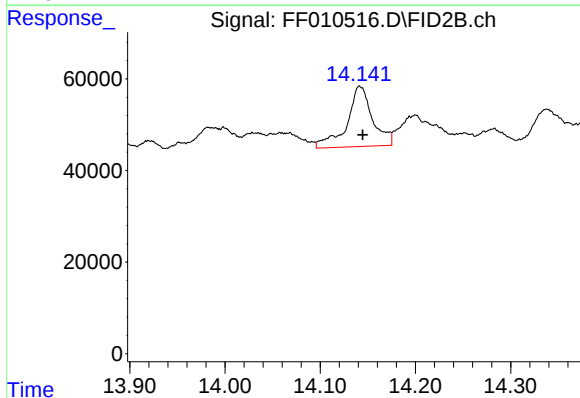


#14 n-Tetracosane (C24)

R.T.: 14.142 min  
Delta R.T.: -0.003 min  
Response: 245881  
Conc: 2.00 ug/ml

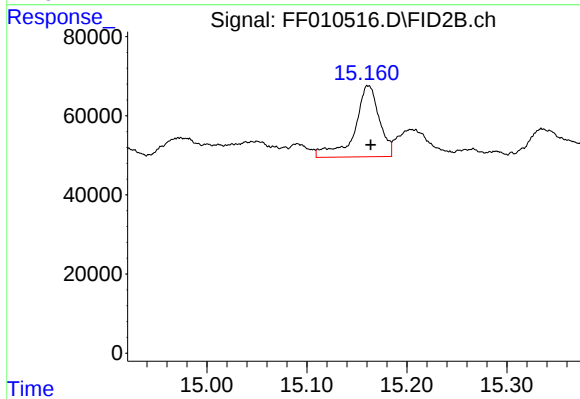

#15 n-Hexacosane (C26)


R.T.: 15.161 min  
Delta R.T.: -0.002 min  
Response: 308091  
Conc: 2.59 ug/ml

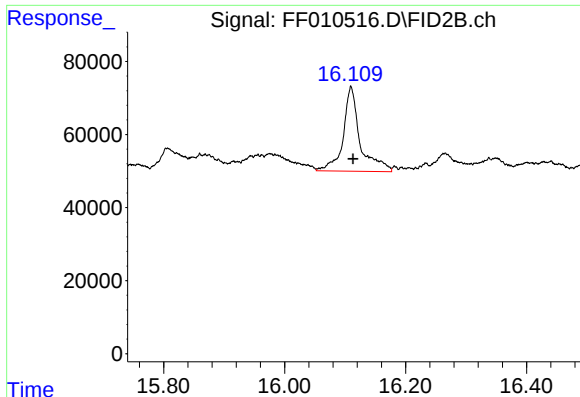

#16 n-Octacosane (C28)


R.T.: 16.110 min  
Delta R.T.: -0.003 min  
Response: 449776  
Conc: 3.94 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

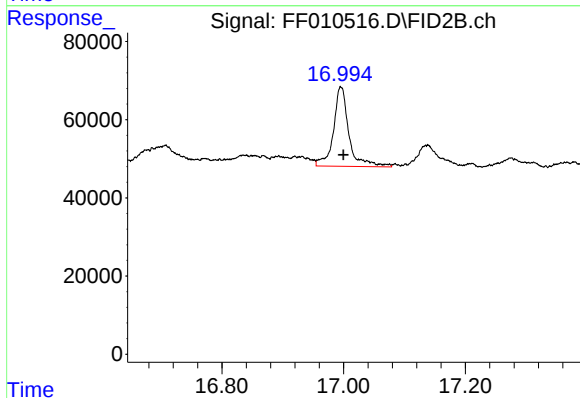


#17 n-Tricontane (C30)

R.T.: 16.996 min  
Delta R.T.: -0.004 min  
Response: 357932  
Conc: 3.28 ug/ml

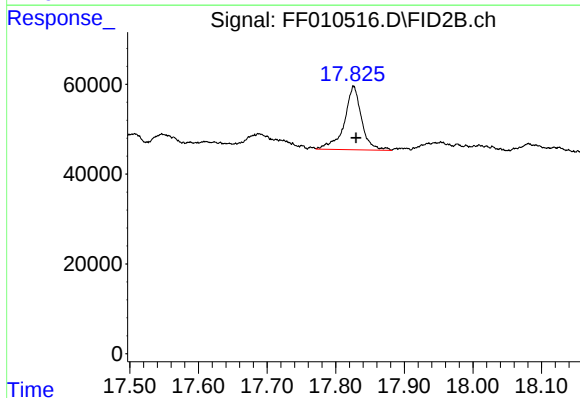


#18 n-Dotriacontane (C32)

R.T.: 17.826 min  
Delta R.T.: -0.003 min  
Response: 247240  
Conc: 2.41 ug/ml

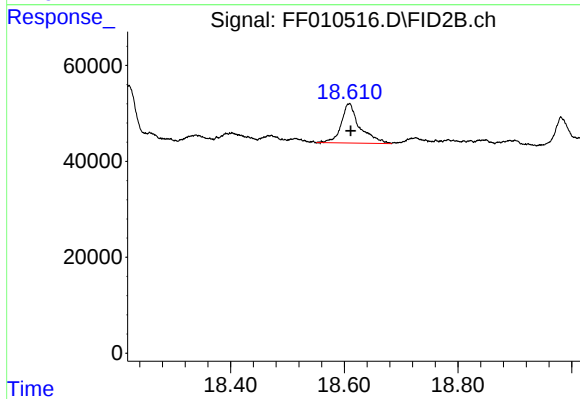

#19 n-Tetratriacontane (C34)


R.T.: 18.609 min  
Delta R.T.: -0.002 min  
Response: 184810  
Conc: 2.00 ug/ml

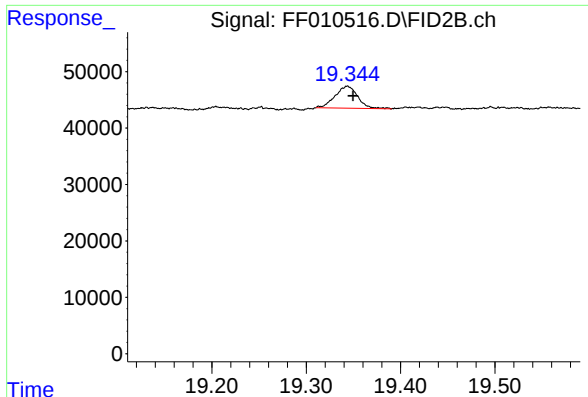

#20 n-Hexatriacontane (C36)

R.T.: 19.344 min  
Delta R.T.: -0.006 min  
Response: 64910  
Conc: 0.78 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

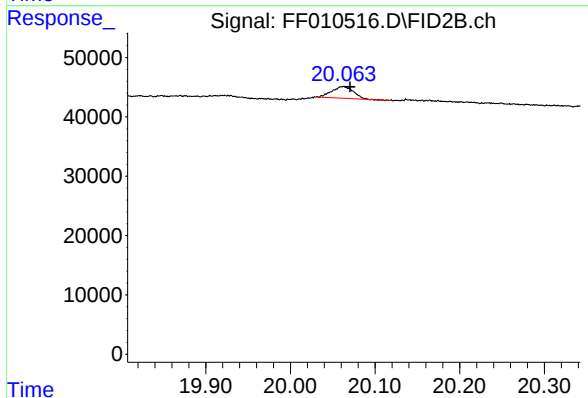

#21 n-Octatriacontane (C38)

R.T.: 20.062 min  
Delta R.T.: -0.008 min  
Response: 34650  
Conc: 0.47 ug/ml