

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050422AL\
 Data File : FF010523.D
 Signal(s) : FID2B.ch
 Acq On : 04 May 2022 17:44
 Operator : AJ\MA
 Sample : N2665-02
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 05 01:22:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
 Quant Title : GC Extractables
 QLast Update : Tue May 03 13:18:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.852	5463220	39.683 ug/ml
Spiked Amount 50.000		Recovery =	79.37%
12) S 1-chlorooctadecane (S...	12.289	4453470	40.950 ug/ml
Spiked Amount 50.000		Recovery =	81.90%
Target Compounds			
6) T n-Tetradecane (C14)	7.430f	14841	0.123 ug/ml
14) T n-Tetracosane (C24)	14.185	22666	0.184 ug/ml
18) T n-Dotriacontane (C32)	17.826	38520	0.376 ug/ml
20) T n-Hexatriacontane (C36)	19.346	18970	0.227 ug/ml
21) T n-Octatriacontane (C38)	20.065	37192	0.500 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050422AL\
Data File : FF010523.D
Signal(s) : FID2B.ch
Acq On : 04 May 2022 17:44
Operator : AJ\MA
Sample : N2665-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 05 01:22:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH -FF050322.M
Quant Title : GC Extractables
QLast Update : Tue May 03 13:18:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

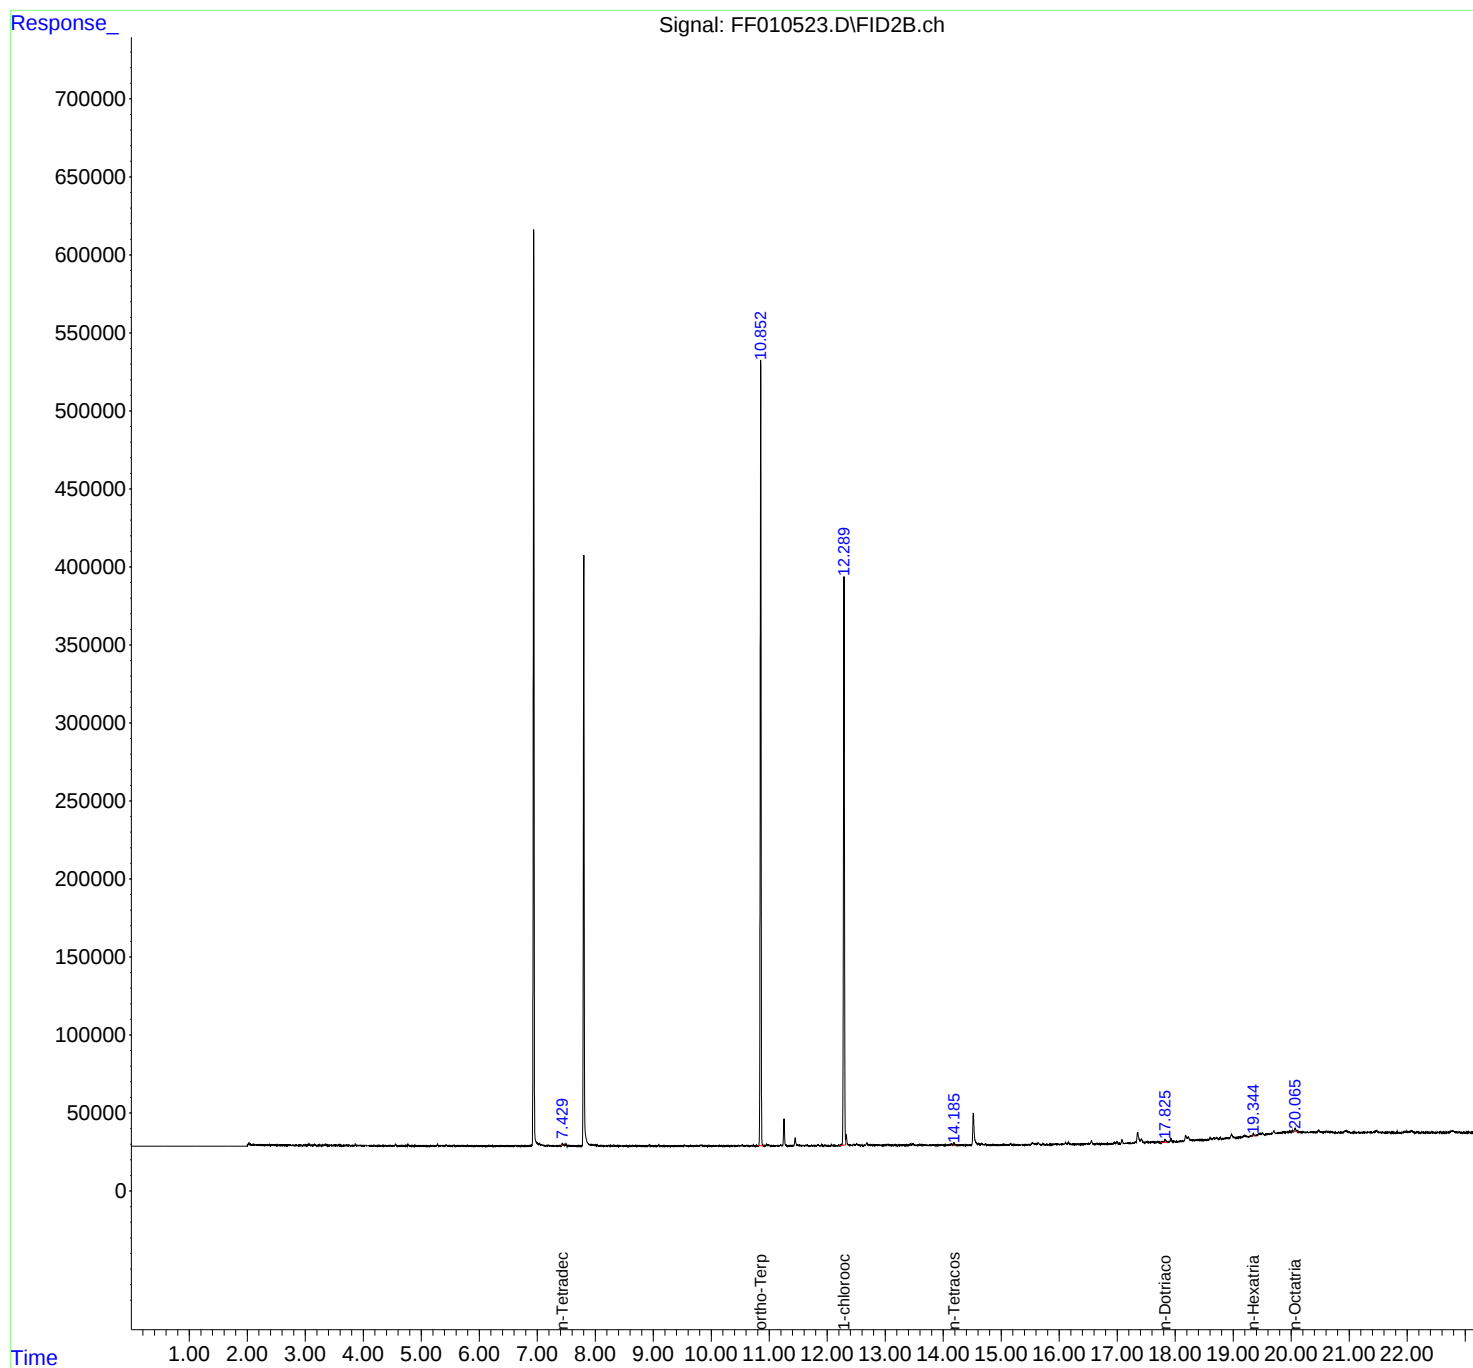


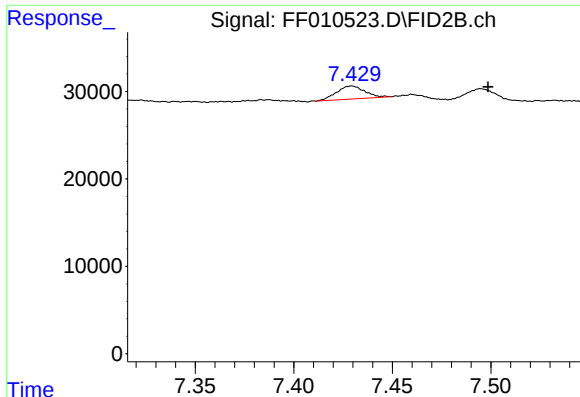

#6 n-Tetradecane (C14)


R.T.: 7.430 min
Delta R.T.: -0.069 min
Response: 14841
Conc: 0.12 ug/ml

Instrument :
FID_F
ClientSampleId :

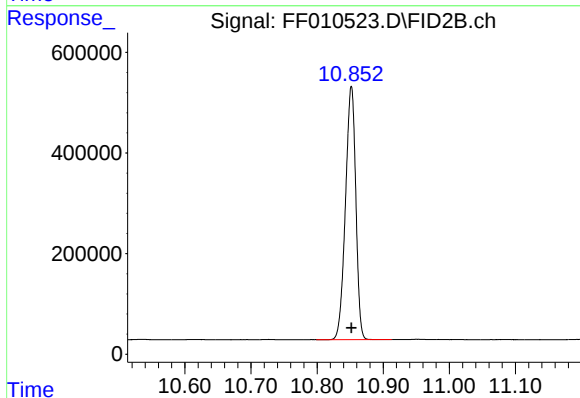


#9 ortho-Terphenyl (SURR)

R.T.: 10.852 min
Delta R.T.: 0.000 min
Response: 5463220
Conc: 39.68 ug/ml

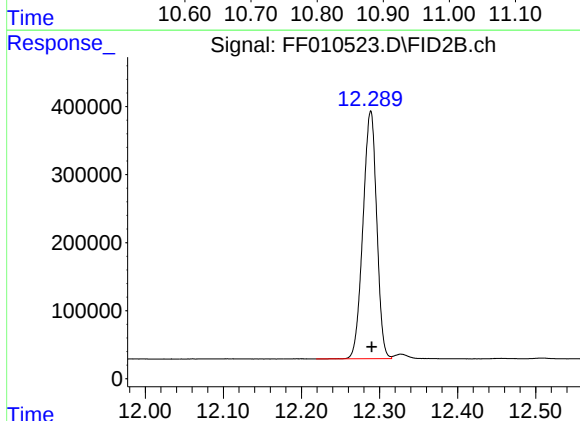


#12 1-chlorooctadecane (SURR)

R.T.: 12.289 min
Delta R.T.: -0.001 min
Response: 4453470
Conc: 40.95 ug/ml

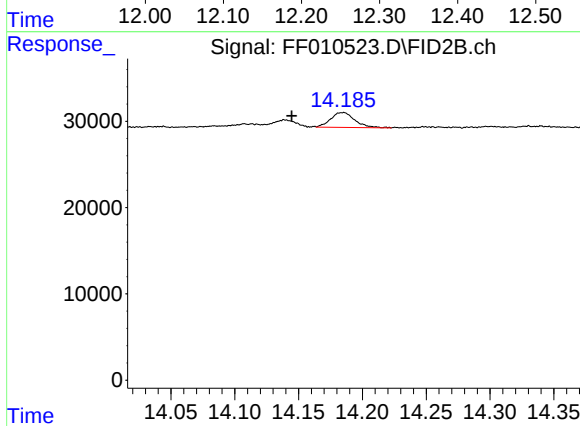

#14 n-Tetracosane (C24)


R.T.: 14.185 min
Delta R.T.: 0.040 min
Response: 22666
Conc: 0.18 ug/ml

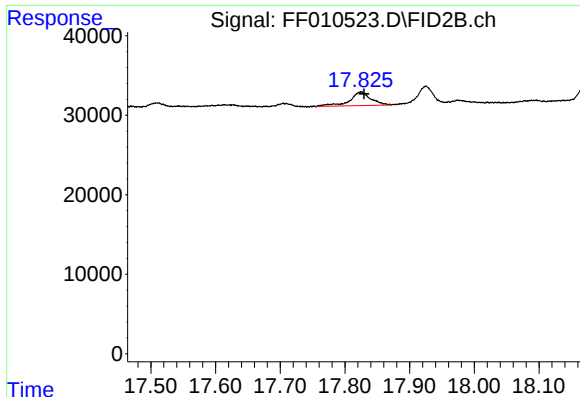

#18 n-Dotriacontane (C32)


R.T.: 17.826 min
Delta R.T.: -0.004 min
Response: 38520
Conc: 0.38 ug/ml

Instrument :
FID_F
ClientSampleId :

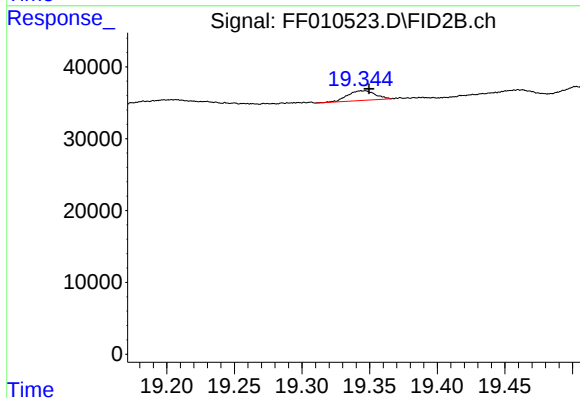

#20 n-Hexatriacontane (C36)

R.T.: 19.346 min
Delta R.T.: -0.004 min
Response: 18970
Conc: 0.23 ug/ml

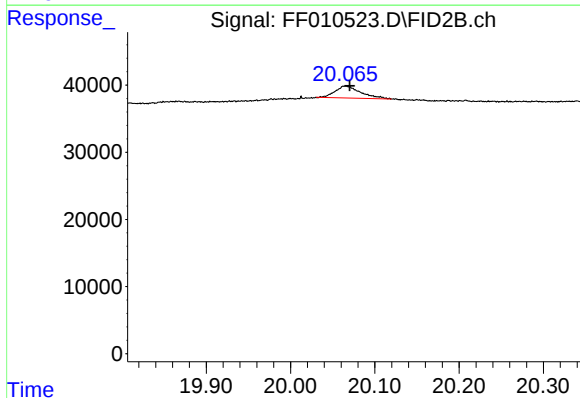

#21 n-Octatriacontane (C38)

R.T.: 20.065 min
Delta R.T.: -0.005 min
Response: 37192
Conc: 0.50 ug/ml