

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
 Data File : FF010549.D
 Signal(s) : FID2B.ch
 Acq On : 05 May 2022 11:49
 Operator : AJ\MA
 Sample : N2674-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 06 01:56:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.609	636521	5.190 ug/ml
Target Compounds			
3) N-DODECANE	6.366	140085	1.034 ug/ml
4) N-TETRADECANE	8.160	215495	1.580 ug/ml
5) N-HEXADECANE	9.758	213812	1.546 ug/ml
6) N-OCTADECANE	11.195	367803	2.561 ug/ml
7) N-EICOSANE	12.511	372866	2.662 ug/ml
8) N-DOCOSANE	13.723	508213	3.659 ug/ml
10) N-TETRACOSANE	14.757f	1400322	10.135 ug/ml
11) N-HEXACOSANE	15.827	278948	2.061 ug/ml
12) N-OCTACOSANE	16.779	71166	0.541 ug/ml
13) N-TRIACONTANE	17.674	2622668	20.634 ug/ml
14) N-DOTRIACONTANE	18.488	2308596	19.247 ug/ml
15) N-TETRATRIACONTANE	19.263	354363	3.339 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
Data File : FF010549.D
Signal(s) : FID2B.ch
Acq On : 05 May 2022 11:49
Operator : AJ\MA
Sample : N2674-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 01:56:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

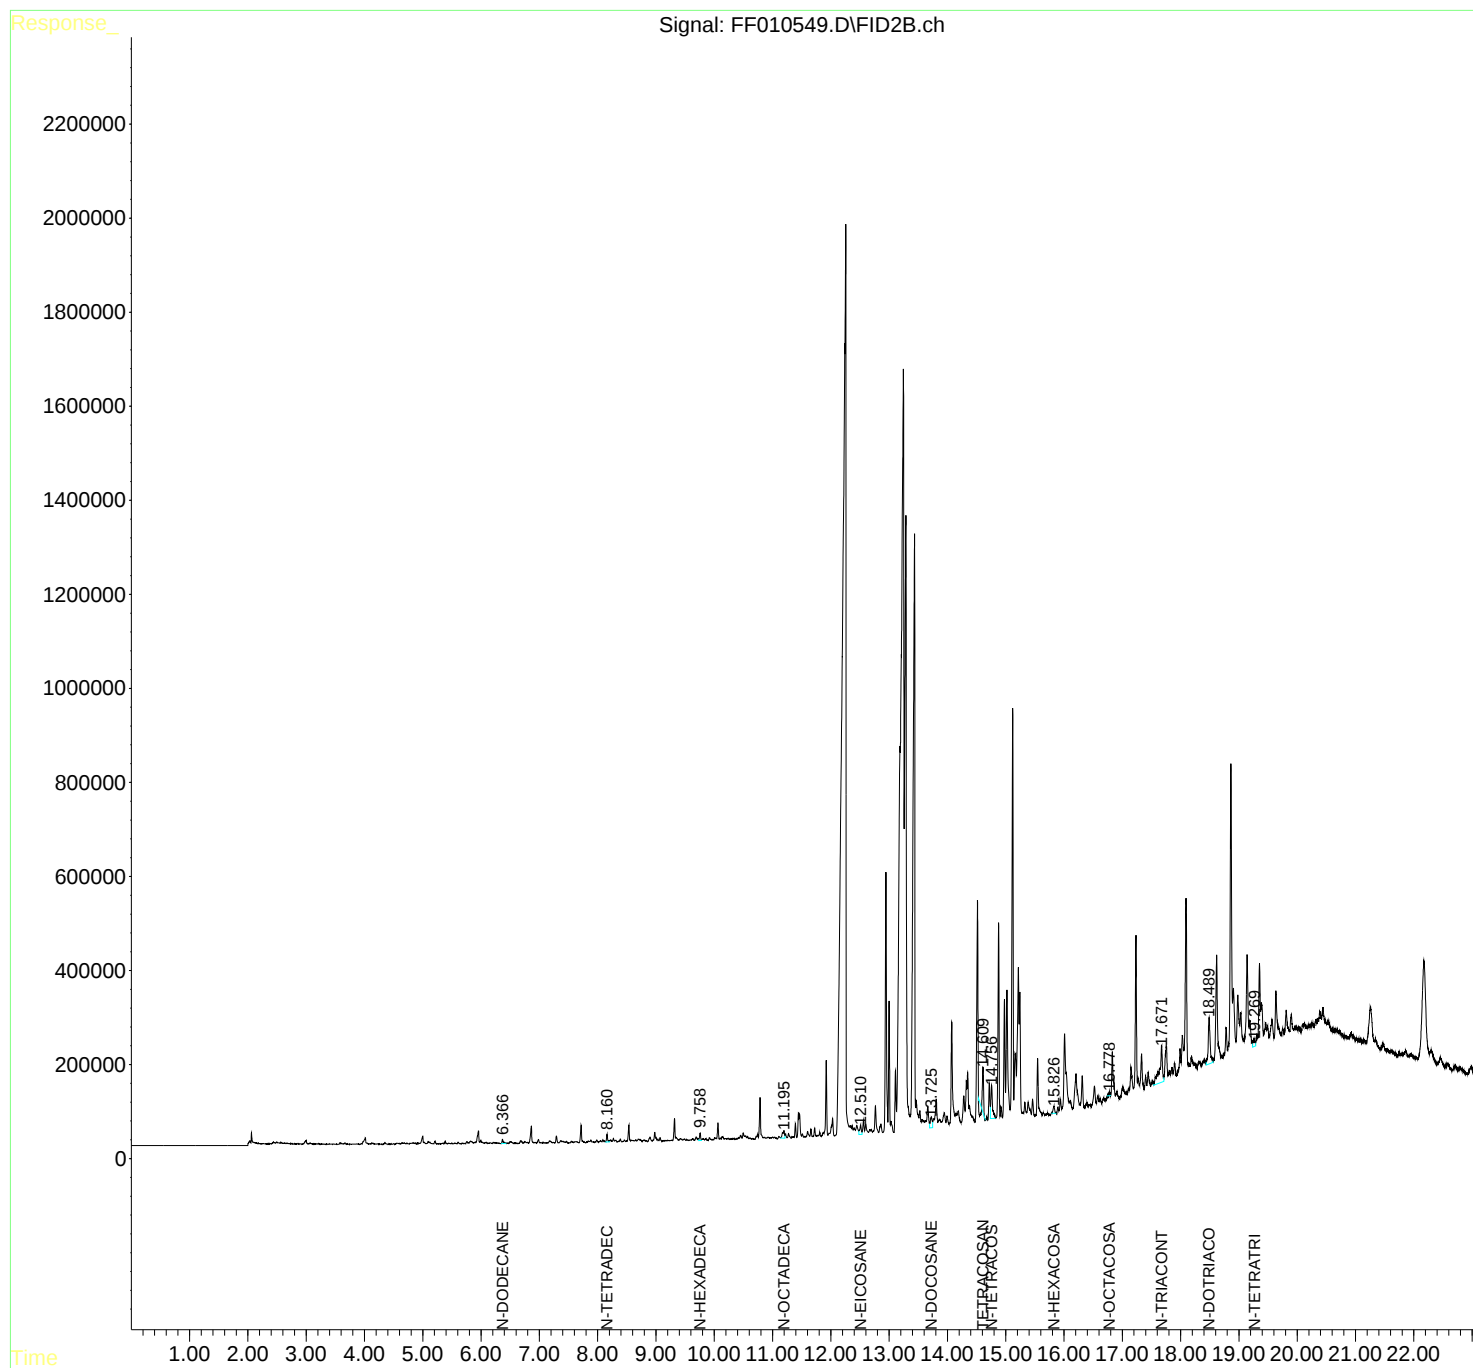


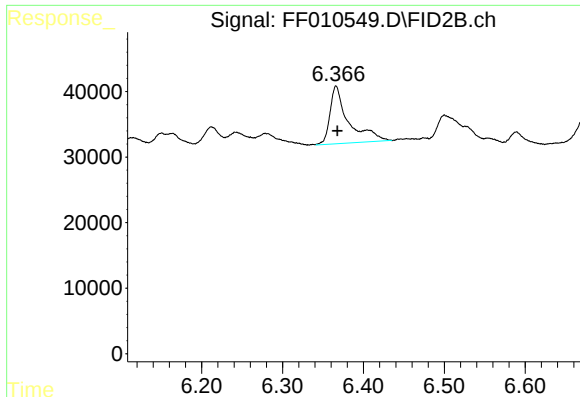

#3 N-DODECANE


R.T.: 6.366 min
Delta R.T.: -0.002 min
Response: 140085
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

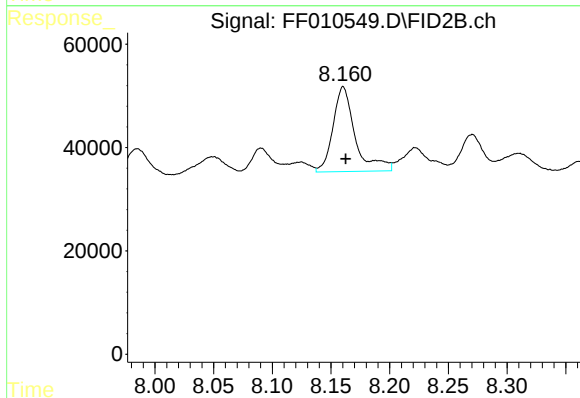


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: -0.002 min
Response: 215495
Conc: 1.58 ug/ml

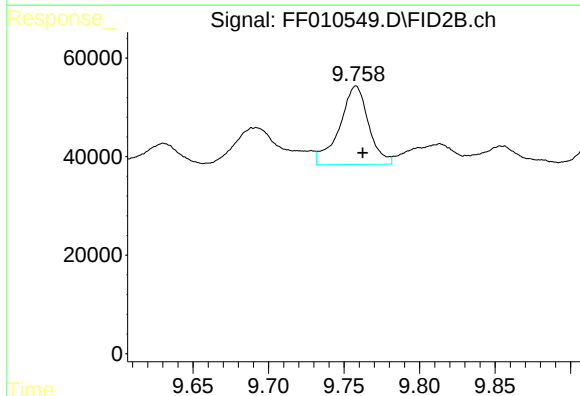


#5 N-HEXADECANE

R.T.: 9.758 min
Delta R.T.: -0.005 min
Response: 213812
Conc: 1.55 ug/ml

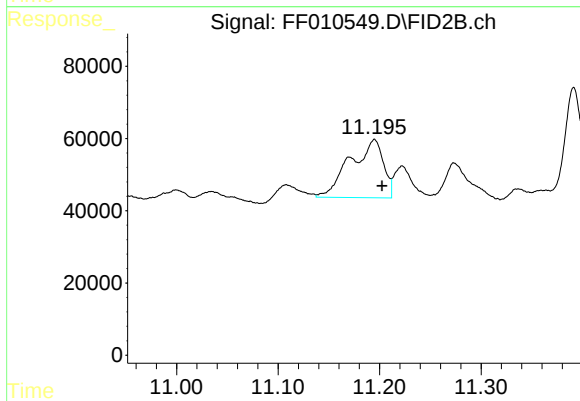

#6 N-OCTADECANE


R.T.: 11.195 min
Delta R.T.: -0.008 min
Response: 367803
Conc: 2.56 ug/ml

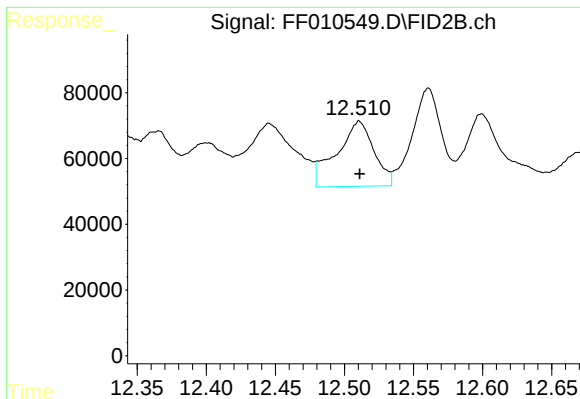

#7 N-EICOSANE


R.T.: 12.511 min
Delta R.T.: 0.000 min
Response: 372866
Conc: 2.66 ug/ml

Instrument :
FID_F
ClientSampleId :

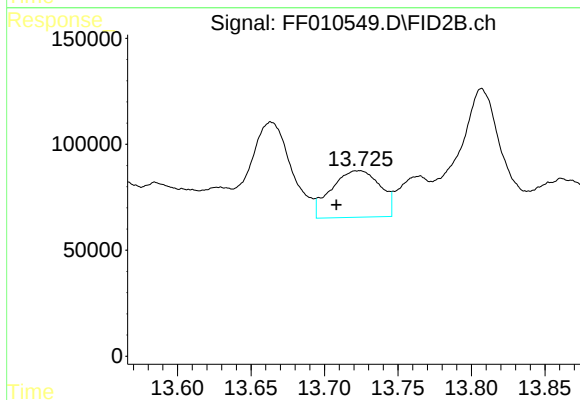


#8 N-DOCOSANE

R.T.: 13.723 min
Delta R.T.: 0.015 min
Response: 508213
Conc: 3.66 ug/ml

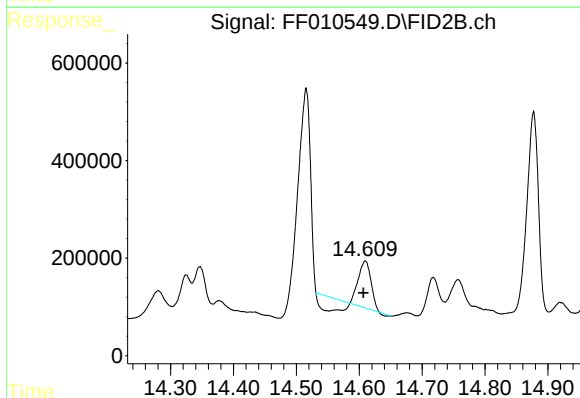


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.609 min
Delta R.T.: 0.003 min
Response: 636521
Conc: 5.19 ug/ml

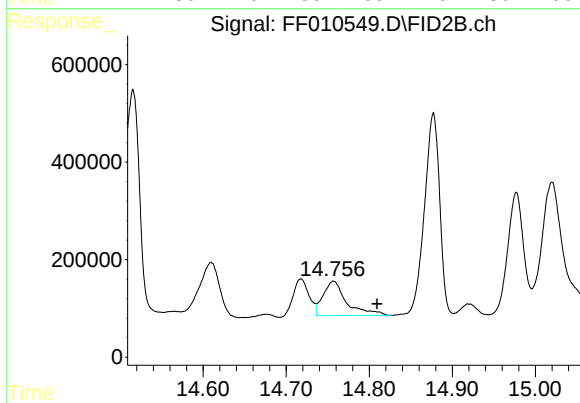

#10 N-TETRACOSANE


R.T.: 14.757 min
Delta R.T.: -0.052 min
Response: 1400322
Conc: 10.14 ug/ml

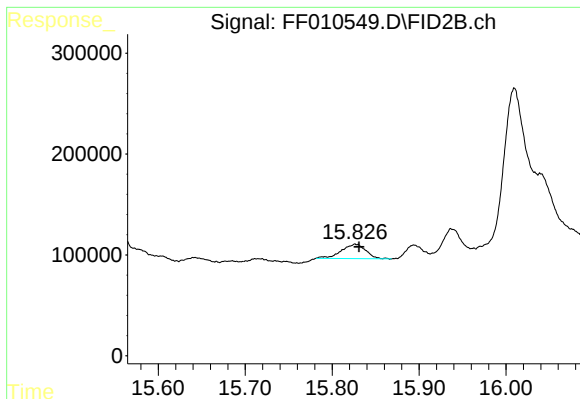

#11 N-HEXACOSANE


R.T.: 15.827 min
Delta R.T.: -0.004 min
Response: 278948
Conc: 2.06 ug/ml

Instrument :
FID_F
ClientSampleId :

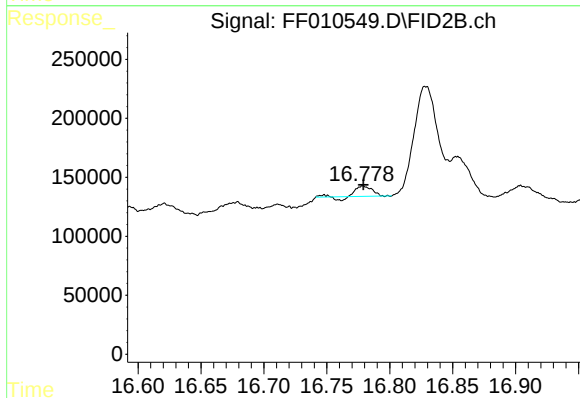


#12 N-OCTACOSANE

R.T.: 16.779 min
Delta R.T.: 0.000 min
Response: 71166
Conc: 0.54 ug/ml

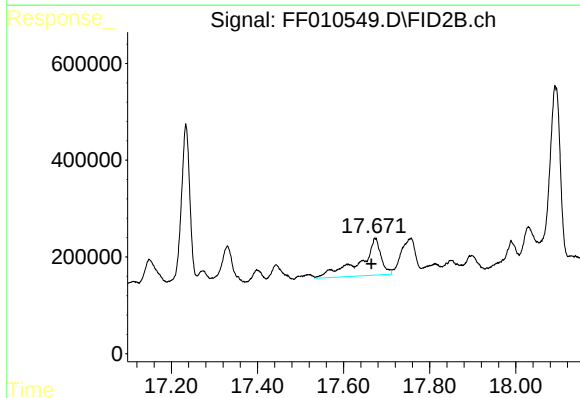


#13 N-TRIACONTANE

R.T.: 17.674 min
Delta R.T.: 0.009 min
Response: 2622668
Conc: 20.63 ug/ml

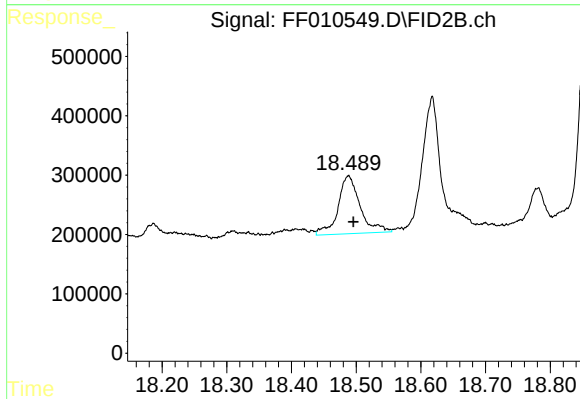

#14 N-DOTRIACONTANE

R.T.: 18.488 min
Delta R.T.: -0.008 min
Response: 2308596
Conc: 19.25 ug/ml

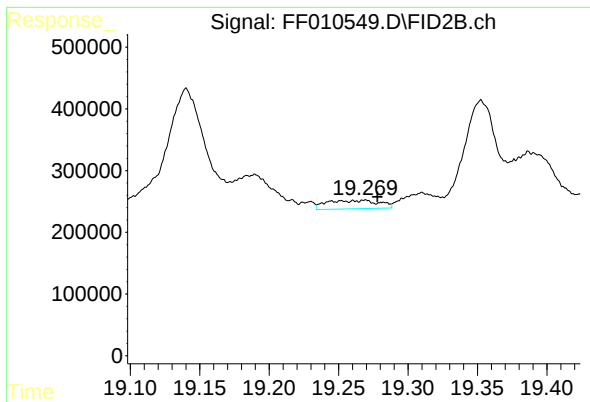

#15 N-TETRATRIACONTANE

R.T.: 19.263 min
Delta R.T.: -0.015 min
Response: 354363
Conc: 3.34 ug/ml

Instrument :

FID_F

ClientSampleId :