

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
 Data File : FF010550.D
 Signal(s) : FID2B.ch
 Acq On : 05 May 2022 12:18
 Operator : AJ\MA
 Sample : N2675-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 06 01:56:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	1335504	10.890 ug/ml
Target Compounds			
7) N-EICOSANE	12.565f	356595	2.546 ug/ml
8) N-DOCOSANE	13.645f	1022458	7.362 ug/ml
10) N-TETRACOSANE	14.780	323448	2.341 ug/ml
12) N-OCTACOSANE	16.782	121286	0.922 ug/ml
13) N-TRIACONTANE	17.668	416162	3.274 ug/ml
14) N-DOTRIACONTANE	18.491	310898	2.592 ug/ml
15) N-TETRATRIACONTANE	19.251	390127	3.676 ug/ml
17) N-OCTATRIACONTANE	20.757	478054	5.931 ug/ml
18) N-TETRACONTANE	21.628	2054177	26.097 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
Data File : FF010550.D
Signal(s) : FID2B.ch
Acq On : 05 May 2022 12:18
Operator : AJ\MA
Sample : N2675-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 01:56:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

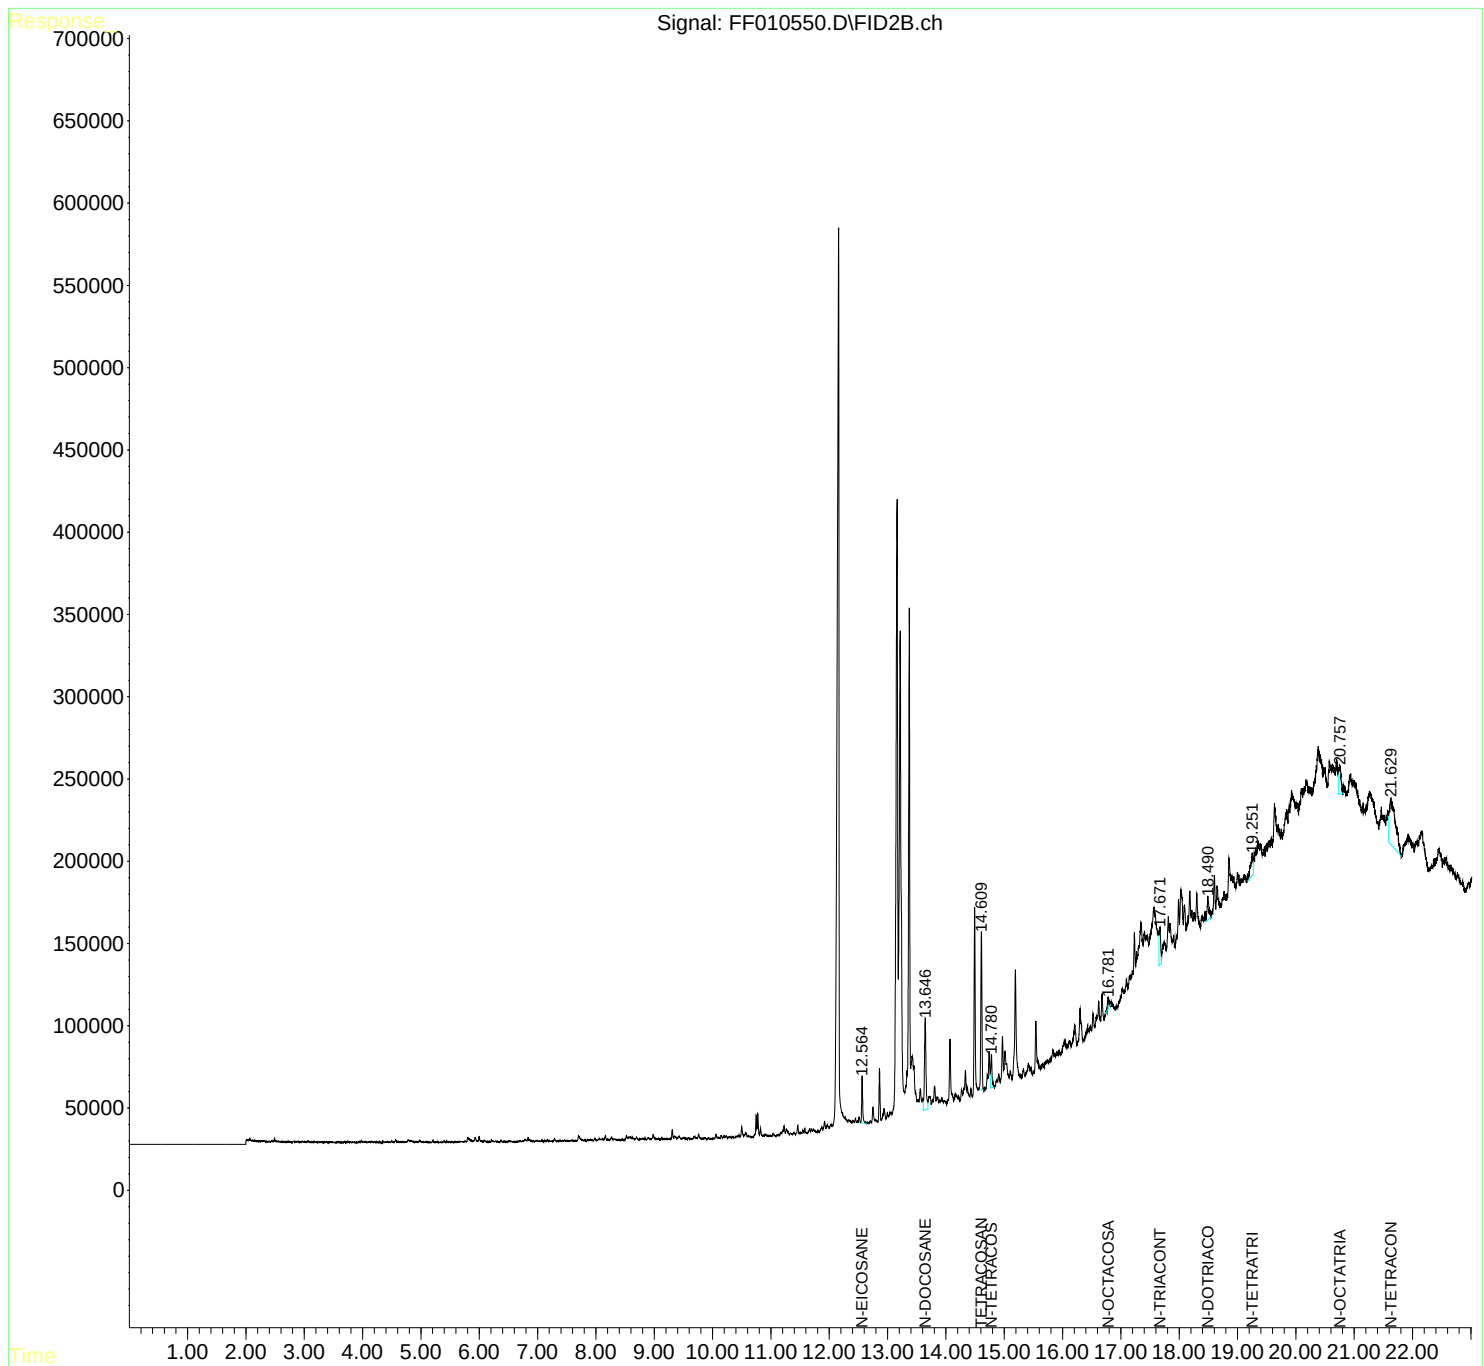


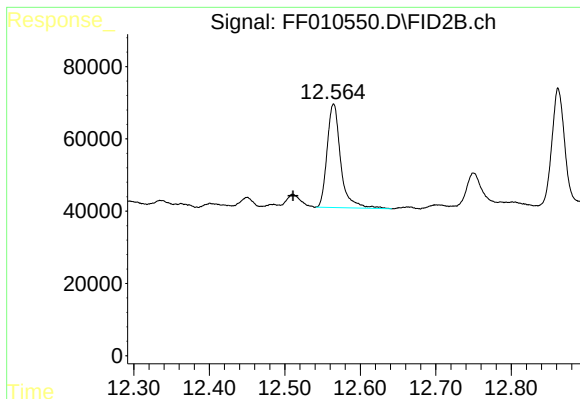

#7 N-EICOSANE


R.T.: 12.565 min
Delta R.T.: 0.054 min
Response: 356595
Conc: 2.55 ug/ml

Instrument :
FID_F
ClientSampleId :

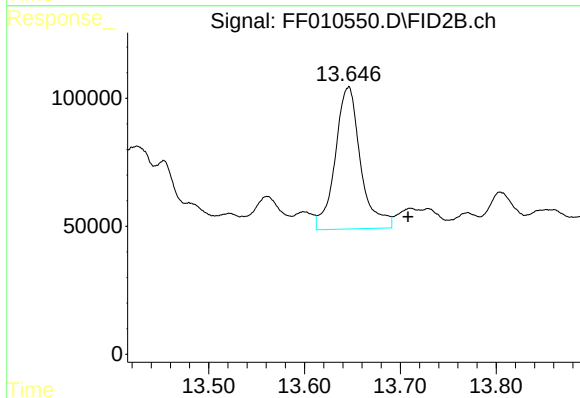


#8 N-DOCOSANE

R.T.: 13.645 min
Delta R.T.: -0.063 min
Response: 1022458
Conc: 7.36 ug/ml

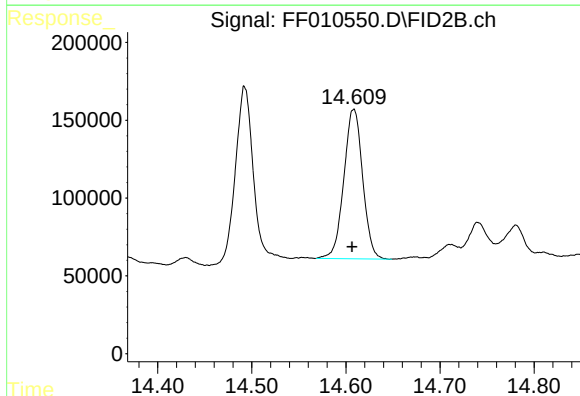


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: 0.002 min
Response: 1335504
Conc: 10.89 ug/ml

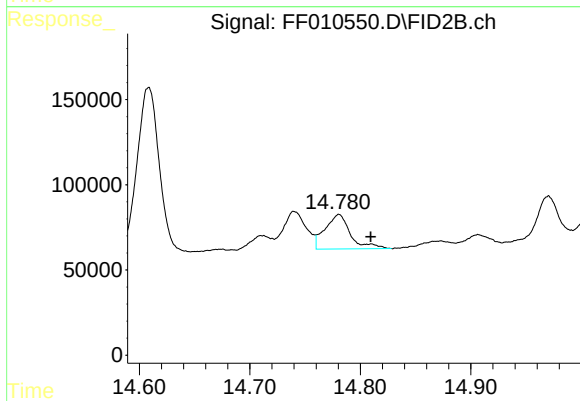

#10 N-TETRACOSANE


R.T.: 14.780 min
Delta R.T.: -0.029 min
Response: 323448
Conc: 2.34 ug/ml

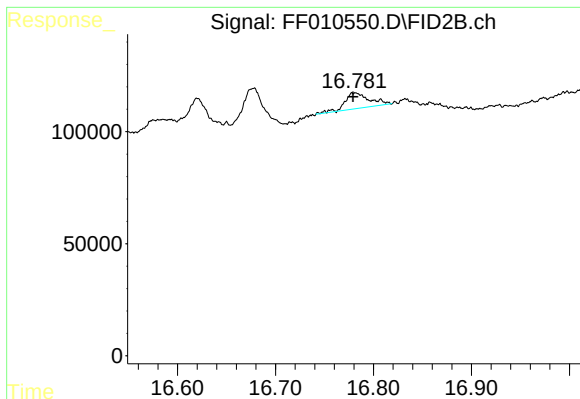

#12 N-OCTACOSANE


R.T.: 16.782 min
Delta R.T.: 0.003 min
Response: 121286
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

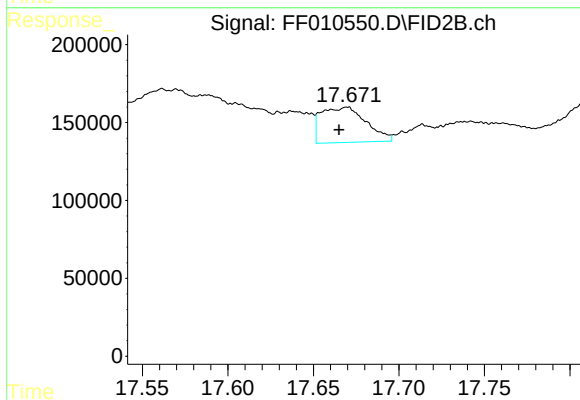


#13 N-TRIACONTANE

R.T.: 17.668 min
Delta R.T.: 0.003 min
Response: 416162
Conc: 3.27 ug/ml

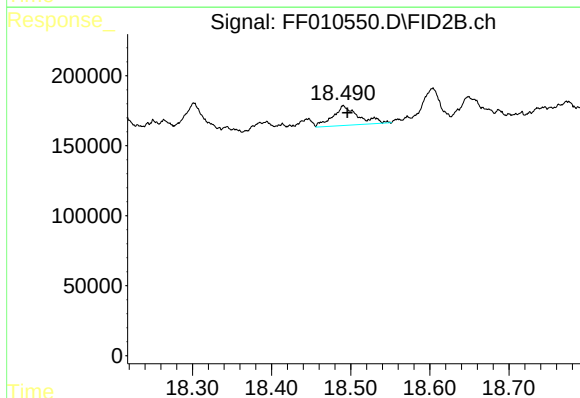


#14 N-DOTRIACONTANE

R.T.: 18.491 min
Delta R.T.: -0.005 min
Response: 310898
Conc: 2.59 ug/ml

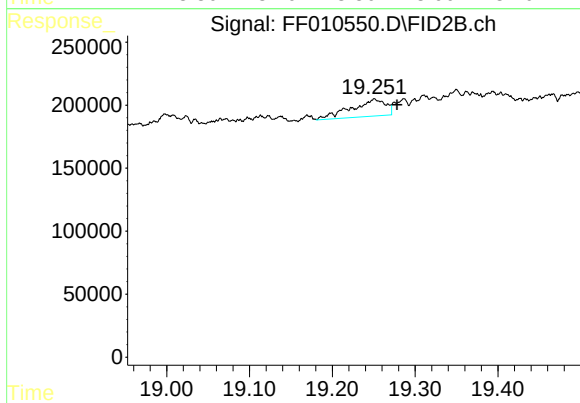

#15 N-TETRATRIACONTANE


R.T.: 19.251 min
Delta R.T.: -0.027 min
Response: 390127
Conc: 3.68 ug/ml

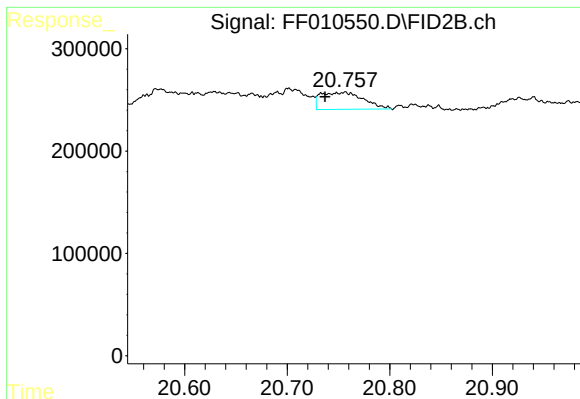

#17 N-OCTATRIACONTANE

R.T.: 20.757 min
Delta R.T.: 0.020 min
Response: 478054
Conc: 5.93 ug/ml

Instrument :
FID_F
ClientSampleId :

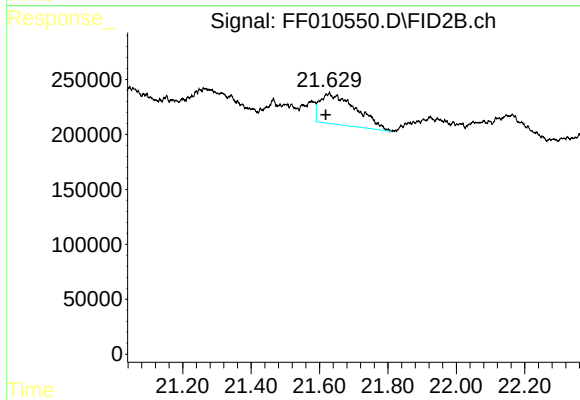

#18 N-TETRACONTANE

R.T.: 21.628 min
Delta R.T.: 0.011 min
Response: 2054177
Conc: 26.10 ug/ml