

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
Data File : FF010557.D
Signal(s) : FID2B.ch
Acq On : 05 May 2022 15:48
Operator : AJ\MA
Sample : N2674-01 50X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 01:57:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10)	N-TETRACOSANE	14.871f	116921	0.846 ug/ml
13)	N-TRIACONTANE	17.669	68869	0.542 ug/ml
14)	N-DOTRIACONTANE	18.495	88001	0.734 ug/ml
15)	N-TETRATRIACONTANE	19.340f	119636	1.127 ug/ml
17)	N-OCTATRIACONTANE	20.695	253075	3.140 ug/ml
18)	N-TETRACONTANE	21.652	443218	5.631 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050522\
Data File : FF010557.D
Signal(s) : FID2B.ch
Acq On : 05 May 2022 15:48
Operator : AJ\MA
Sample : N2674-01 50X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 01:57:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

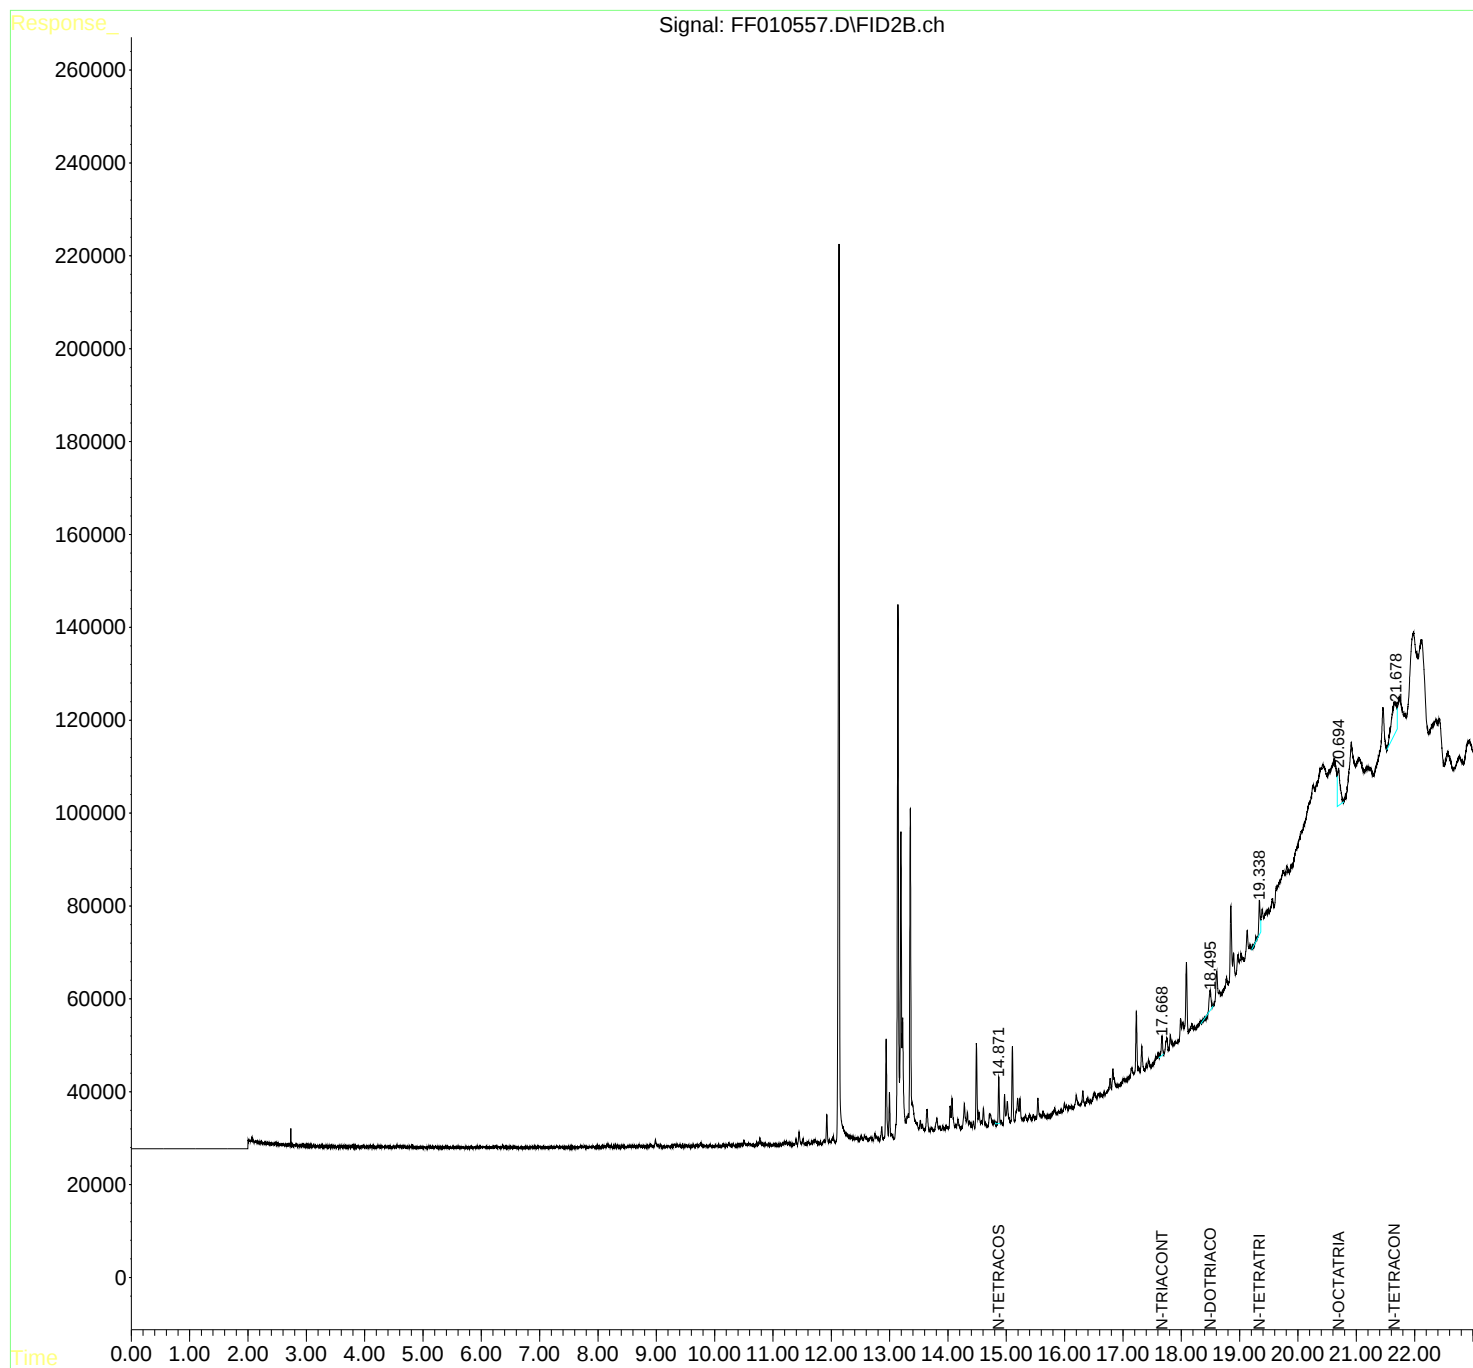


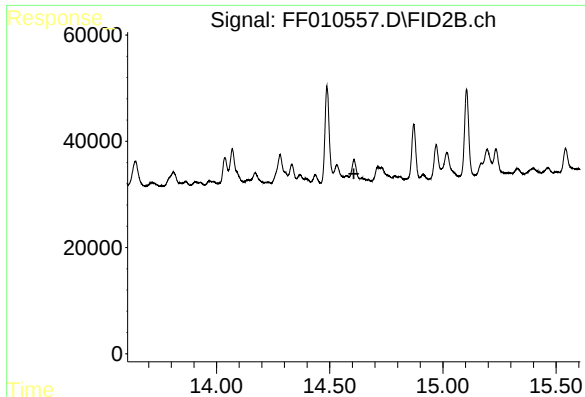

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.607 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

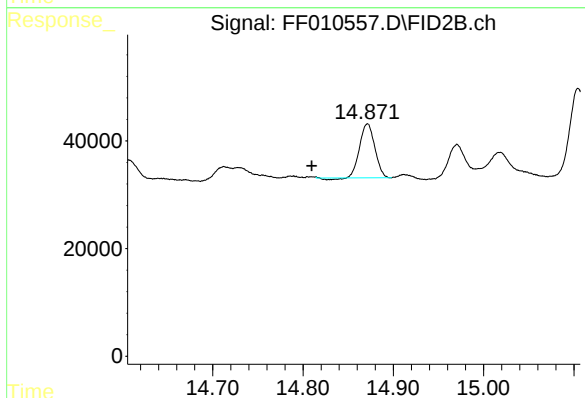


#10 N-TETRACOSANE

R.T.: 14.871 min
Delta R.T.: 0.062 min
Response: 116921
Conc: 0.85 ug/ml

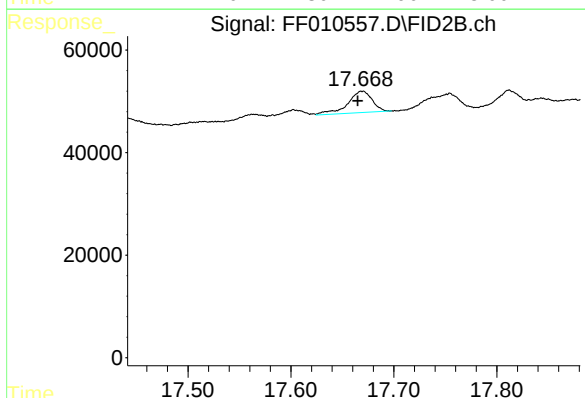


#13 N-TRIACONTANE

R.T.: 17.669 min
Delta R.T.: 0.004 min
Response: 68869
Conc: 0.54 ug/ml

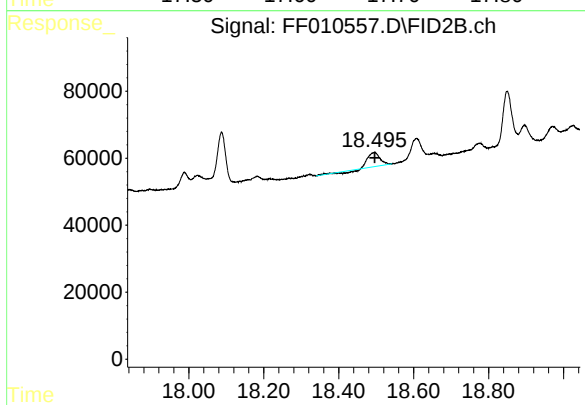

#14 N-DOTRIACONTANE


R.T.: 18.495 min
Delta R.T.: -0.001 min
Response: 88001
Conc: 0.73 ug/ml

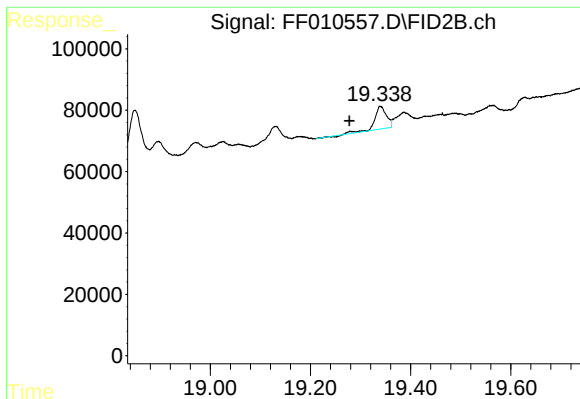

#15 N-TETRATRIACONTANE


R.T.: 19.340 min
Delta R.T.: 0.062 min
Response: 119636
Conc: 1.13 ug/ml

Instrument :
FID_F
ClientSampleId :

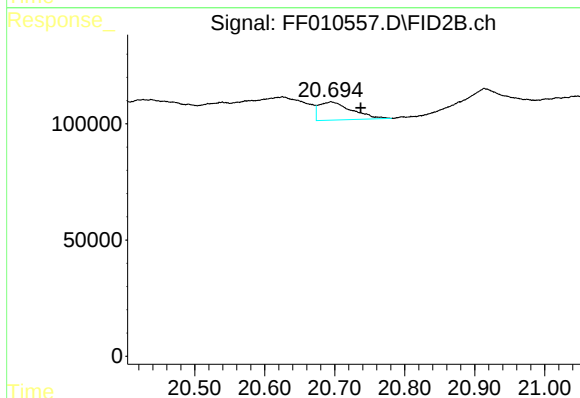

#17 N-OCTATRIACONTANE

R.T.: 20.695 min
Delta R.T.: -0.042 min
Response: 253075
Conc: 3.14 ug/ml

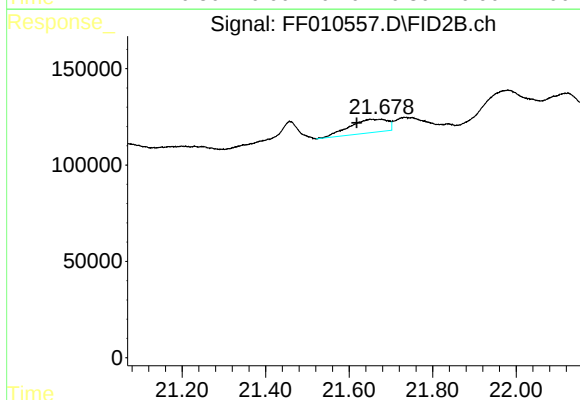

#18 N-TETRACONTANE

R.T.: 21.652 min
Delta R.T.: 0.034 min
Response: 443218
Conc: 5.63 ug/ml