

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050620\
 Data File : FF006841.D
 Signal(s) : FID2B.ch
 Acq On : 06 May 2020 07:58
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: May 07 00:41:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.353	2869988	20.129 ug/ml
12) N-OCTACOSANE	16.727	3125145	20.276 ug/ml
13) N-TRIACONTANE	17.611	94783	0.611 ug/ml
14) N-DOTRIACONTANE	18.439	137811	0.937 ug/ml
16) N-HEXATRIACONTANE	19.986	202062	1.678 ug/ml
18) N-TETRACONTANE	21.550	337798	3.225 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050620\
Data File : FF006841.D
Signal(s) : FID2B.ch
Acq On : 06 May 2020 07:58
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 07 00:41:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

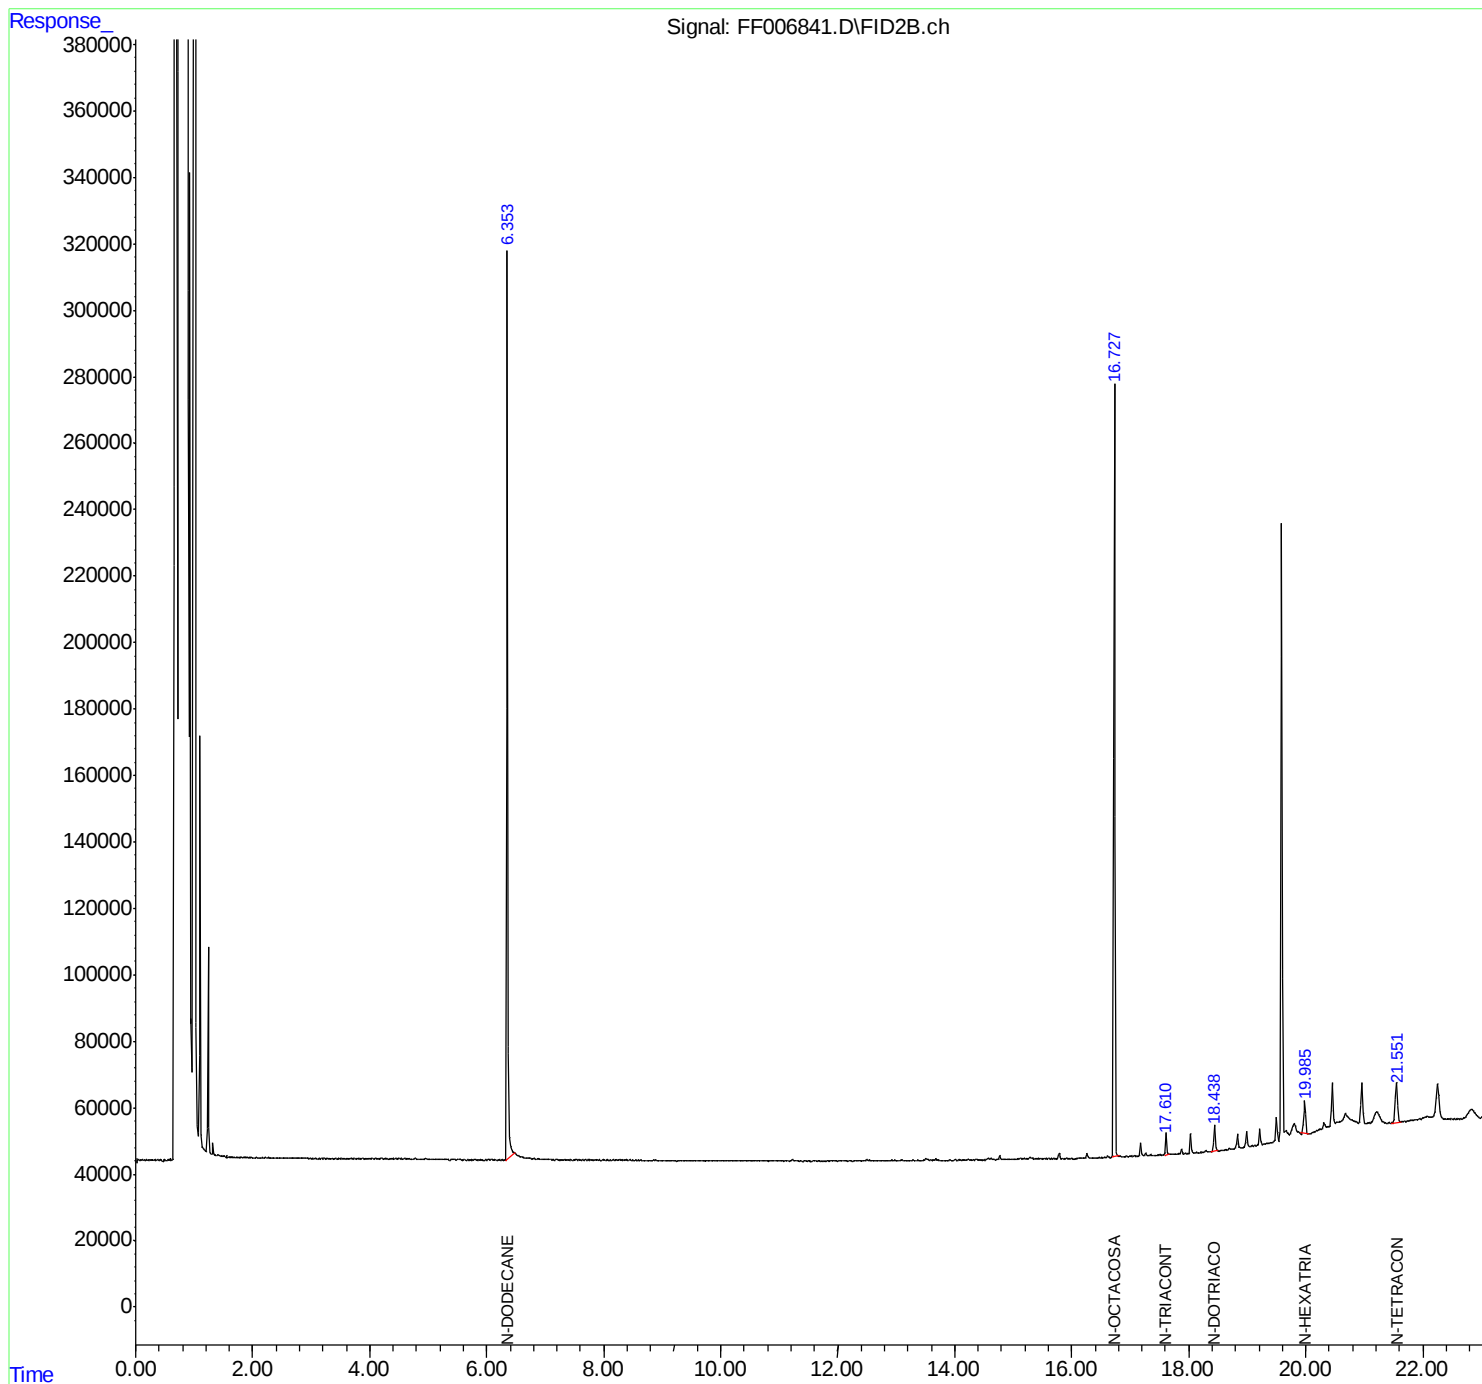


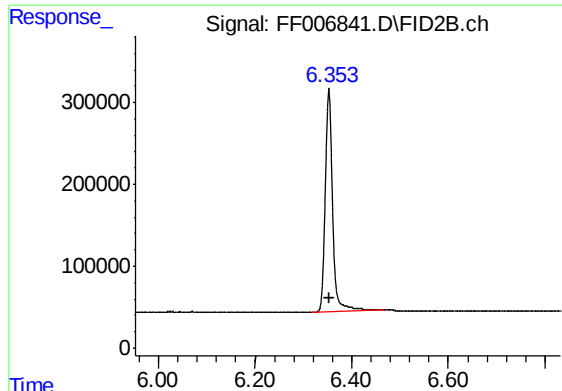

#3 N-DODECANE


R.T.: 6.353 min
Delta R.T.: -0.001 min
Response: 2869988
Conc: 20.13 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

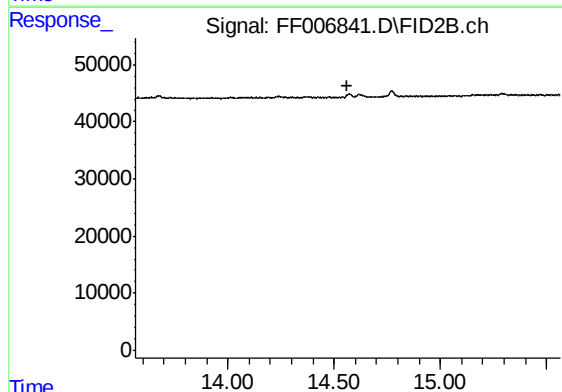


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.565 min
Response: 0
Conc: N.D.

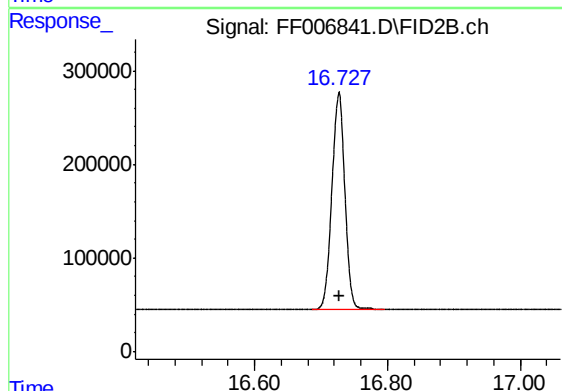


#12 N-OCTACOSANE

R.T.: 16.727 min
Delta R.T.: -0.001 min
Response: 3125145
Conc: 20.28 ug/ml

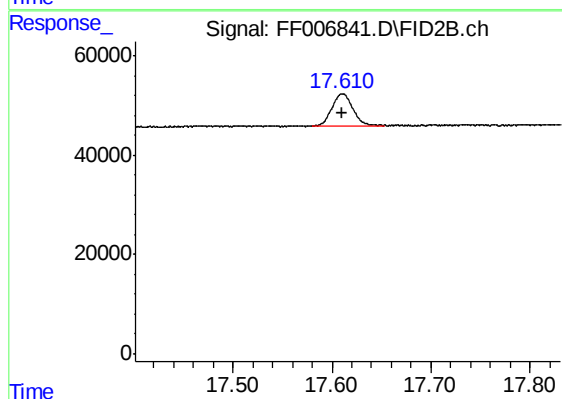

#13 N-TRIACONTANE


R.T.: 17.611 min
Delta R.T.: 0.000 min
Response: 94783
Conc: 0.61 ug/ml

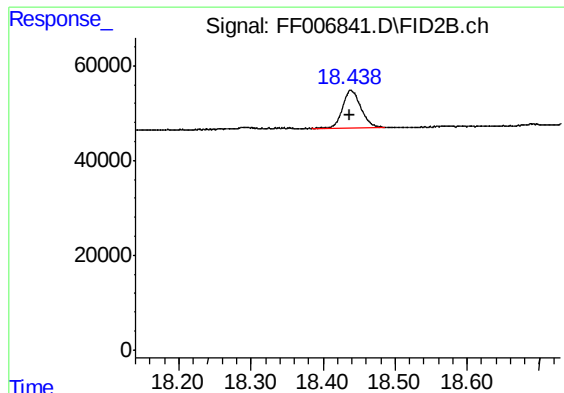

#14 N-DOTRIACONTANE


R.T.: 18.439 min
Delta R.T.: 0.000 min
Response: 137811
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

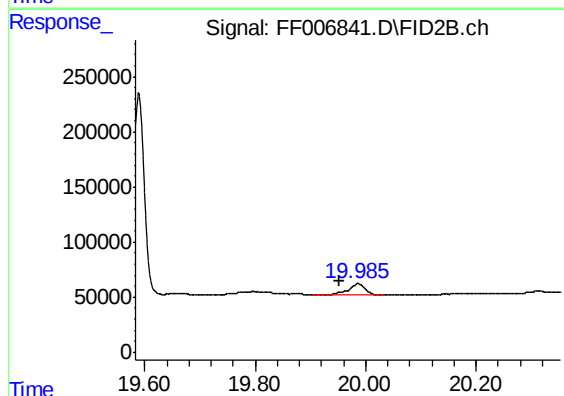

#16 N-HEXATRIACONTANE

R.T.: 19.986 min
Delta R.T.: 0.032 min
Response: 202062
Conc: 1.68 ug/ml

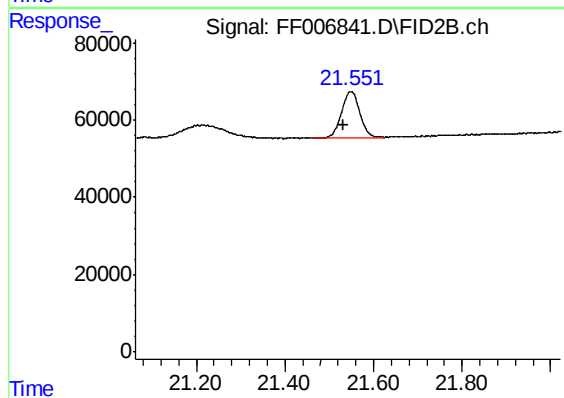

#18 N-TETRACONTANE

R.T.: 21.550 min
Delta R.T.: 0.017 min
Response: 337798
Conc: 3.23 ug/ml