

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050621\
Data File : FF008365.D
Signal(s) : FID2B.ch
Acq On : 06 May 2021 10:49
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 07 01:58:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.547	4840316	35.403 ug/ml
12)	N-OCTACOSANE	16.950	5104395	36.378 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050621\
Data File : FF008365.D
Signal(s) : FID2B.ch
Acq On : 06 May 2021 10:49
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 07 01:58:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

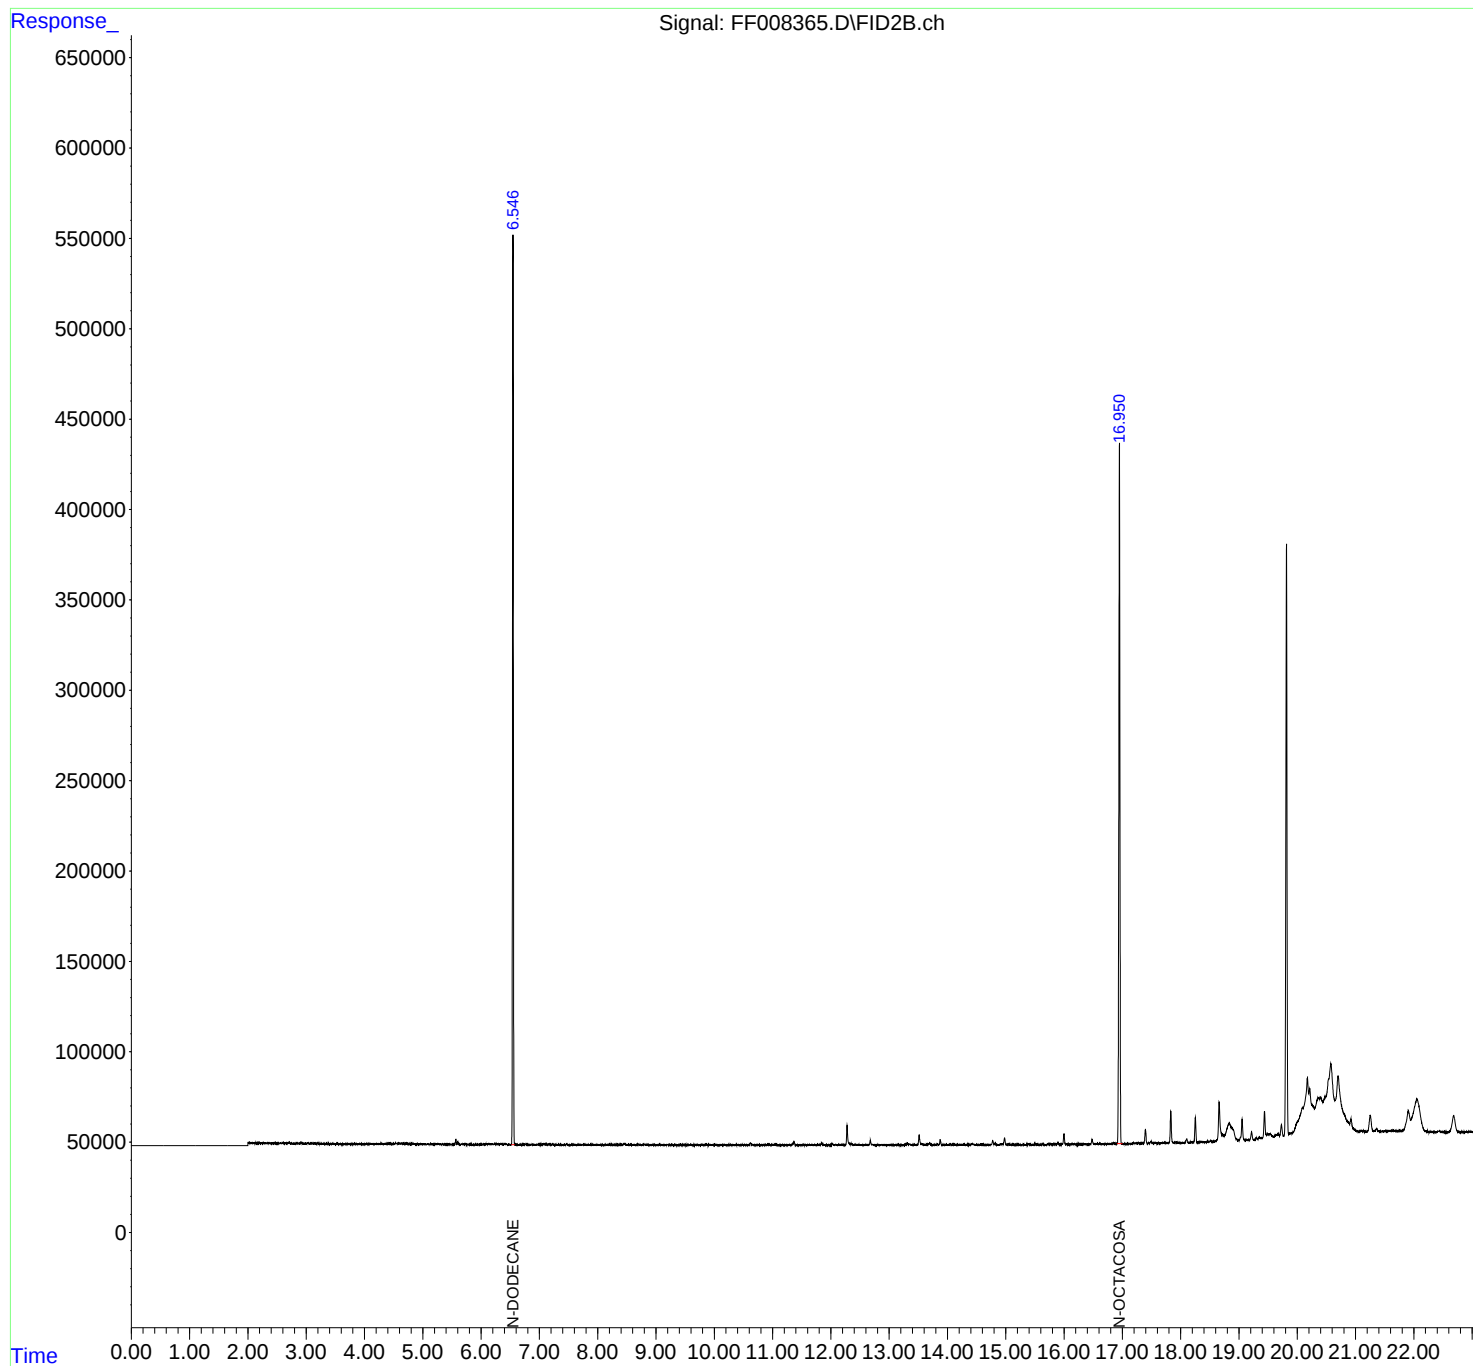


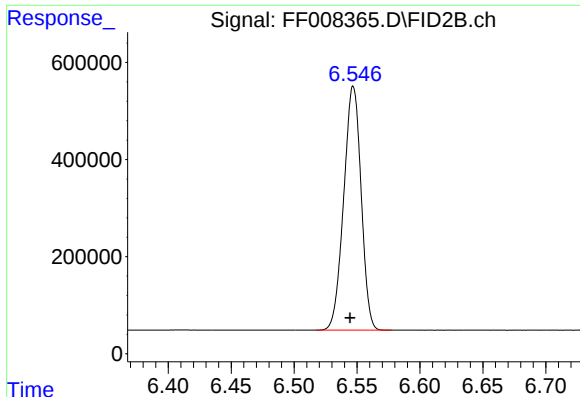

#3 N-DODECANE


R.T.: 6.547 min
Delta R.T.: 0.002 min
Response: 4840316
Conc: 35.40 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

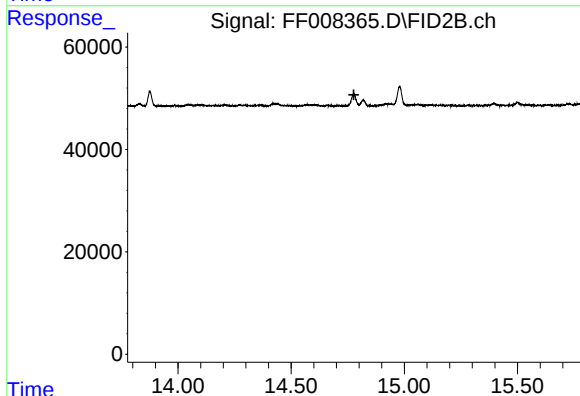

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

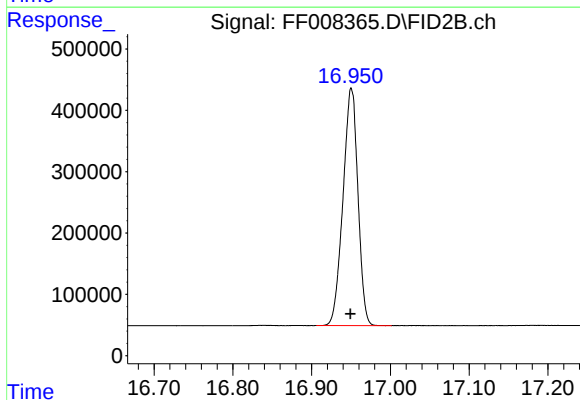

#12 N-OCTACOSANE

R.T.: 16.950 min
Delta R.T.: 0.000 min
Response: 5104395
Conc: 36.38 ug/ml