

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050622\
 Data File : FF010561.D
 Signal(s) : FID2B.ch
 Acq On : 06 May 2022 08:41
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 08 22:51:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.495	182439	1.303 ug/ml
8)	N-DOCOSANE	13.703	209431	1.508 ug/ml
10)	N-TETRACOSANE	14.807	121540	0.880 ug/ml
13)	N-TRIACONTANE	17.664	186145	1.465 ug/ml
14)	N-DOTRIACONTANE	18.496	221580	1.847 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050622\
Data File : FF010561.D
Signal(s) : FID2B.ch
Acq On : 06 May 2022 08:41
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 08 22:51:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

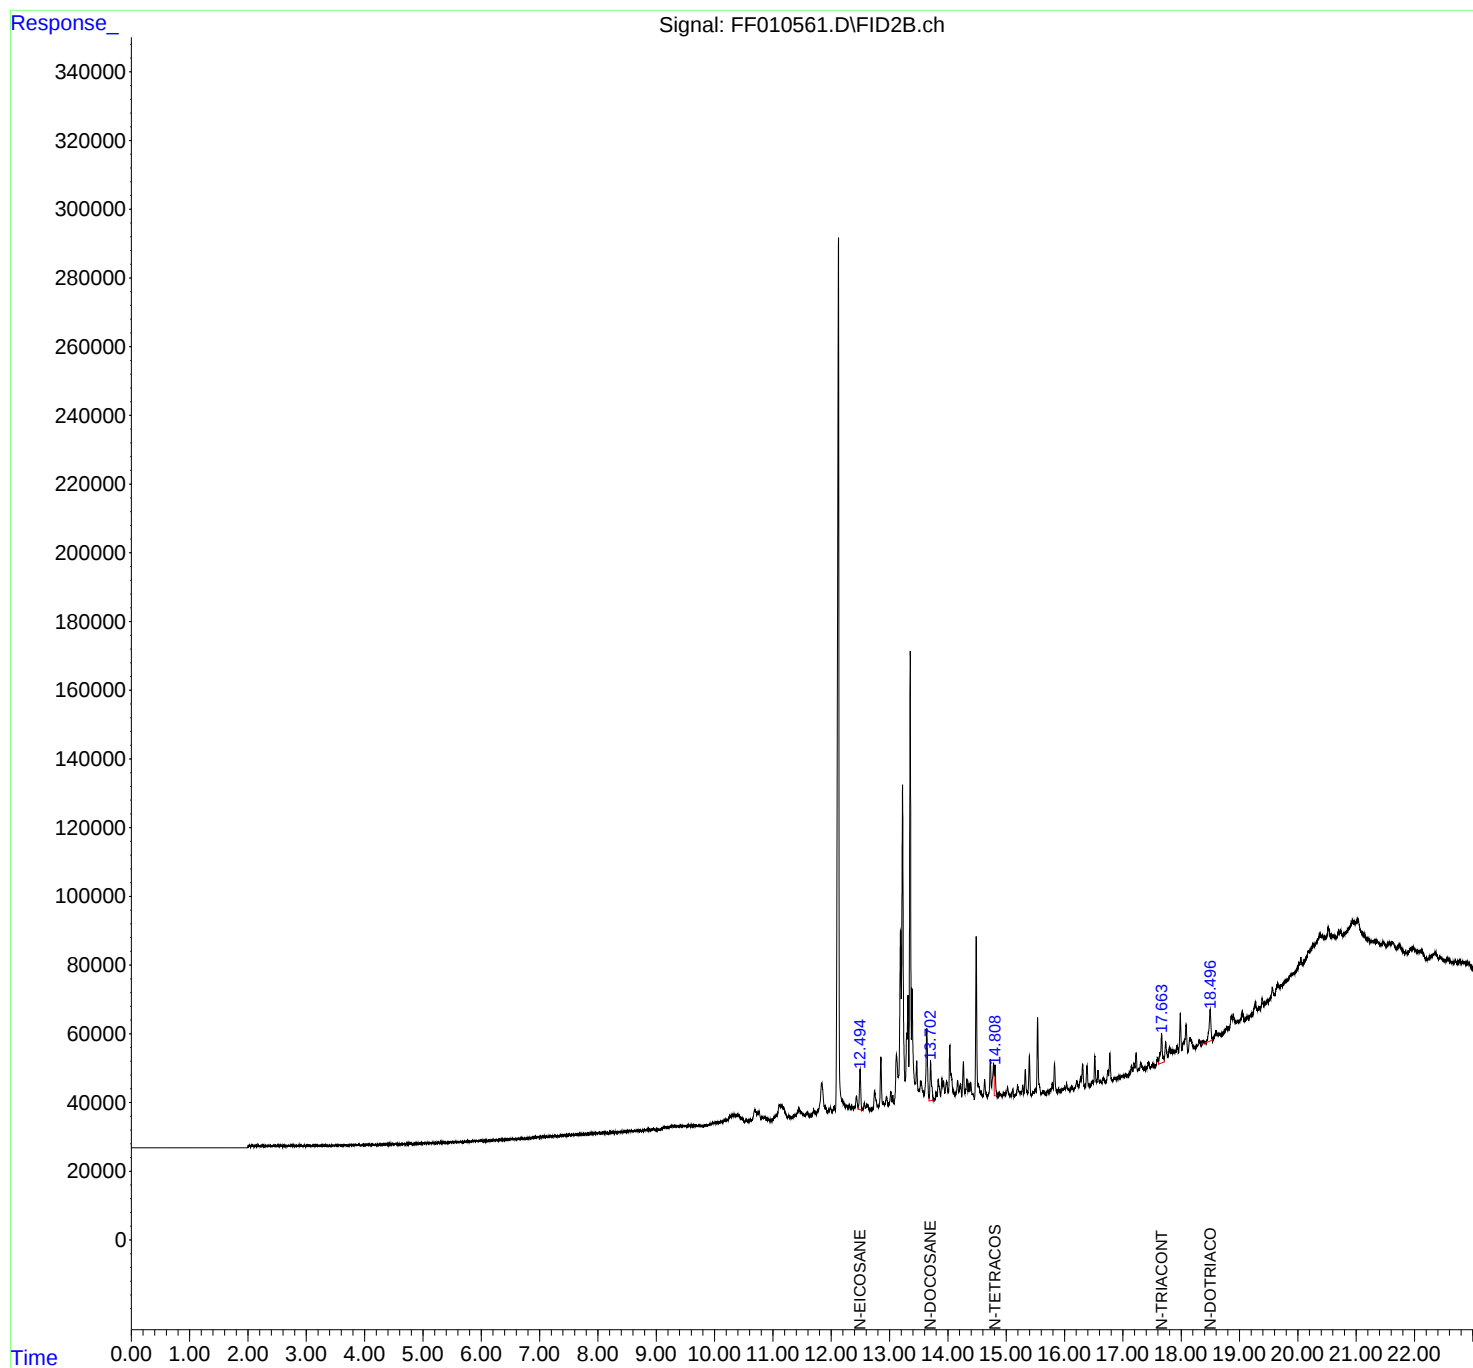


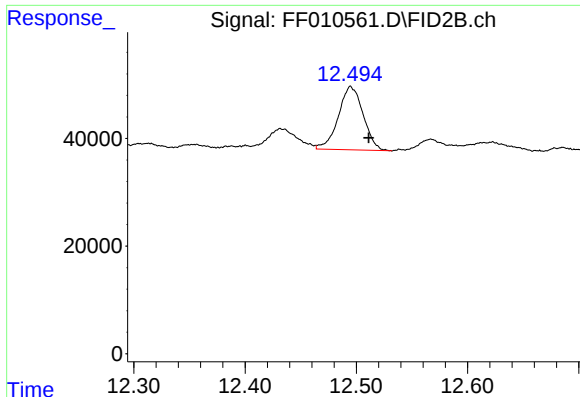

#7 N-EICOSANE


R.T.: 12.495 min
Delta R.T.: -0.016 min
Response: 182439
Conc: 1.30 ug/ml

Instrument :
FID_F
ClientSampleId :

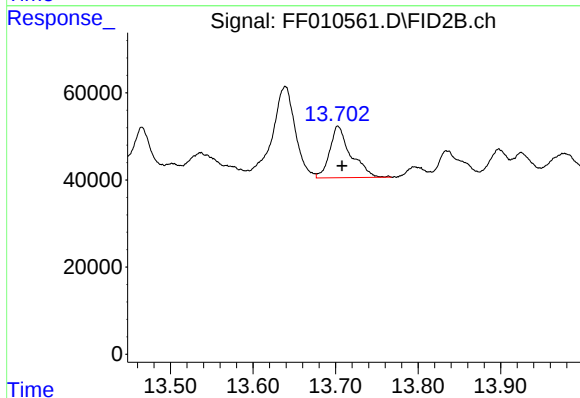


#8 N-DOCOSANE

R.T.: 13.703 min
Delta R.T.: -0.005 min
Response: 209431
Conc: 1.51 ug/ml

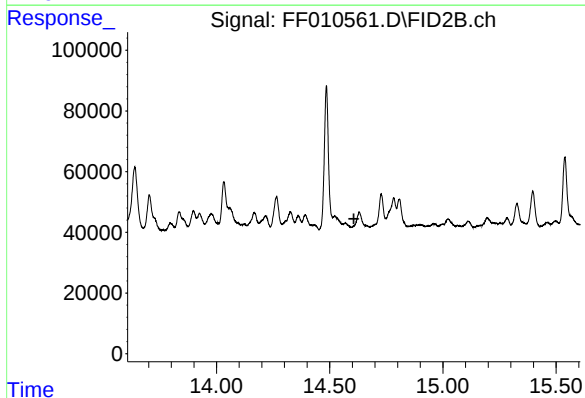


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.607 min
Response: 0
Conc: N.D.

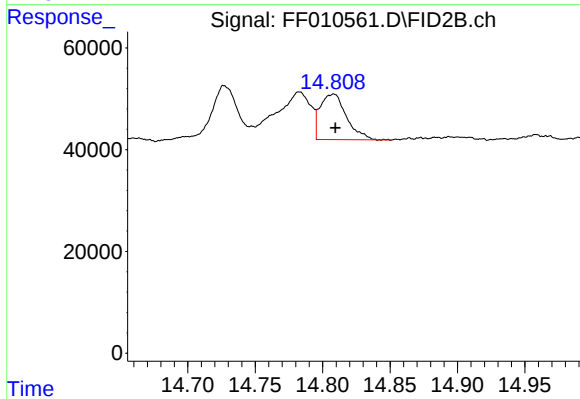

#10 N-TETRACOSANE


R.T.: 14.807 min
Delta R.T.: -0.002 min
Response: 121540
Conc: 0.88 ug/ml

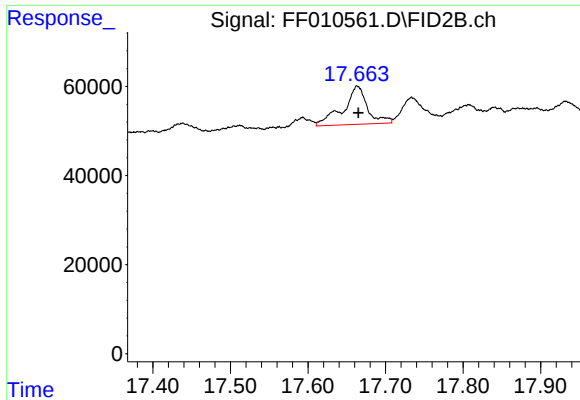

#13 N-TRIACONTANE

R.T.: 17.664 min
Delta R.T.: -0.001 min
Response: 186145
Conc: 1.46 ug/ml

Instrument :
FID_F
ClientSampleId :

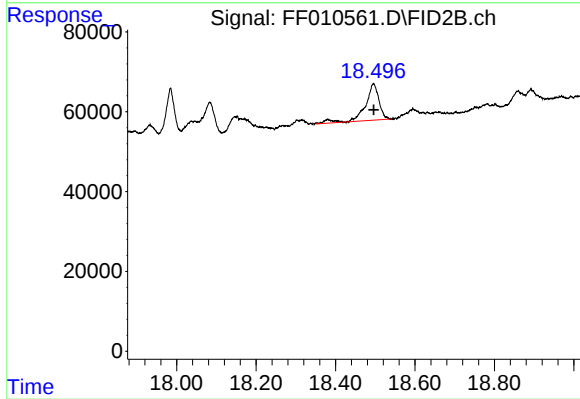

#14 N-DOTRIACONTANE

R.T.: 18.496 min
Delta R.T.: 0.000 min
Response: 221580
Conc: 1.85 ug/ml