

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050622\
Data File : FF010575.D
Signal(s) : FID2B.ch
Acq On : 06 May 2022 18:57
Operator : AJ\MA
Sample : N2706-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RBS-BD002-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

Integration File: autoint1.e
Quant Time: May 08 22:53:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.600	5882396	47.965 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050622\
Data File : FF010575.D
Signal(s) : FID2B.ch
Acq On : 06 May 2022 18:57
Operator : AJ\MA
Sample : N2706-01
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
RBS-BD002-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/09/2022
Supervised By :mohammad ahmed 05/09/2022

Integration File: autoint1.e
Quant Time: May 08 22:53:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

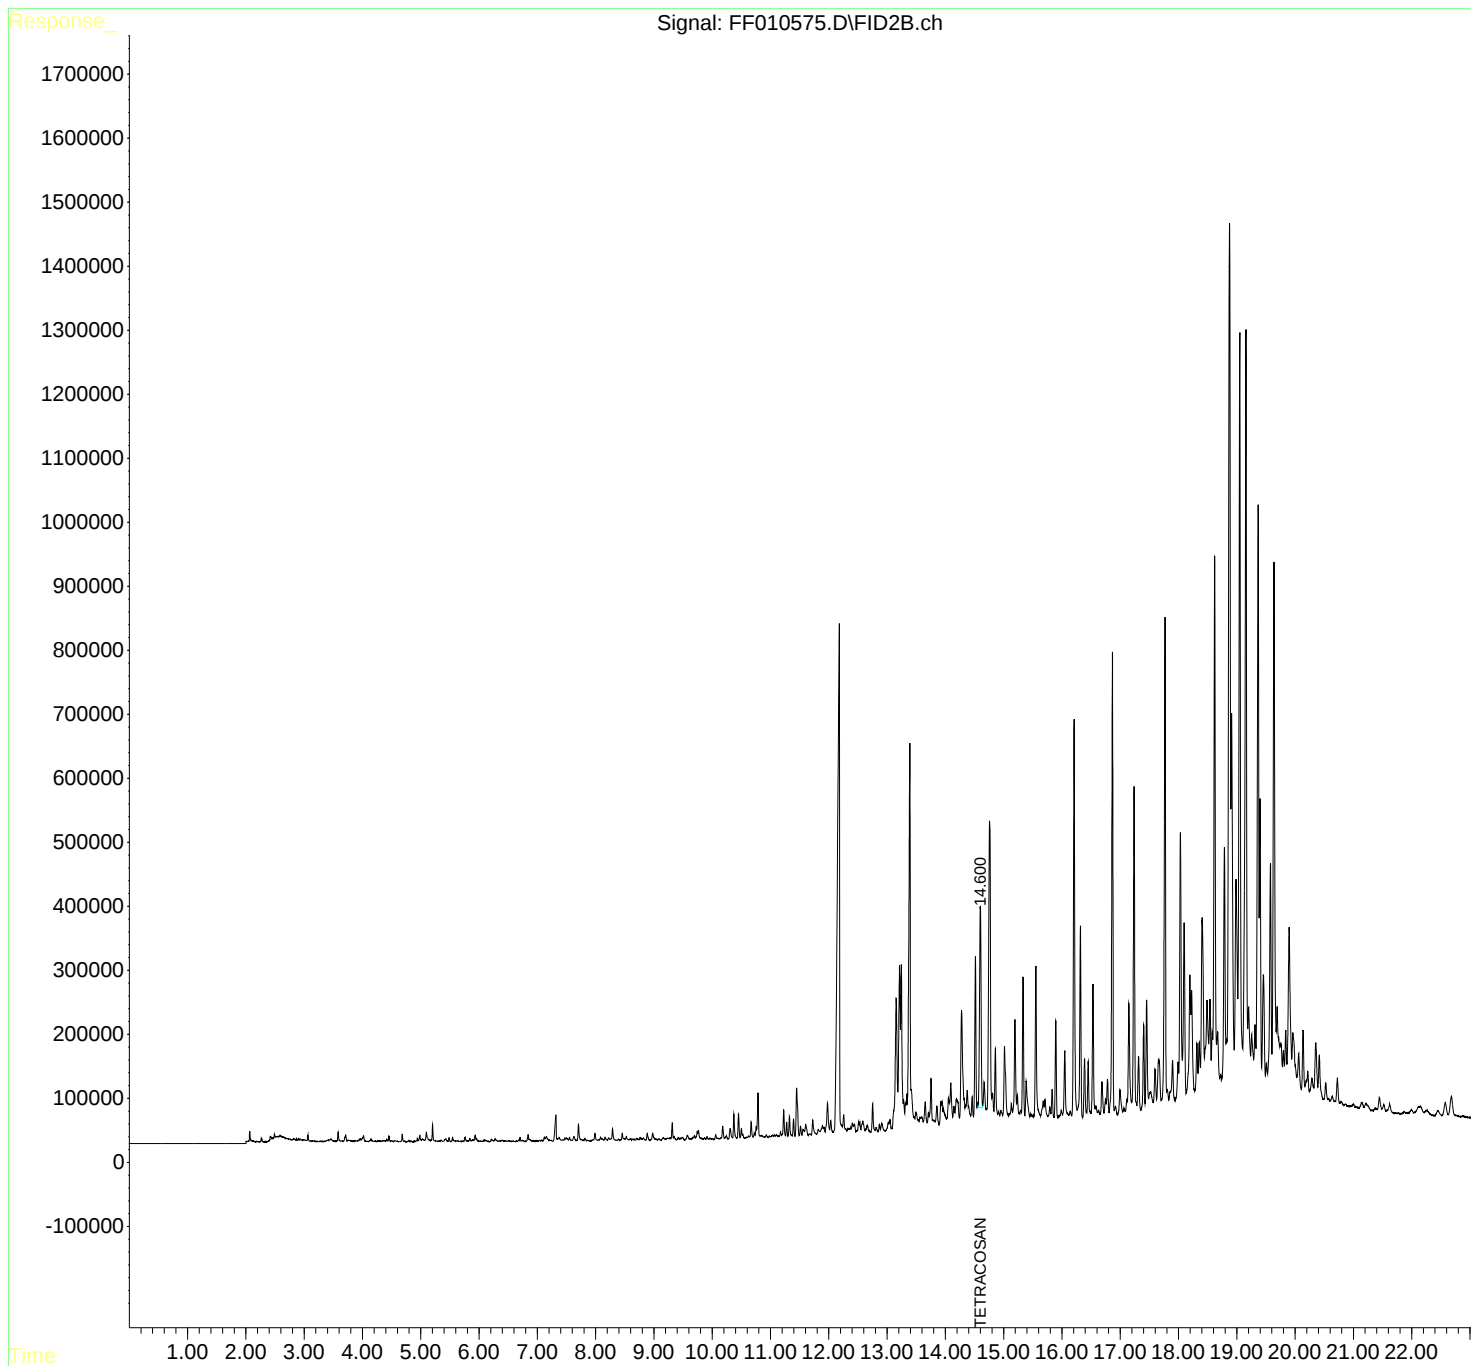

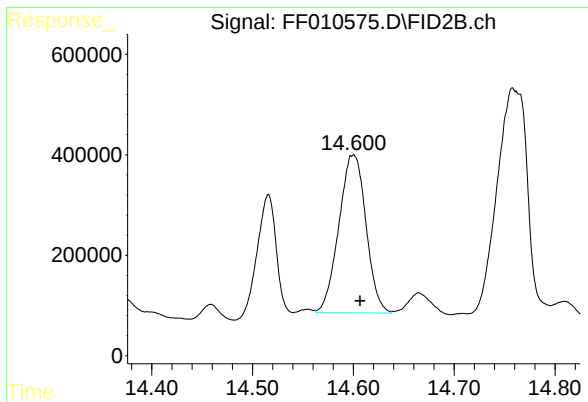

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.600 min
Delta R.T.: -0.006 min
Response: 5882396
Conc: 47.96 ug/ml

Instrument :

FID_F

ClientSampleId :

RBS-BD002-01

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/09/2022

Supervised By :mohammad ahmed 05/09/2022