

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
 Data File : FF006846.D
 Signal(s) : FID2B.ch
 Acq On : 07 May 2020 06:56
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: May 08 00:57:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.608	95248	0.614 ug/ml
14) N-DOTRIACONTANE	18.440	267258	1.817 ug/ml
16) N-HEXATRIACONTANE	19.984	264014	2.193 ug/ml
18) N-TETRACONTANE	21.546	225244	2.151 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006846.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 06:56
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
MECL2

Integration File: autoint1.e
Quant Time: May 08 00:57:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

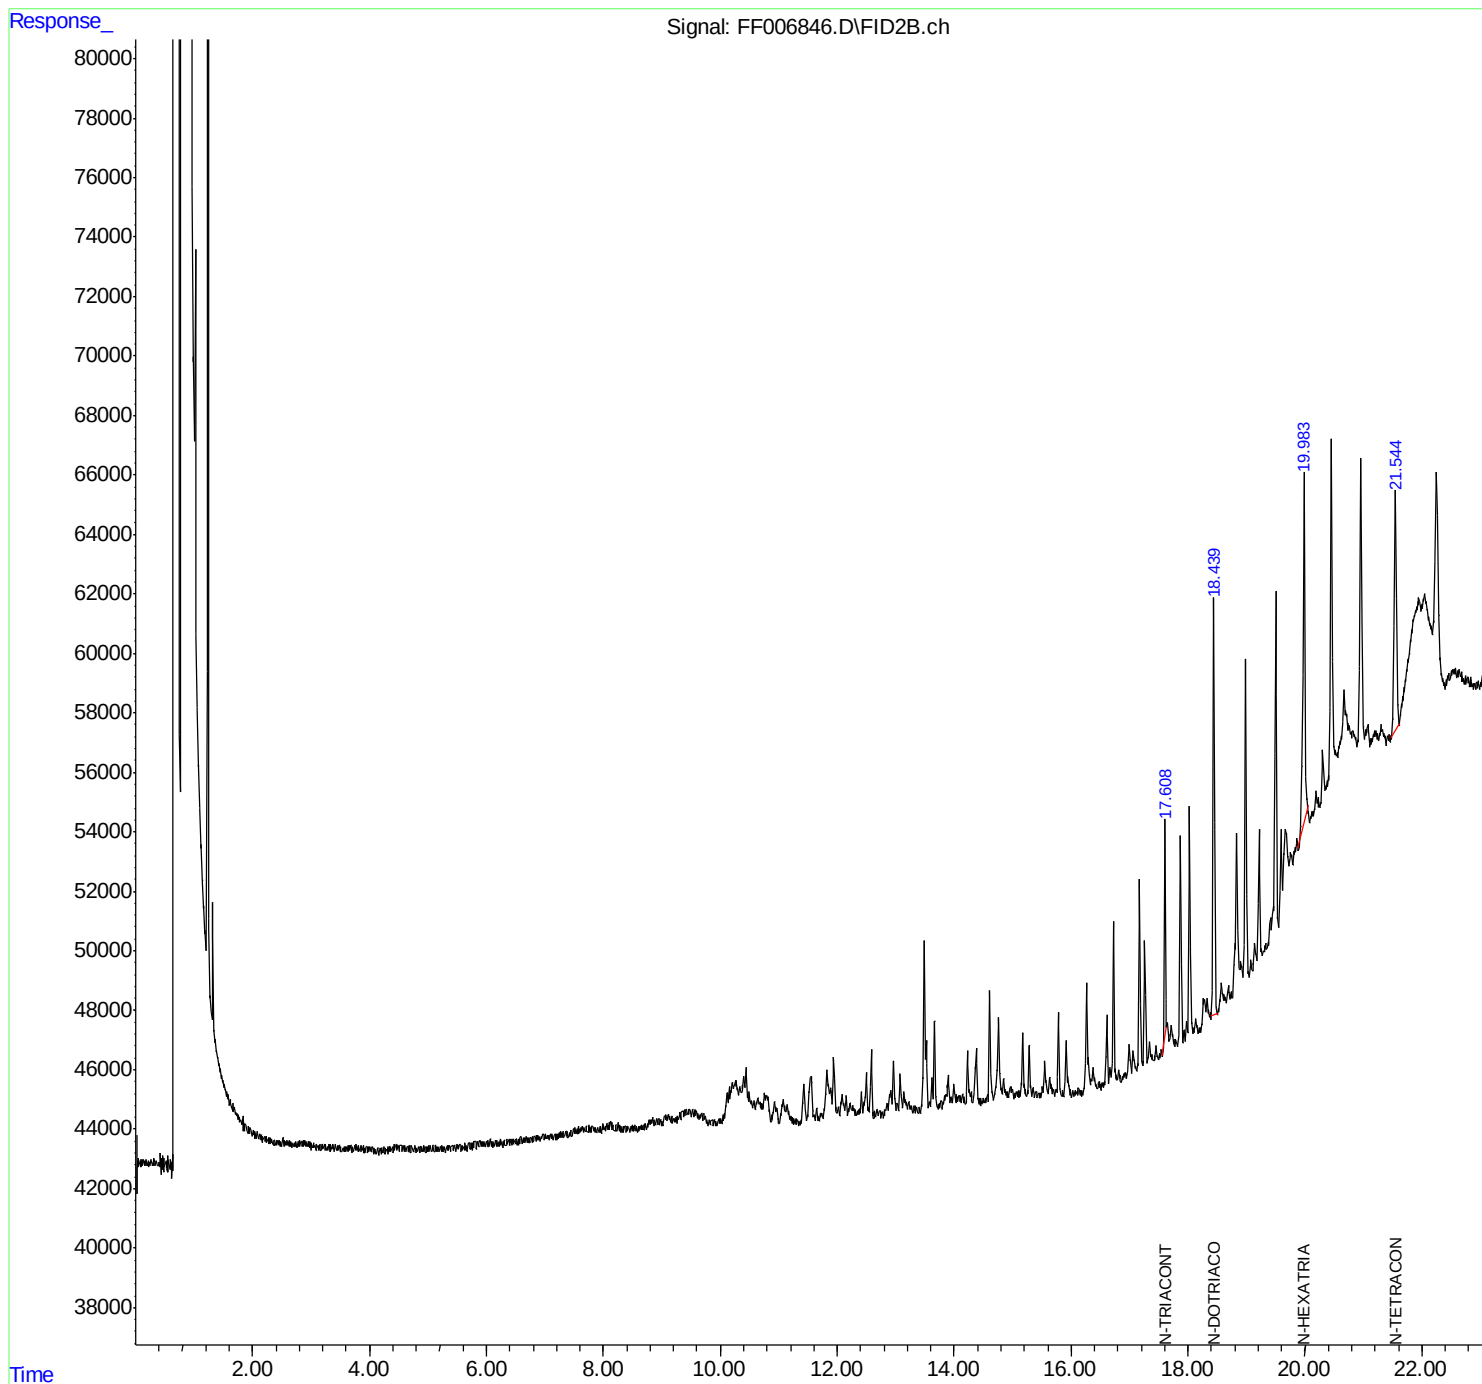


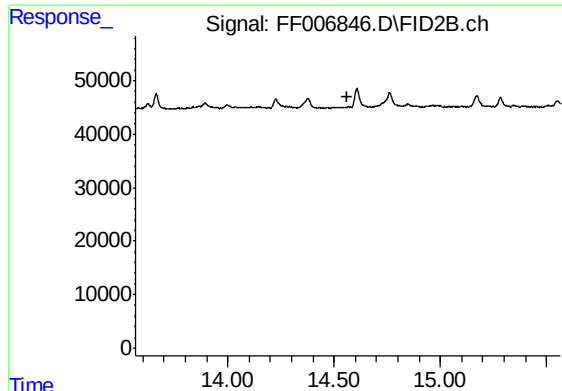

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.565 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

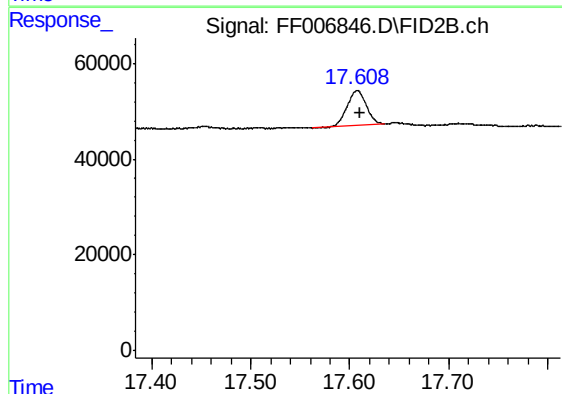


#13 N-TRIACONTANE

R.T.: 17.608 min
Delta R.T.: -0.003 min
Response: 95248
Conc: 0.61 ug/ml

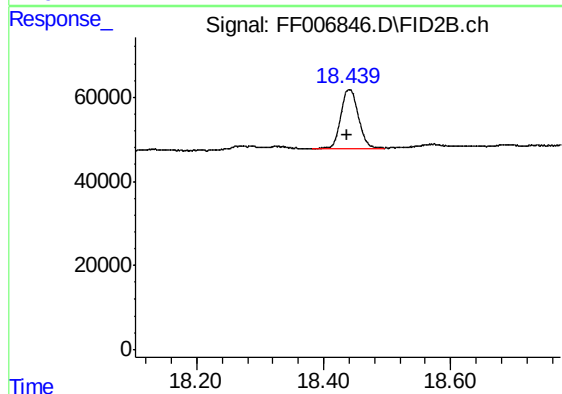


#14 N-DOTRIACONTANE

R.T.: 18.440 min
Delta R.T.: 0.002 min
Response: 267258
Conc: 1.82 ug/ml

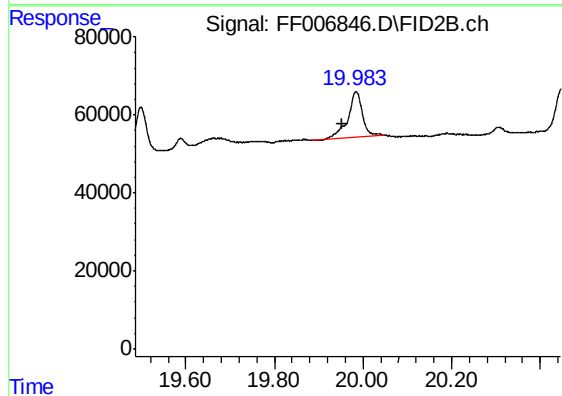

#16 N-HEXATRIACONTANE

R.T.: 19.984 min
Delta R.T.: 0.030 min
Response: 264014
Conc: 2.19 ug/ml

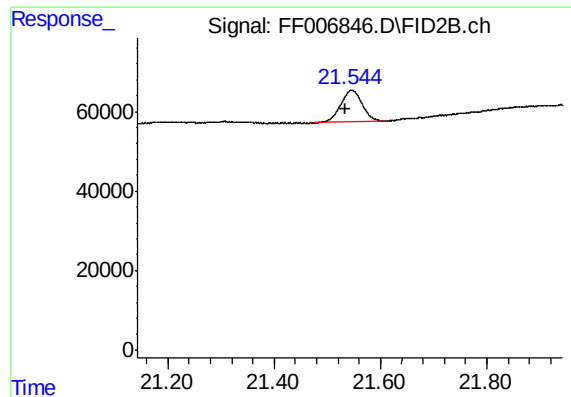

#18 N-TETRACONTANE

R.T.: 21.546 min
Delta R.T.: 0.013 min
Response: 225244
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :
MECL2