

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
 Data File : FF006852.D
 Signal(s) : FID2B.ch
 Acq On : 07 May 2020 10:27
 Operator : DD\AJ
 Sample : L2473-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WASTE

Integration File: autoint1.e
 Quant Time: May 08 00:58:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.563	1868984	13.758 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.780	147071	0.952 ug/ml
12) N-OCTACOSANE	16.726	284332	1.845 ug/ml
13) N-TRIACONTANE	17.608	347759	2.241 ug/ml
14) N-DOTRIACONTANE	18.435	299879	2.038 ug/ml
16) N-HEXATRIACONTANE	19.987	121424	1.008 ug/ml
18) N-TETRACONTANE	21.547	244223	2.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006852.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 10:27
Operator : DD\AJ
Sample : L2473-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: May 08 00:58:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

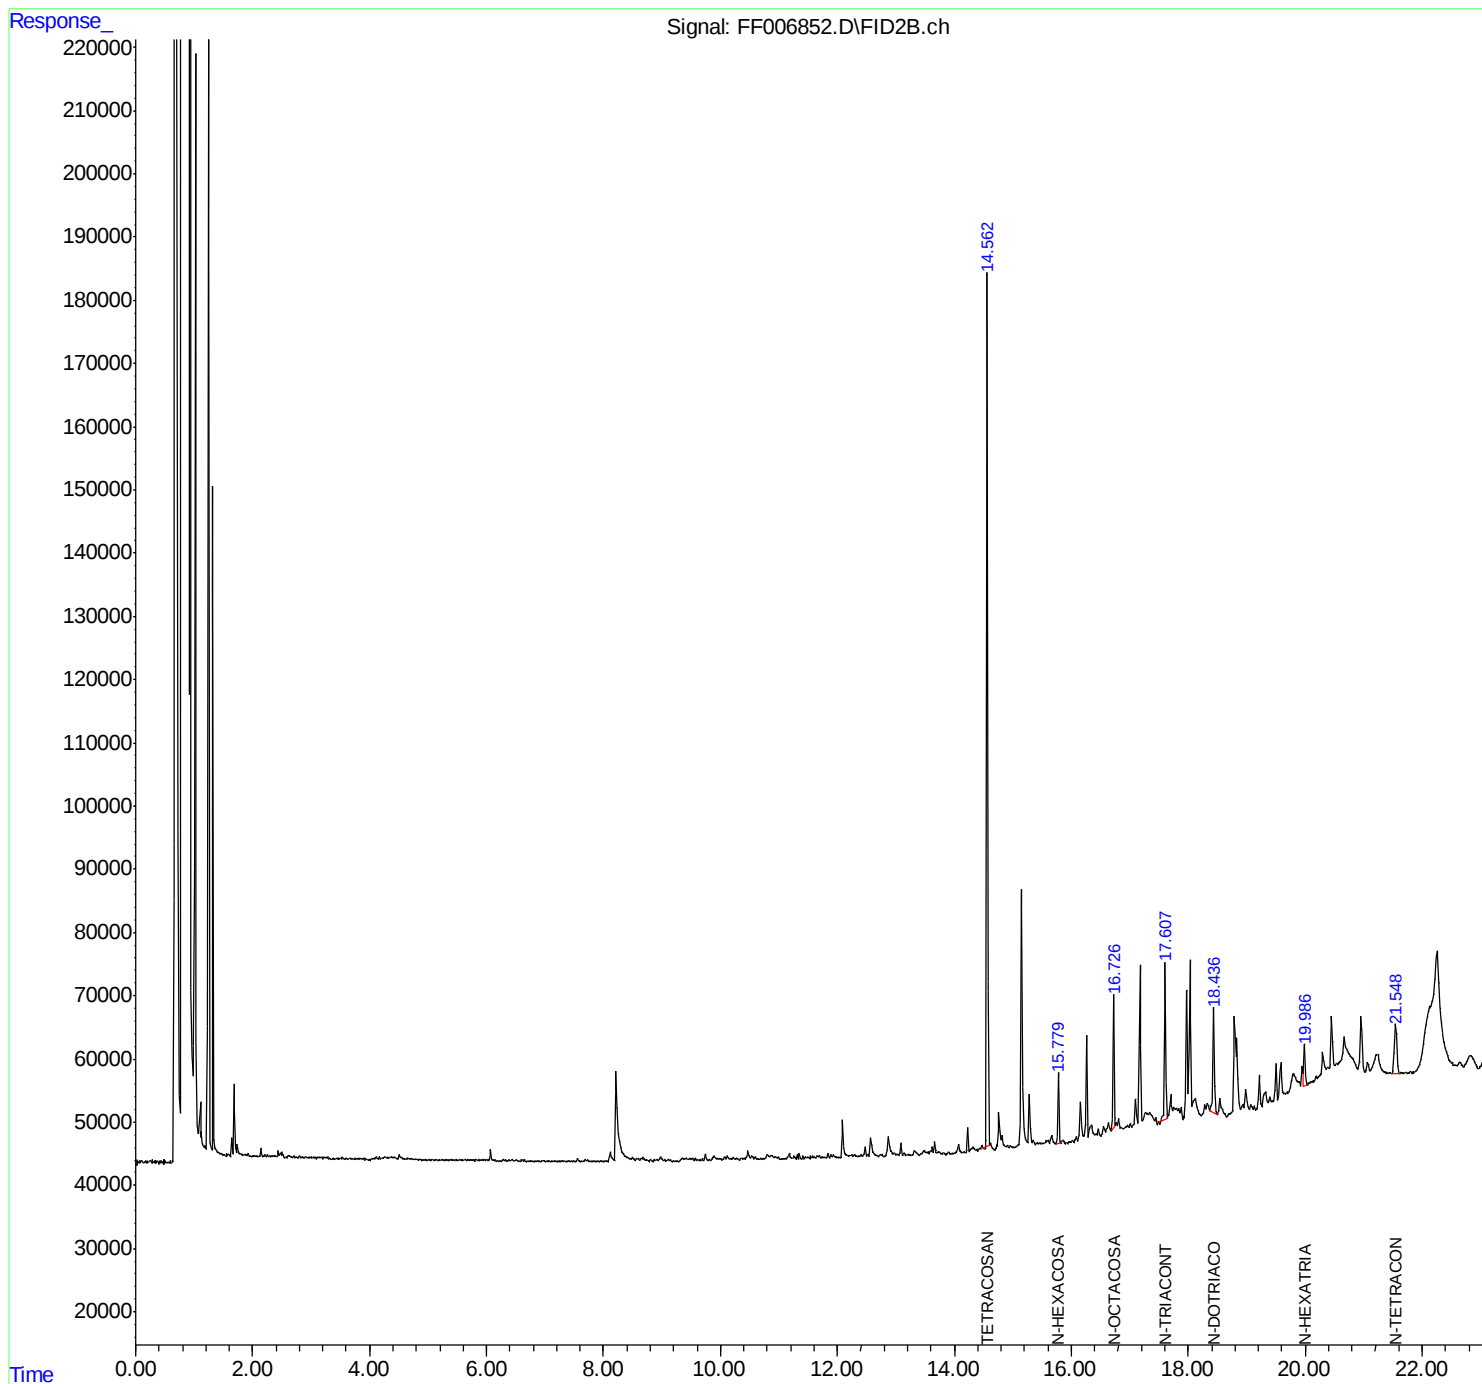


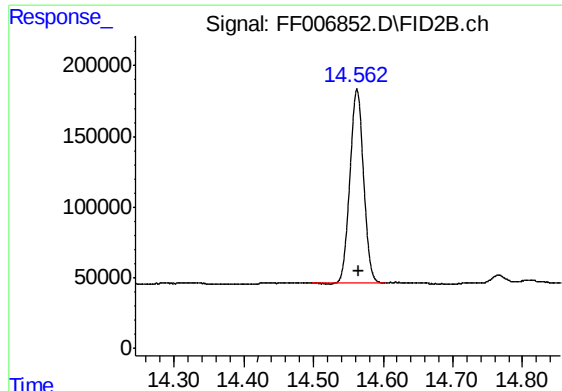

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.563 min
Delta R.T.: -0.002 min
Response: 1868984
Conc: 13.76 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE

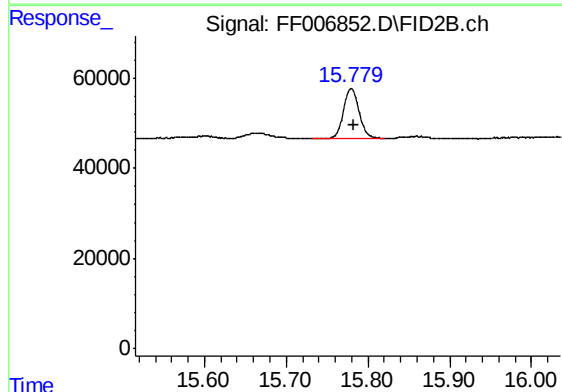


#11 N-HEXACOSANE

R.T.: 15.780 min
Delta R.T.: -0.004 min
Response: 147071
Conc: 0.95 ug/ml

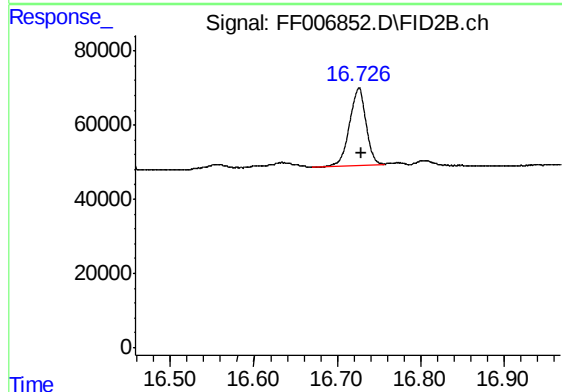


#12 N-OCTACOSANE

R.T.: 16.726 min
Delta R.T.: -0.002 min
Response: 284332
Conc: 1.84 ug/ml

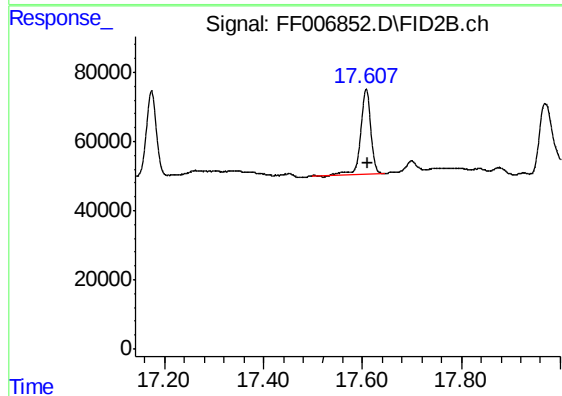

#13 N-TRIACONTANE


R.T.: 17.608 min
Delta R.T.: -0.003 min
Response: 347759
Conc: 2.24 ug/ml

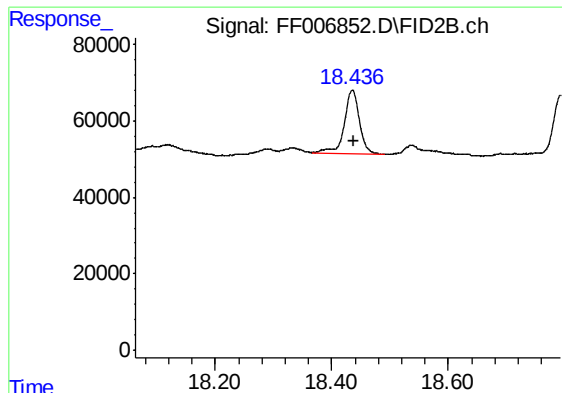

#14 N-DOTRIACONTANE


R.T.: 18.435 min
Delta R.T.: -0.003 min
Response: 299879
Conc: 2.04 ug/ml

Instrument :
FID_F
ClientSampleId :
WASTE

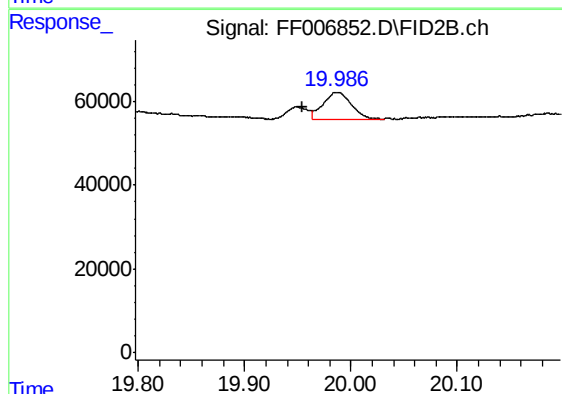

#16 N-HEXATRIACONTANE

R.T.: 19.987 min
Delta R.T.: 0.033 min
Response: 121424
Conc: 1.01 ug/ml

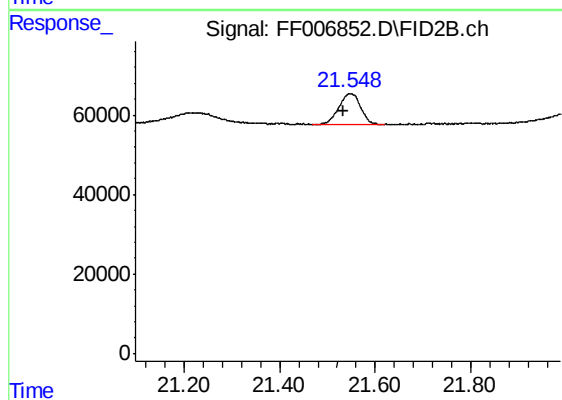

#18 N-TETRACONTANE

R.T.: 21.547 min
Delta R.T.: 0.015 min
Response: 244223
Conc: 2.33 ug/ml