

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006856.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 12:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 08 00:59:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.564	2439624	17.959 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.610	113517	0.732 ug/ml
14) N-DOTRIACONTANE	18.438	141102	0.959 ug/ml
18) N-TETRACONTANE	21.564	8654199	82.633 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006856.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 12:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 08 00:59:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

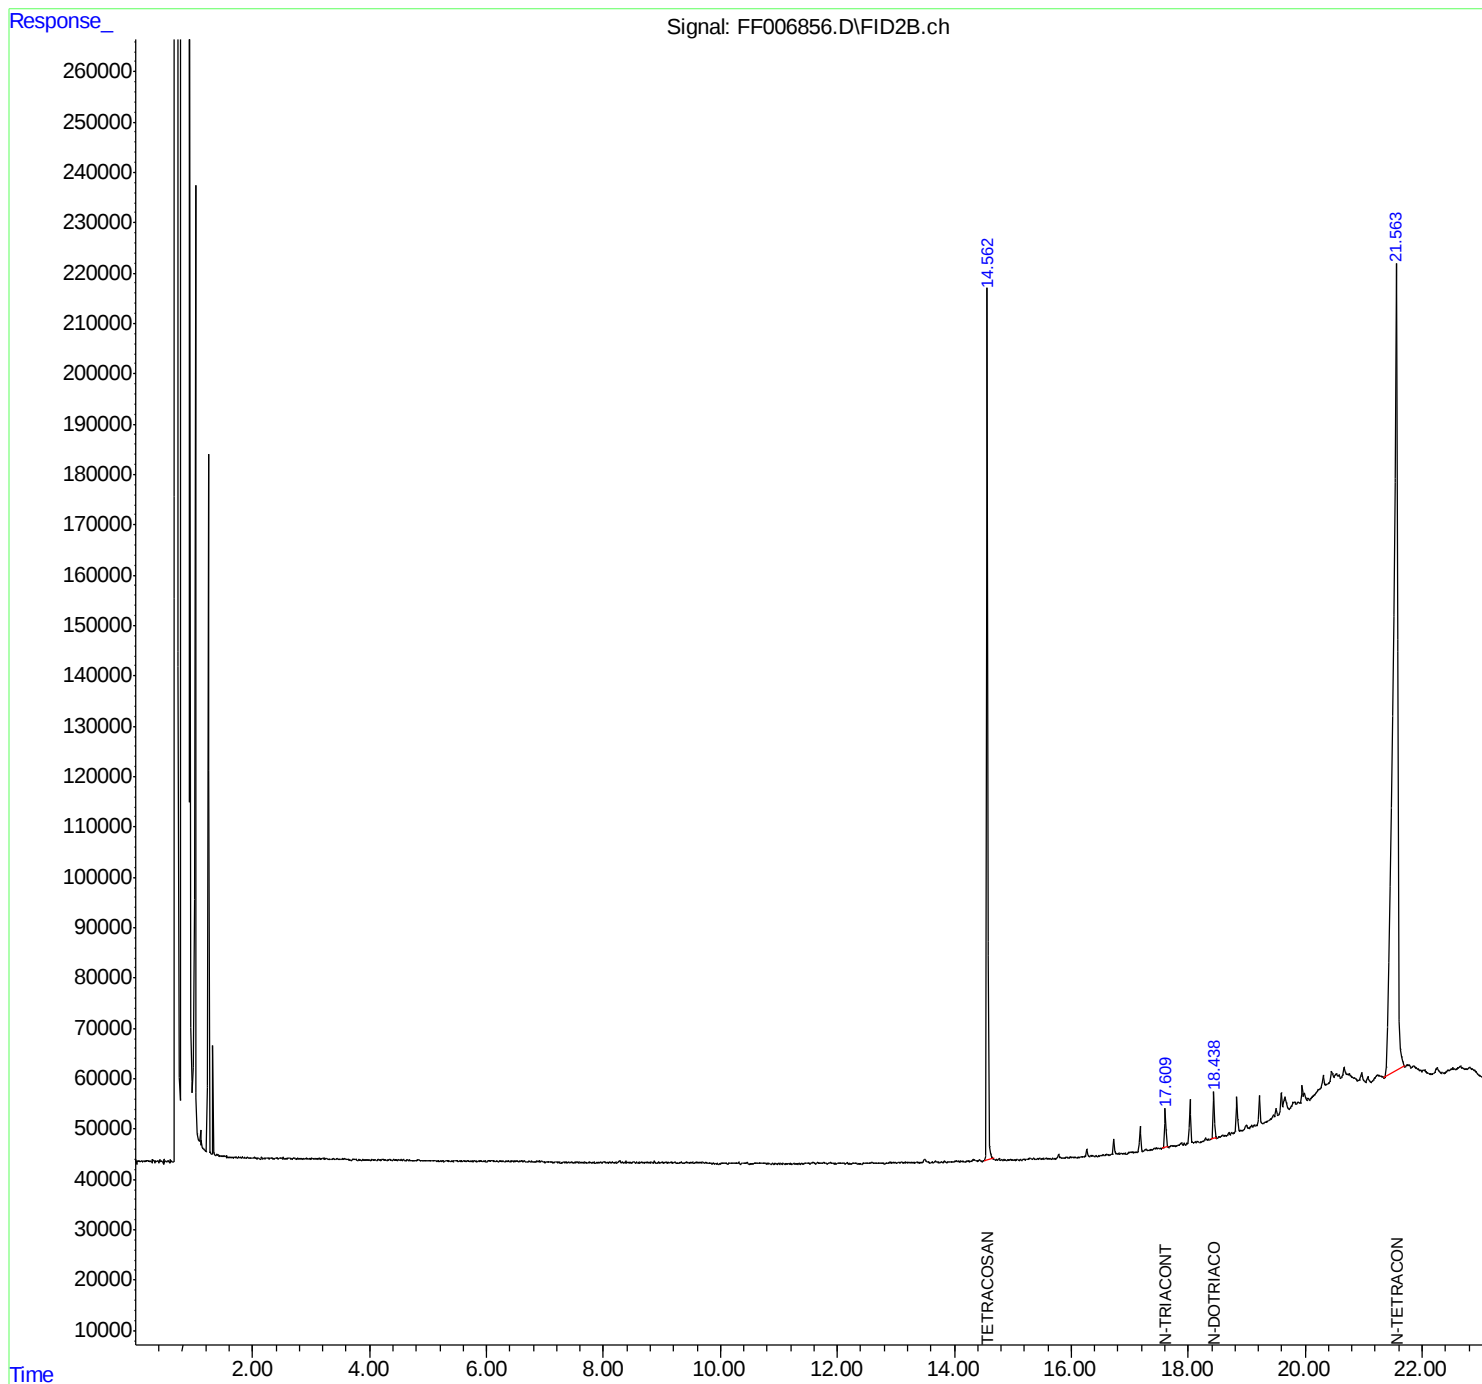


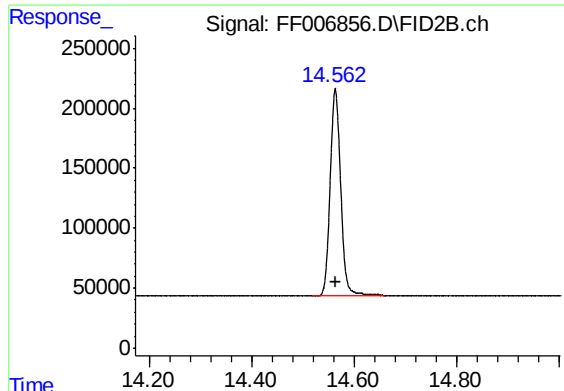

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.564 min
Delta R.T.: -0.001 min
Response: 2439624
Conc: 17.96 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

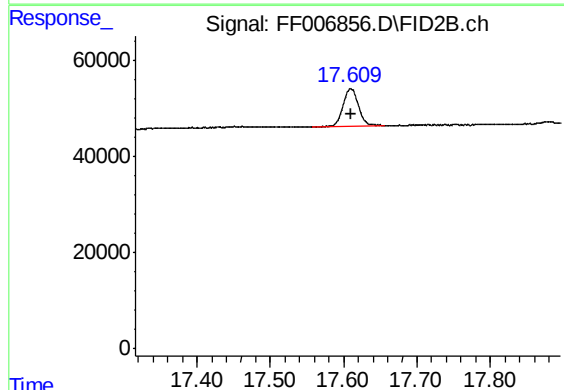


#13 N-TRIACONTANE

R.T.: 17.610 min
Delta R.T.: 0.000 min
Response: 113517
Conc: 0.73 ug/ml

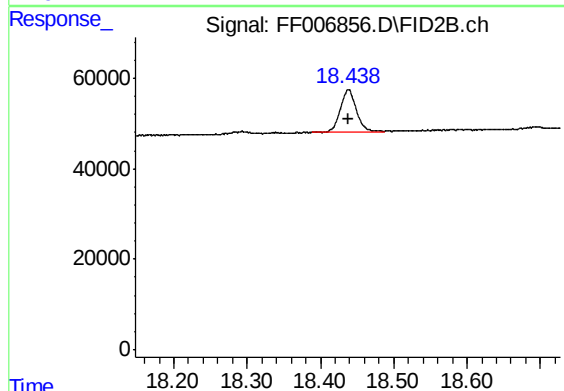

#14 N-DOTRIACONTANE

R.T.: 18.438 min
Delta R.T.: 0.000 min
Response: 141102
Conc: 0.96 ug/ml

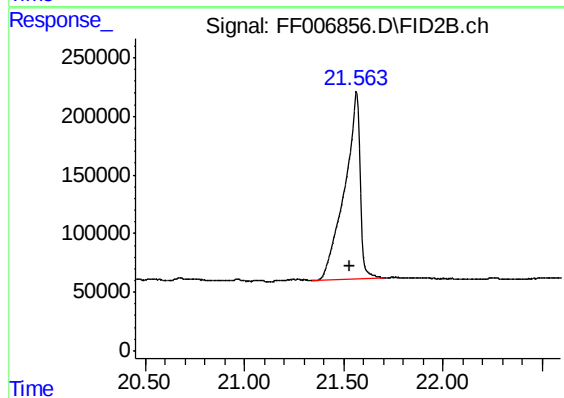

#18 N-TETRACONTANE

R.T.: 21.564 min
Delta R.T.: 0.031 min
Response: 8654199
Conc: 82.63 ug/ml