

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006860.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 14:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 08 01:00:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.352	3172861	22.253 ug/ml
12)	N-OCTACOSANE	16.727	3350960	21.741 ug/ml
13)	N-TRIACONTANE	17.608	193793	1.249 ug/ml
14)	N-DOTRIACONTANE	18.435	216178	1.469 ug/ml
15)	N-TETRATRIACONTANE	19.215	156338	1.182 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050720\
Data File : FF006860.D
Signal(s) : FID2B.ch
Acq On : 07 May 2020 14:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: May 08 01:00:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

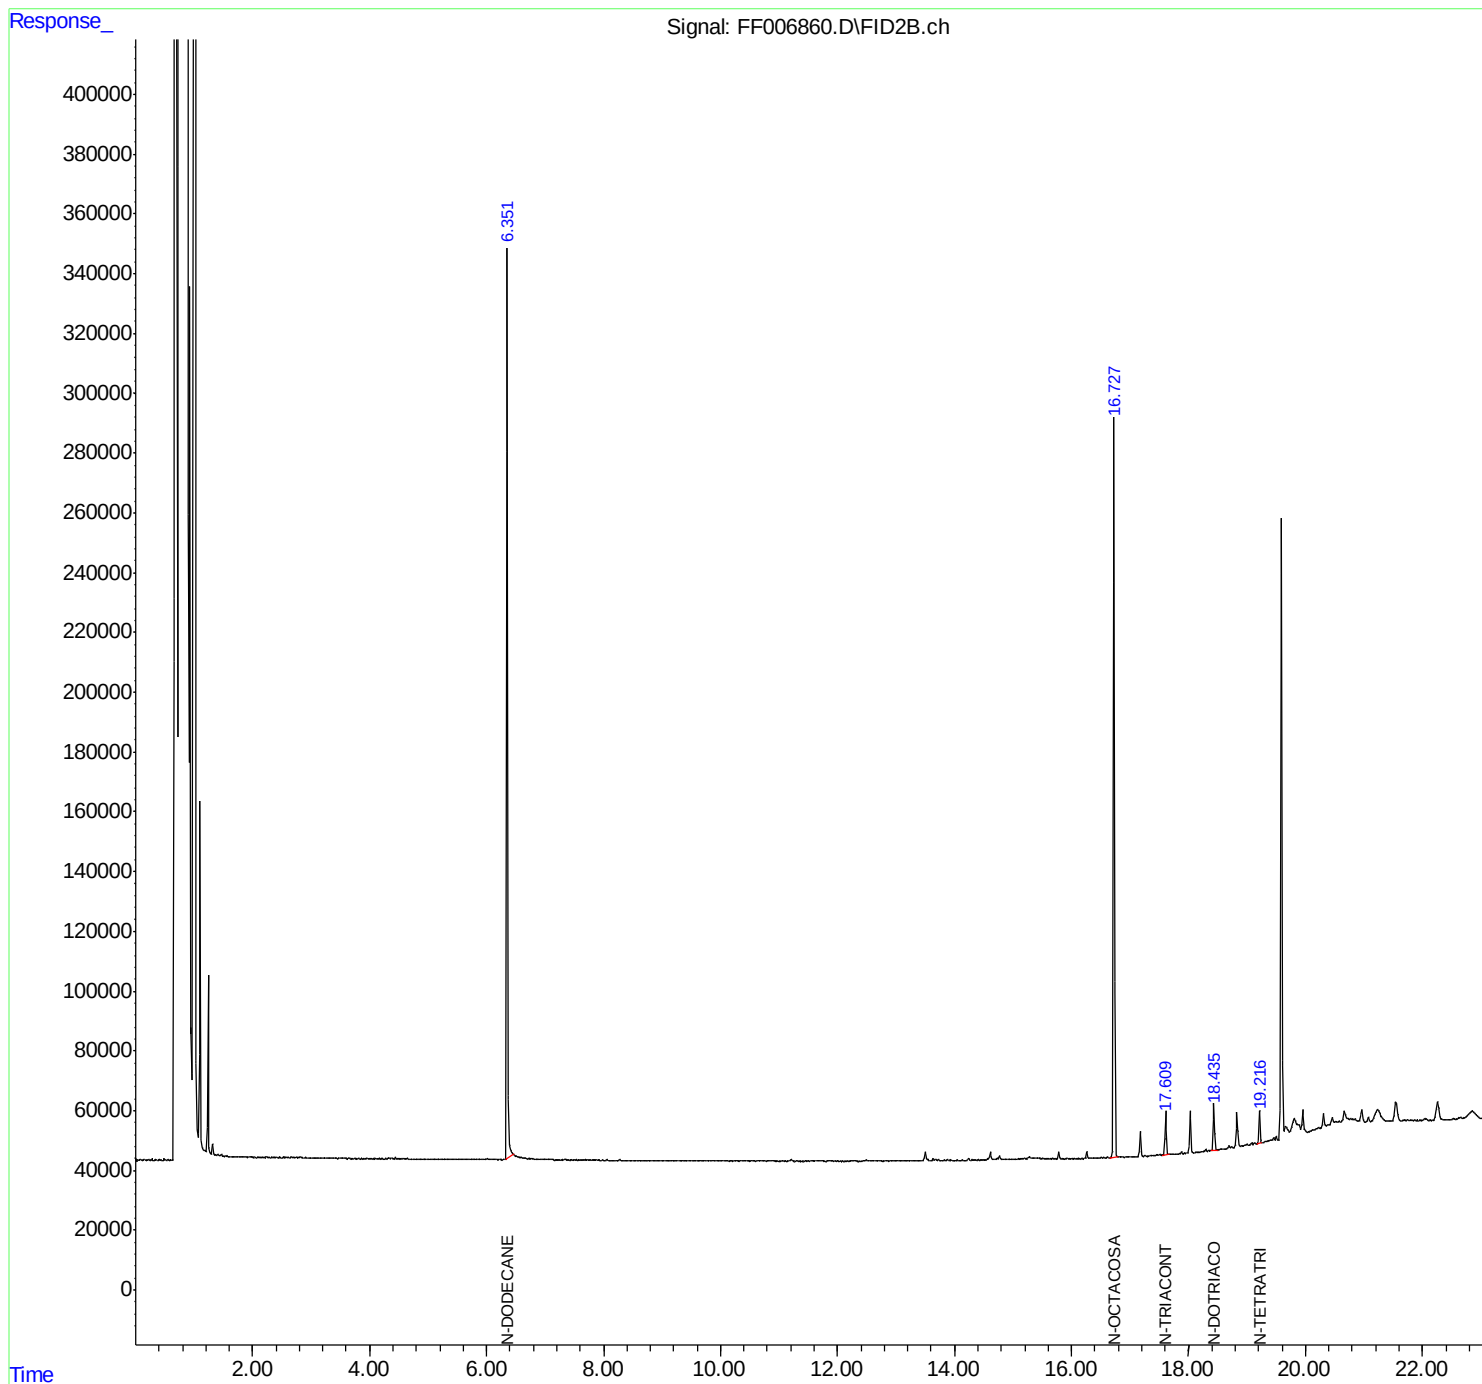


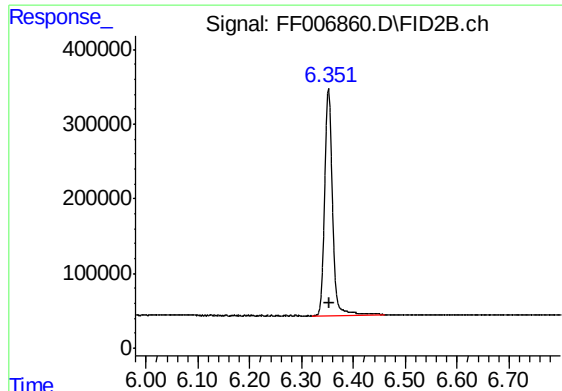

#3 N-DODECANE


R.T.: 6.352 min
Delta R.T.: -0.003 min
Response: 3172861
Conc: 22.25 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

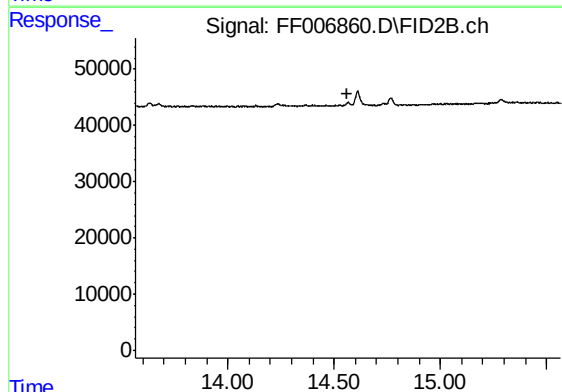


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.565 min
Response: 0
Conc: N.D.

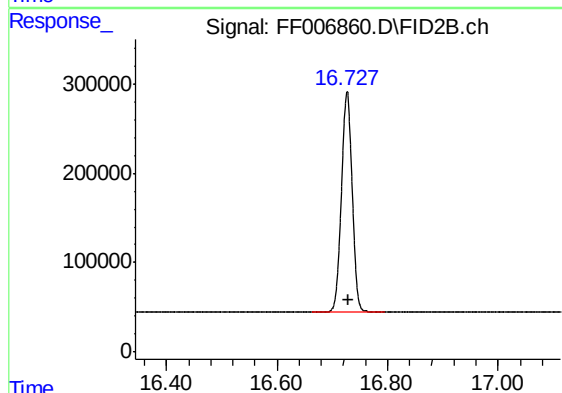


#12 N-OCTACOSANE

R.T.: 16.727 min
Delta R.T.: -0.002 min
Response: 3350960
Conc: 21.74 ug/ml

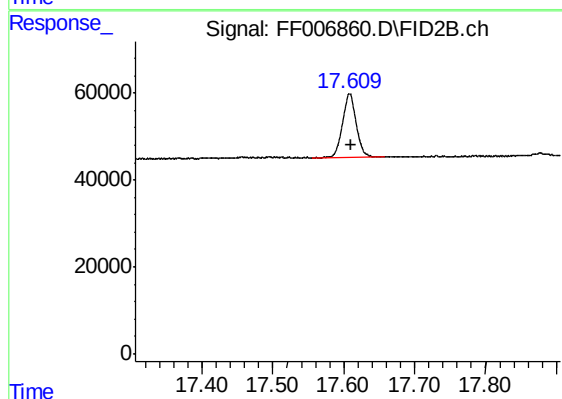

#13 N-TRIACONTANE


R.T.: 17.608 min
Delta R.T.: -0.002 min
Response: 193793
Conc: 1.25 ug/ml

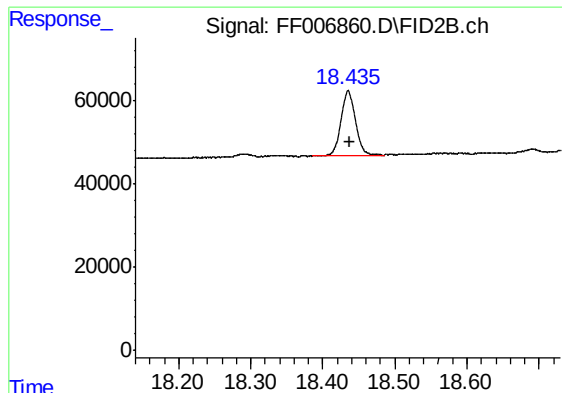

#14 N-DOTRIACONTANE

R.T.: 18.435 min
Delta R.T.: -0.003 min
Response: 216178
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

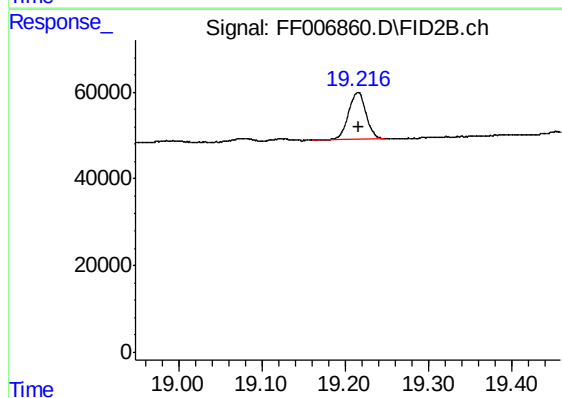

#15 N-TETRATRIACONTANE

R.T.: 19.215 min
Delta R.T.: -0.002 min
Response: 156338
Conc: 1.18 ug/ml