

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050820\
 Data File : FF006896.D
 Signal(s) : FID2B.ch
 Acq On : 08 May 2020 17:23
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 09 03:25:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.577	5460468	40.196 ug/mlm
Target Compounds				
2)	N-DECANE	4.344	6714819	48.755 ug/ml
3)	N-DODECANE	6.359	6816861	47.810 ug/ml
4)	N-TETRADECANE	8.149	6802141	46.836 ug/ml
5)	N-HEXADECANE	9.745	6674259	45.306 ug/ml
6)	N-OCTADECANE	11.182	6806109	43.698 ug/ml
7)	N-EICOSANE	12.487	6530391	42.251 ug/ml
8)	N-DOCOSANE	13.681	6393960	40.821 ug/ml
10)	N-TETRACOSANE	14.780	6188005	39.703 ug/ml
11)	N-HEXACOSANE	15.798	6036845	39.068 ug/ml
12)	N-OCTACOSANE	16.742	5961646	38.679 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050820\
Data File : FF006896.D
Signal(s) : FID2B.ch
Acq On : 08 May 2020 17:23
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 09 03:25:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

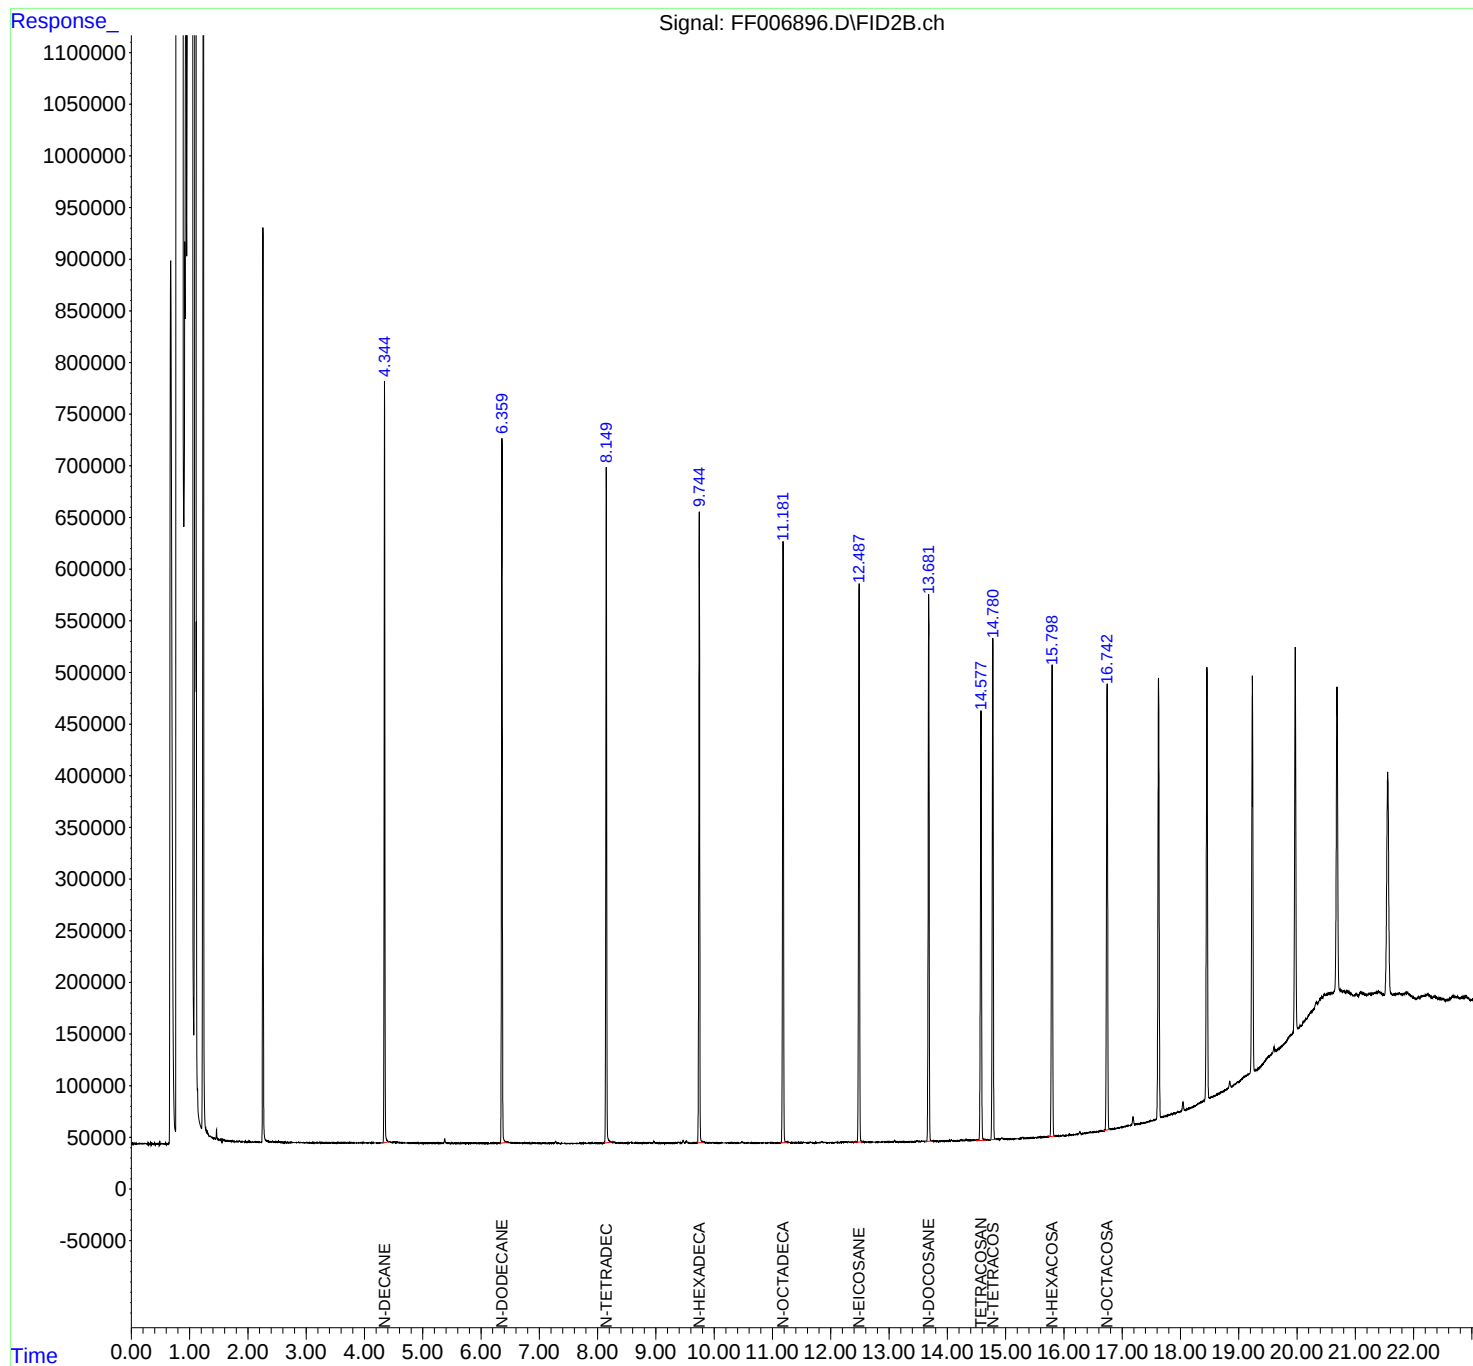

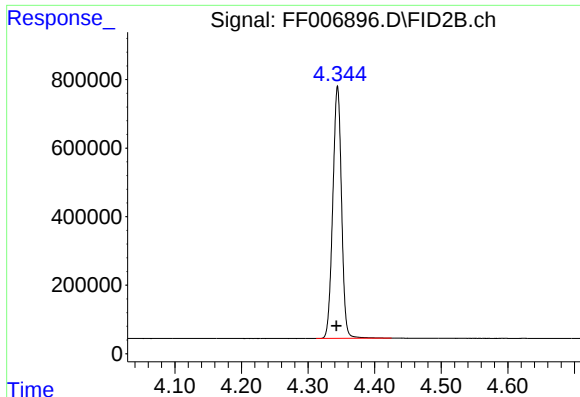


#2 N-DECANE

R.T.: 4.344 min
Delta R.T.: 0.002 min
Response: 6714819
Conc: 48.75 ug/ml

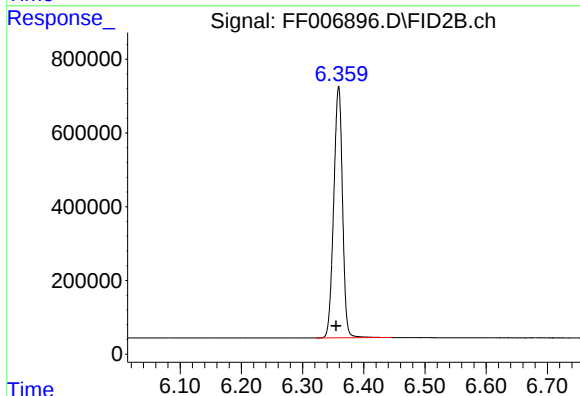


#3 N-DODECANE

R.T.: 6.359 min
Delta R.T.: 0.004 min
Response: 6816861
Conc: 47.81 ug/ml

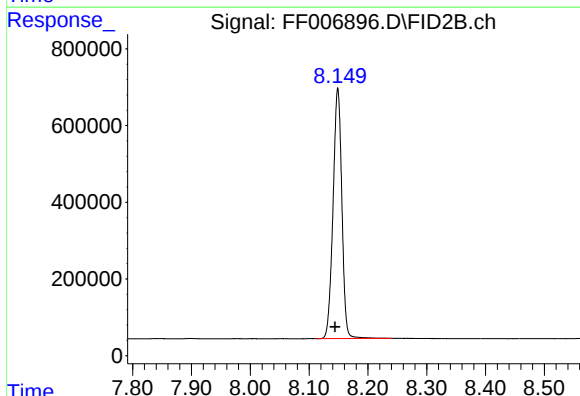


#4 N-TETRADECANE

R.T.: 8.149 min
Delta R.T.: 0.004 min
Response: 6802141
Conc: 46.84 ug/ml

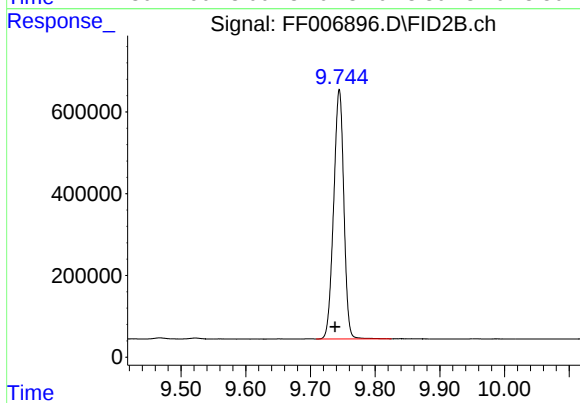


#5 N-HEXADECANE

R.T.: 9.745 min
Delta R.T.: 0.006 min
Response: 6674259
Conc: 45.31 ug/ml

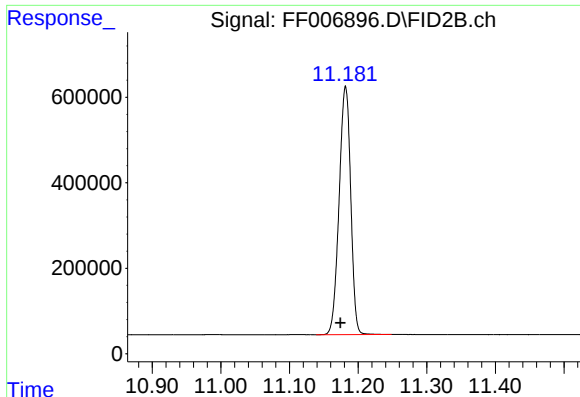


#6 N-OCTADECANE

R.T.: 11.182 min
Delta R.T.: 0.007 min
Response: 6806109
Conc: 43.70 ug/ml

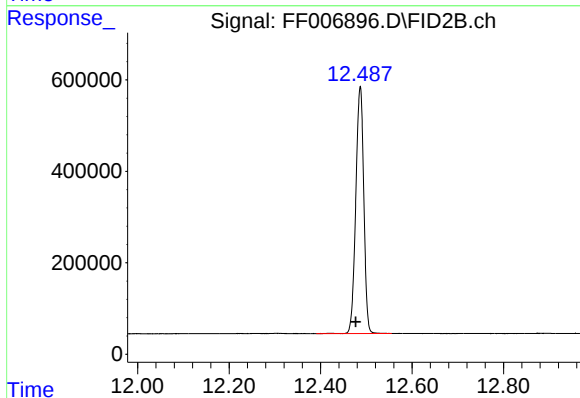


#7 N-EICOSANE

R.T.: 12.487 min
Delta R.T.: 0.010 min
Response: 6530391
Conc: 42.25 ug/ml

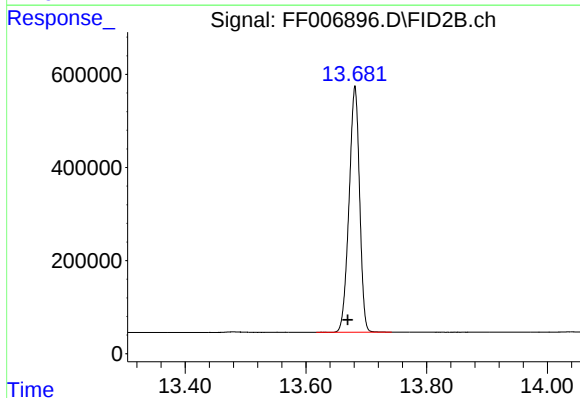


#8 N-DOCOSANE

R.T.: 13.681 min
Delta R.T.: 0.012 min
Response: 6393960
Conc: 40.82 ug/ml

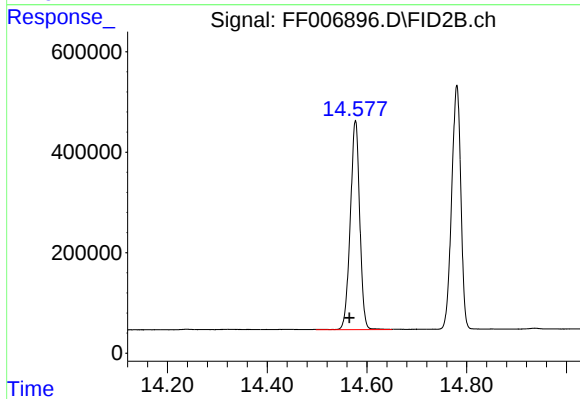


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.577 min
Delta R.T.: 0.012 min
Response: 5460468
Conc: 40.20 ug/ml m

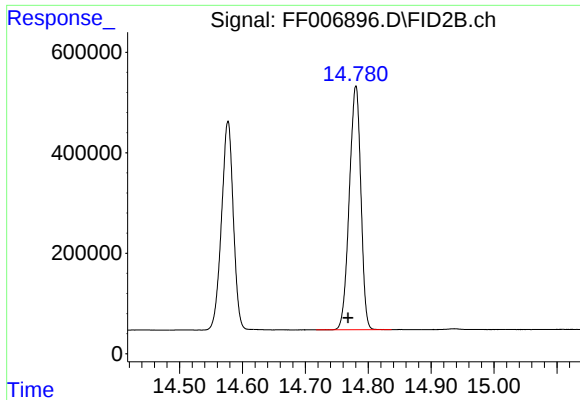


#10 N-TETRACOSANE

R.T.: 14.780 min
Delta R.T.: 0.012 min
Response: 6188005
Conc: 39.70 ug/ml

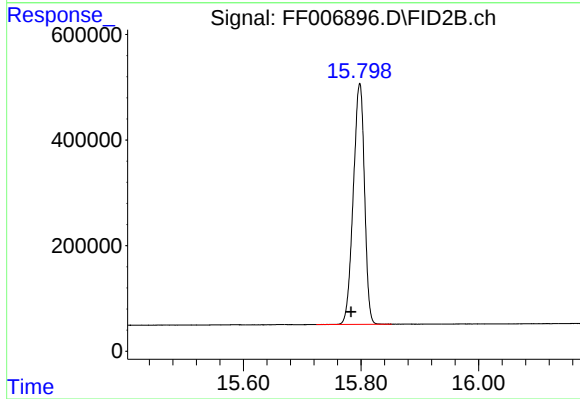

#11 N-HEXACOSANE

R.T.: 15.798 min
Delta R.T.: 0.014 min
Response: 6036845
Conc: 39.07 ug/ml

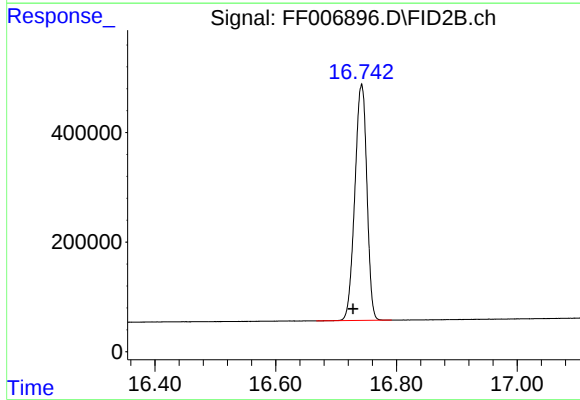

#12 N-OCTACOSANE

R.T.: 16.742 min
Delta R.T.: 0.014 min
Response: 5961646
Conc: 38.68 ug/ml