

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
 Data File : FF014127.D
 Signal(s) : FID2B.ch
 Acq On : 08 May 2024 15:31
 Operator : YP\AJ
 Sample : P2403-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 09 04:34:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:04:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.941	2461913	22.562 ug/ml
Target Compounds			
1) N-OCTANE	1.987	304121	2.713 ug/ml
2) N-DECANE	4.495	247016	2.307 ug/ml
3) N-DODECANE	6.660	174078	1.620 ug/ml
4) N-TETRADECANE	8.493	172589	1.552 ug/ml
5) N-HEXADECANE	10.099	238454	2.066 ug/ml
6) N-OCTADECANE	11.538	278939	2.337 ug/ml
7) N-EICOSANE	12.846	306554	2.417 ug/ml
8) N-DOCOSANE	14.044	337129	2.738 ug/ml
10) N-TETRACOSANE	15.147	348373	2.840 ug/ml
11) N-HEXACOSANE	16.171	331746	2.734 ug/ml
12) N-OCTACOSANE	17.122	328094	2.742 ug/ml
13) N-TRIACONTANE	18.008	343107	2.825 ug/ml
14) N-DOTRIACONTANE	18.842	376906	3.096 ug/ml
15) N-TETRATRIACONTANE	19.624	392041	3.549 ug/ml
16) N-HEXATRIACONTANE	20.367	461486	4.623 ug/ml
17) N-OCTATRIACONTANE	21.096	441264	4.910 ug/ml
18) N-TETRACONTANE	21.993	336506	4.079 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
Data File : FF014127.D
Signal(s) : FID2B.ch
Acq On : 08 May 2024 15:31
Operator : YP\AJ
Sample : P2403-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 04:34:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

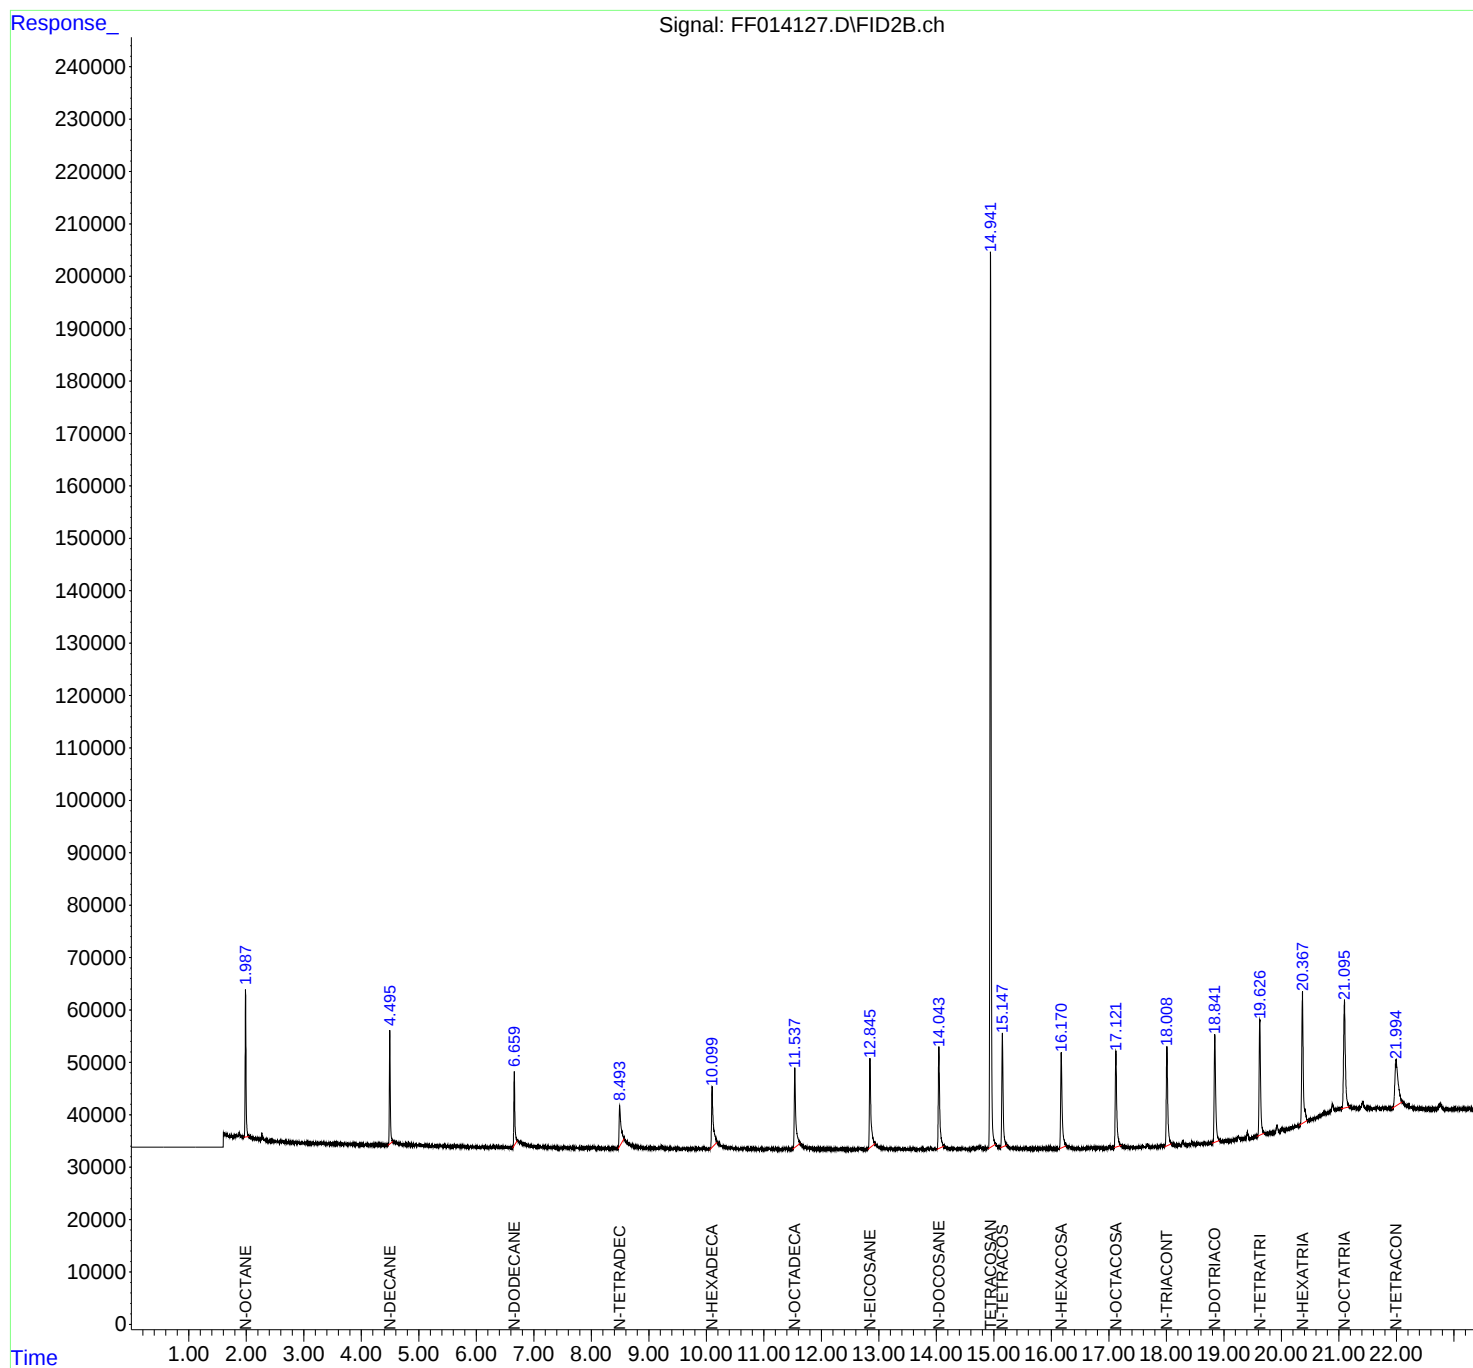


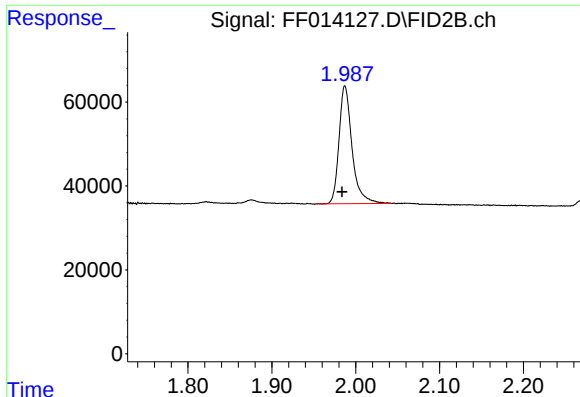

#1 N-OCTANE


R.T.: 1.987 min
Delta R.T.: 0.003 min
Response: 304121
Conc: 2.71 ug/ml

Instrument :
FID_F
ClientSampleId :

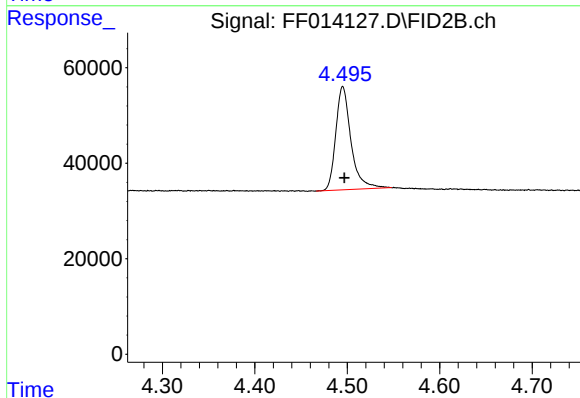


#2 N-DECANE

R.T.: 4.495 min
Delta R.T.: -0.002 min
Response: 247016
Conc: 2.31 ug/ml

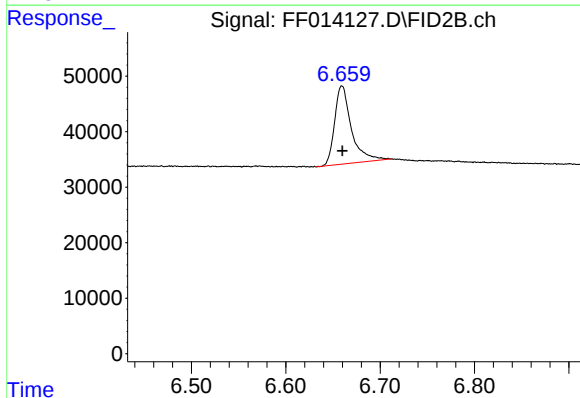


#3 N-DODECANE

R.T.: 6.660 min
Delta R.T.: 0.000 min
Response: 174078
Conc: 1.62 ug/ml

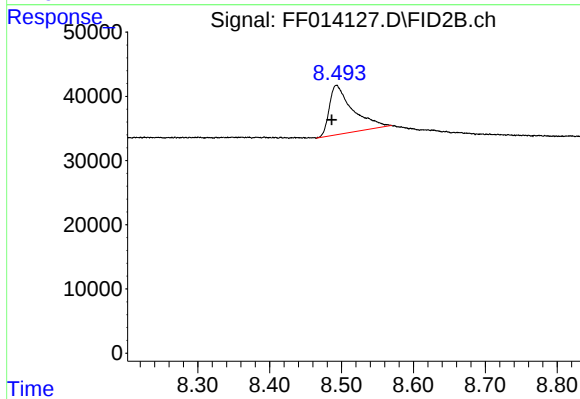

#4 N-TETRADECANE


R.T.: 8.493 min
Delta R.T.: 0.006 min
Response: 172589
Conc: 1.55 ug/ml

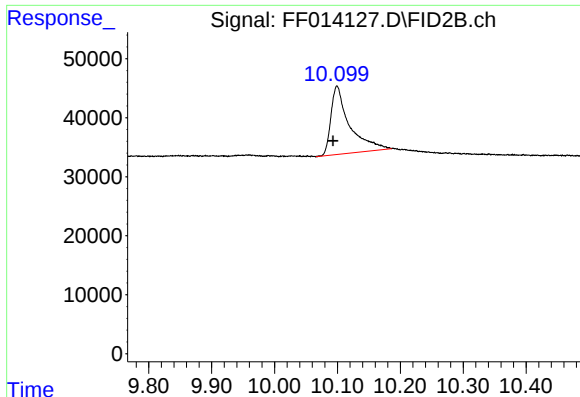

#5 N-HEXADECANE


R.T.: 10.099 min
Delta R.T.: 0.006 min
Response: 238454
Conc: 2.07 ug/ml

Instrument :
FID_F
ClientSampleId :

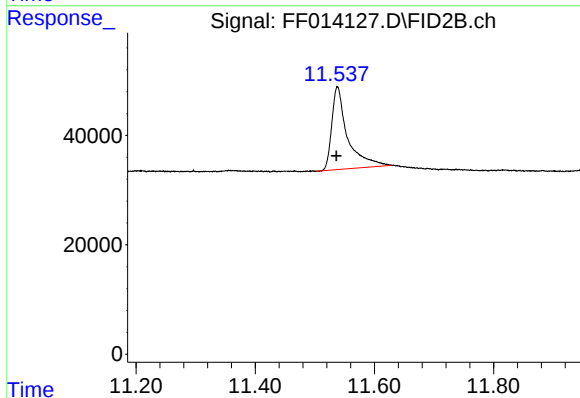


#6 N-OCTADECANE

R.T.: 11.538 min
Delta R.T.: 0.002 min
Response: 278939
Conc: 2.34 ug/ml

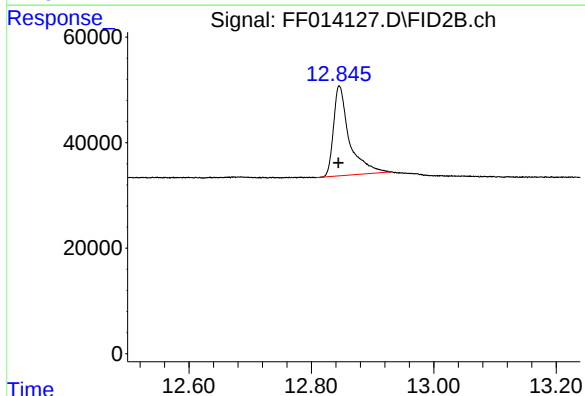


#7 N-EICOSANE

R.T.: 12.846 min
Delta R.T.: 0.001 min
Response: 306554
Conc: 2.42 ug/ml

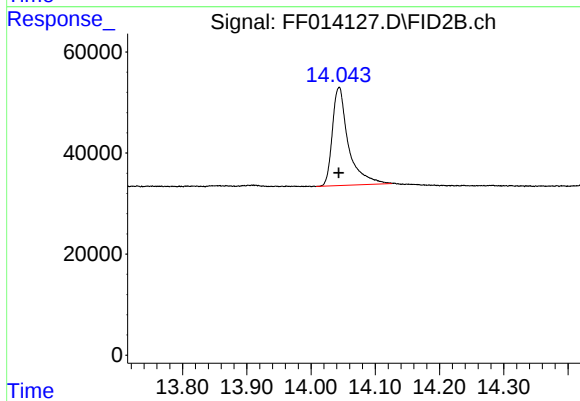

#8 N-DOCOSANE


R.T.: 14.044 min
Delta R.T.: 0.000 min
Response: 337129
Conc: 2.74 ug/ml

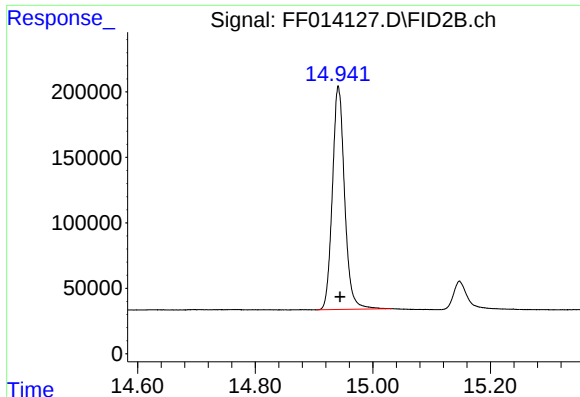

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.941 min
Delta R.T.: -0.003 min
Response: 2461913
Conc: 22.56 ug/ml

Instrument :
FID_F
ClientSampleId :

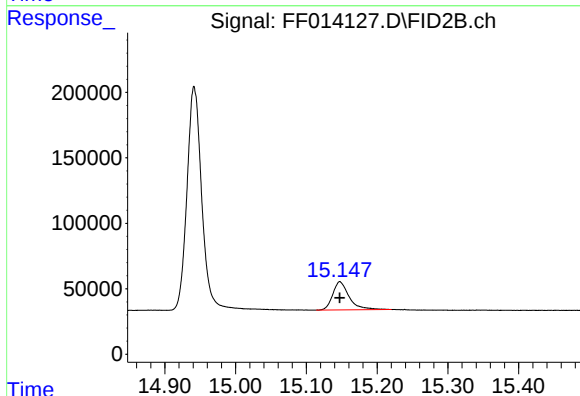


#10 N-TETRACOSANE

R.T.: 15.147 min
Delta R.T.: 0.000 min
Response: 348373
Conc: 2.84 ug/ml

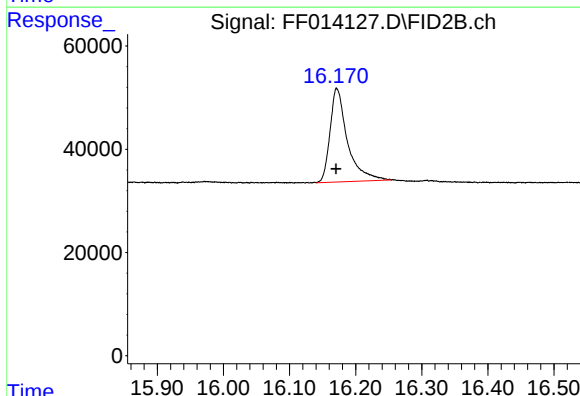


#11 N-HEXACOSANE

R.T.: 16.171 min
Delta R.T.: 0.001 min
Response: 331746
Conc: 2.73 ug/ml

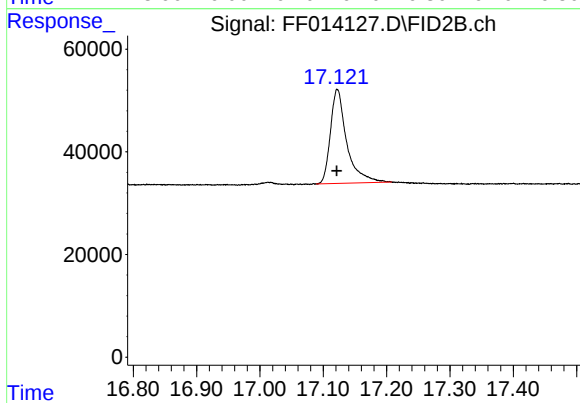

#12 N-OCTACOSANE


R.T.: 17.122 min
Delta R.T.: 0.000 min
Response: 328094
Conc: 2.74 ug/ml

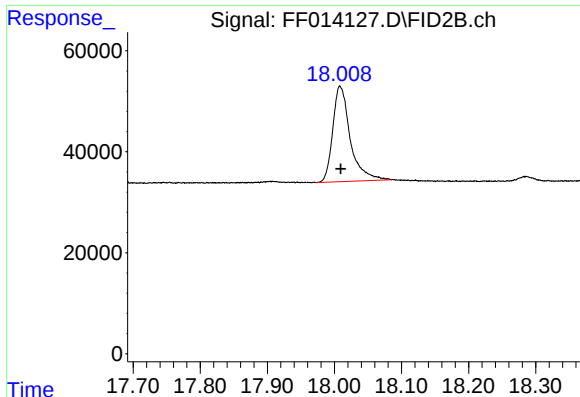

#13 N-TRIACONTANE


R.T.: 18.008 min
Delta R.T.: -0.001 min
Response: 343107
Conc: 2.82 ug/ml

Instrument :
FID_F
ClientSampleId :

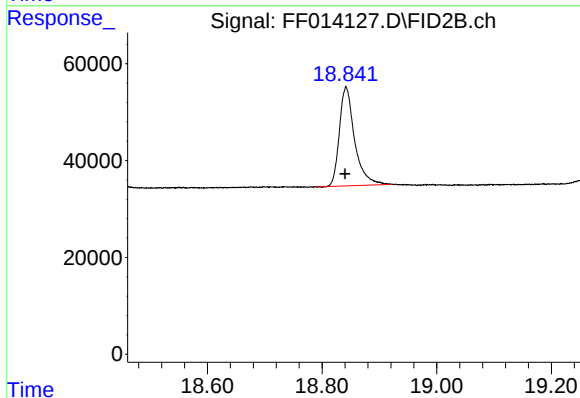


#14 N-DOTRIACONTANE

R.T.: 18.842 min
Delta R.T.: 0.002 min
Response: 376906
Conc: 3.10 ug/ml

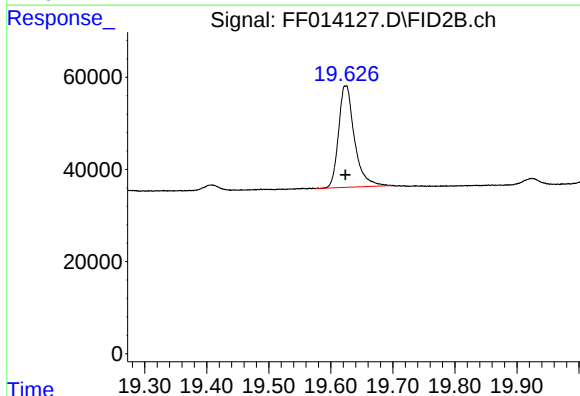


#15 N-TETRATRIACONTANE

R.T.: 19.624 min
Delta R.T.: 0.000 min
Response: 392041
Conc: 3.55 ug/ml

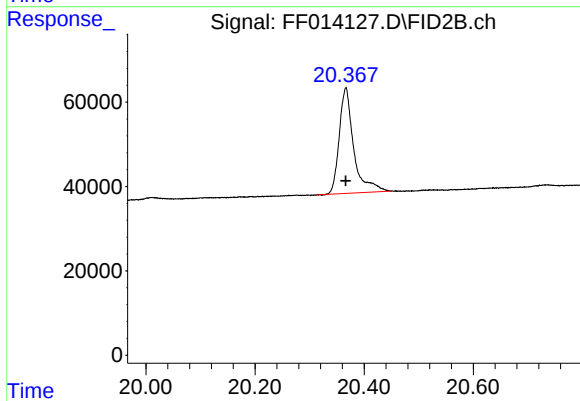

#16 N-HEXATRIACONTANE


R.T.: 20.367 min
Delta R.T.: 0.000 min
Response: 461486
Conc: 4.62 ug/ml

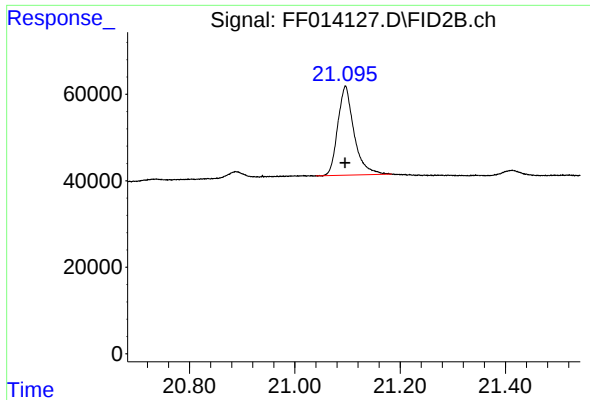

#17 N-OCTATRIACONTANE

R.T.: 21.096 min
Delta R.T.: 0.000 min
Response: 441264
Conc: 4.91 ug/ml

Instrument :
FID_F
ClientSampleId :

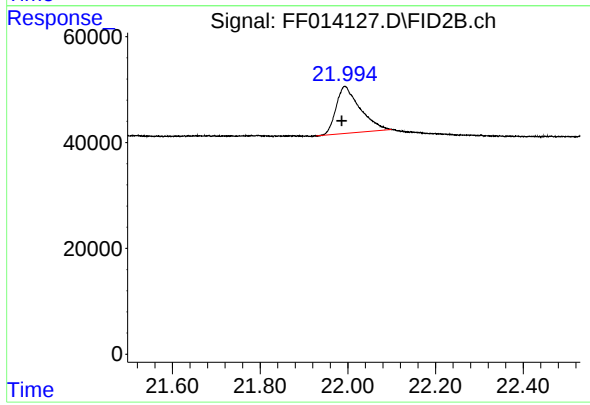

#18 N-TETRACONTANE

R.T.: 21.993 min
Delta R.T.: 0.007 min
Response: 336506
Conc: 4.08 ug/ml