

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
Data File : FF014138.D
Signal(s) : FID2B.ch
Acq On : 08 May 2024 21:29
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 04:36:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.656	1934437	18.008 ug/ml
12)	N-OCTACOSANE	17.117	2286999	19.117 ug/ml
14)	N-DOTRIACONTANE	18.846	75872	0.623 ug/ml
15)	N-TETRATRIACONTANE	19.626	63691	0.577 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
Data File : FF014138.D
Signal(s) : FID2B.ch
Acq On : 08 May 2024 21:29
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 09 04:36:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

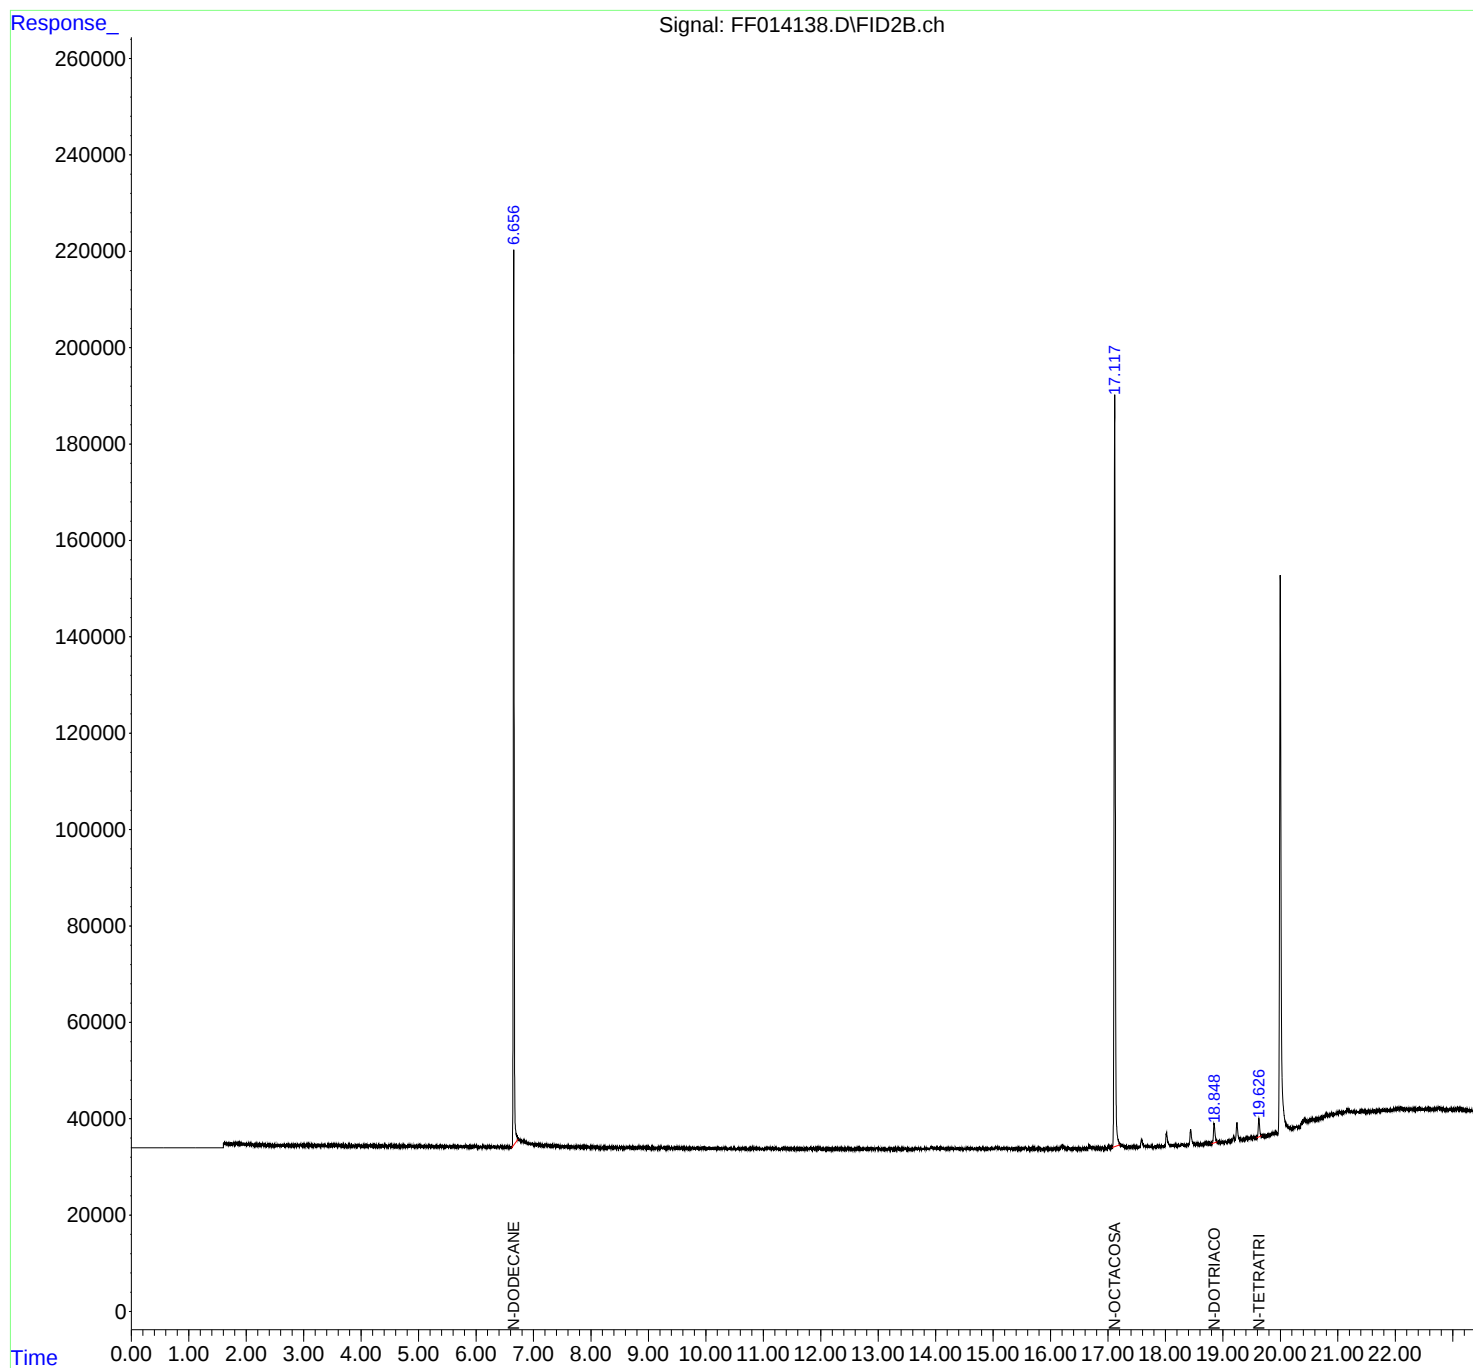


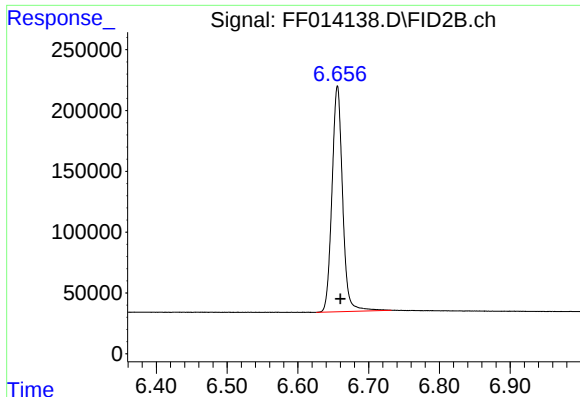

#3 N-DODECANE


R.T.: 6.656 min
Delta R.T.: -0.004 min
Response: 1934437
Conc: 18.01 ug/ml

Instrument :
FID_F
ClientSampleId :

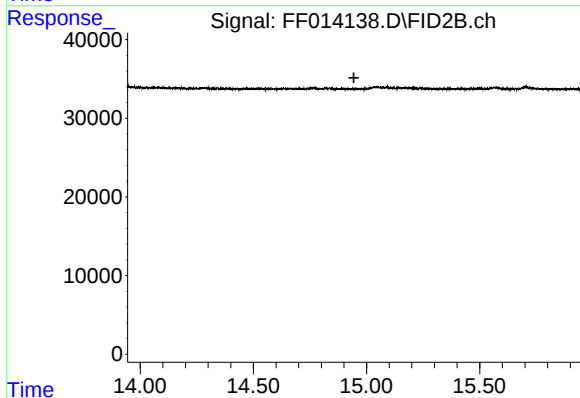


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.944 min
Response: 0
Conc: N.D.

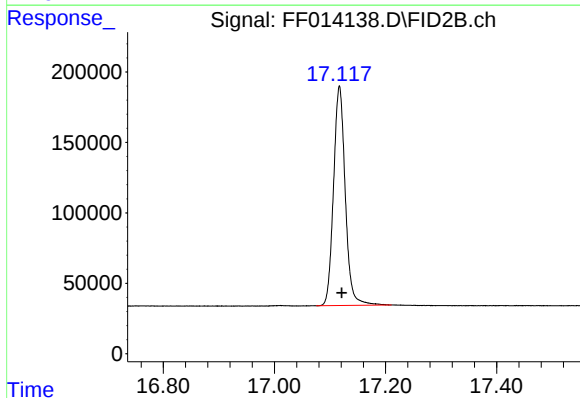


#12 N-OCTACOSANE

R.T.: 17.117 min
Delta R.T.: -0.004 min
Response: 2286999
Conc: 19.12 ug/ml

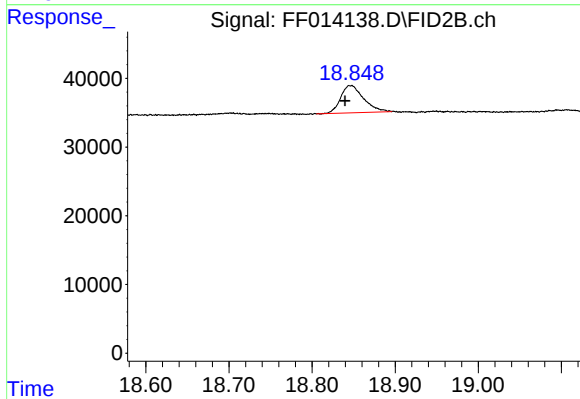

#14 N-DOTRIACONTANE

R.T.: 18.846 min
Delta R.T.: 0.006 min
Response: 75872
Conc: 0.62 ug/ml

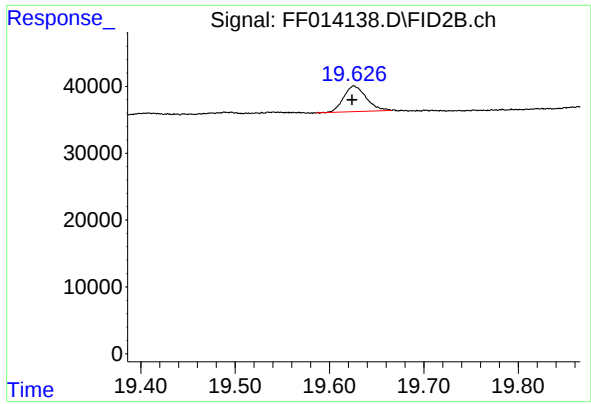

#15 N-TETRATRIACONTANE

R.T.: 19.626 min

Delta R.T.: 0.002 min

Response: 63691

Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :