

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
 Data File : FF014122.D
 Signal(s) : FID2B.ch
 Acq On : 08 May 2024 13:02
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: May 09 04:33:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
 Quant Title :
 QLast Update : Thu Apr 11 13:04:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.942	5898827	54.060 ug/ml
Target Compounds			
2) N-DECANE	4.492	5879325	54.918 ug/ml
3) N-DODECANE	6.657	6111494	56.892 ug/ml
4) N-TETRADECANE	8.483	6118597	55.021 ug/ml
5) N-HEXADECANE	10.090	6280871	54.409 ug/ml
6) N-OCTADECANE	11.533	6546682	54.850 ug/ml
7) N-EICOSANE	12.843	6499653	51.254 ug/ml
8) N-DOCOSANE	14.042	6450787	52.392 ug/ml
10) N-TETRACOSANE	15.146	6430263	52.429 ug/ml
11) N-HEXACOSANE	16.168	6314076	52.034 ug/ml
12) N-OCTACOSANE	17.118	6224430	52.029 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050824\
Data File : FF014122.D
Signal(s) : FID2B.ch
Acq On : 08 May 2024 13:02
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: May 09 04:33:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041124.M
Quant Title :
QLast Update : Thu Apr 11 13:04:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

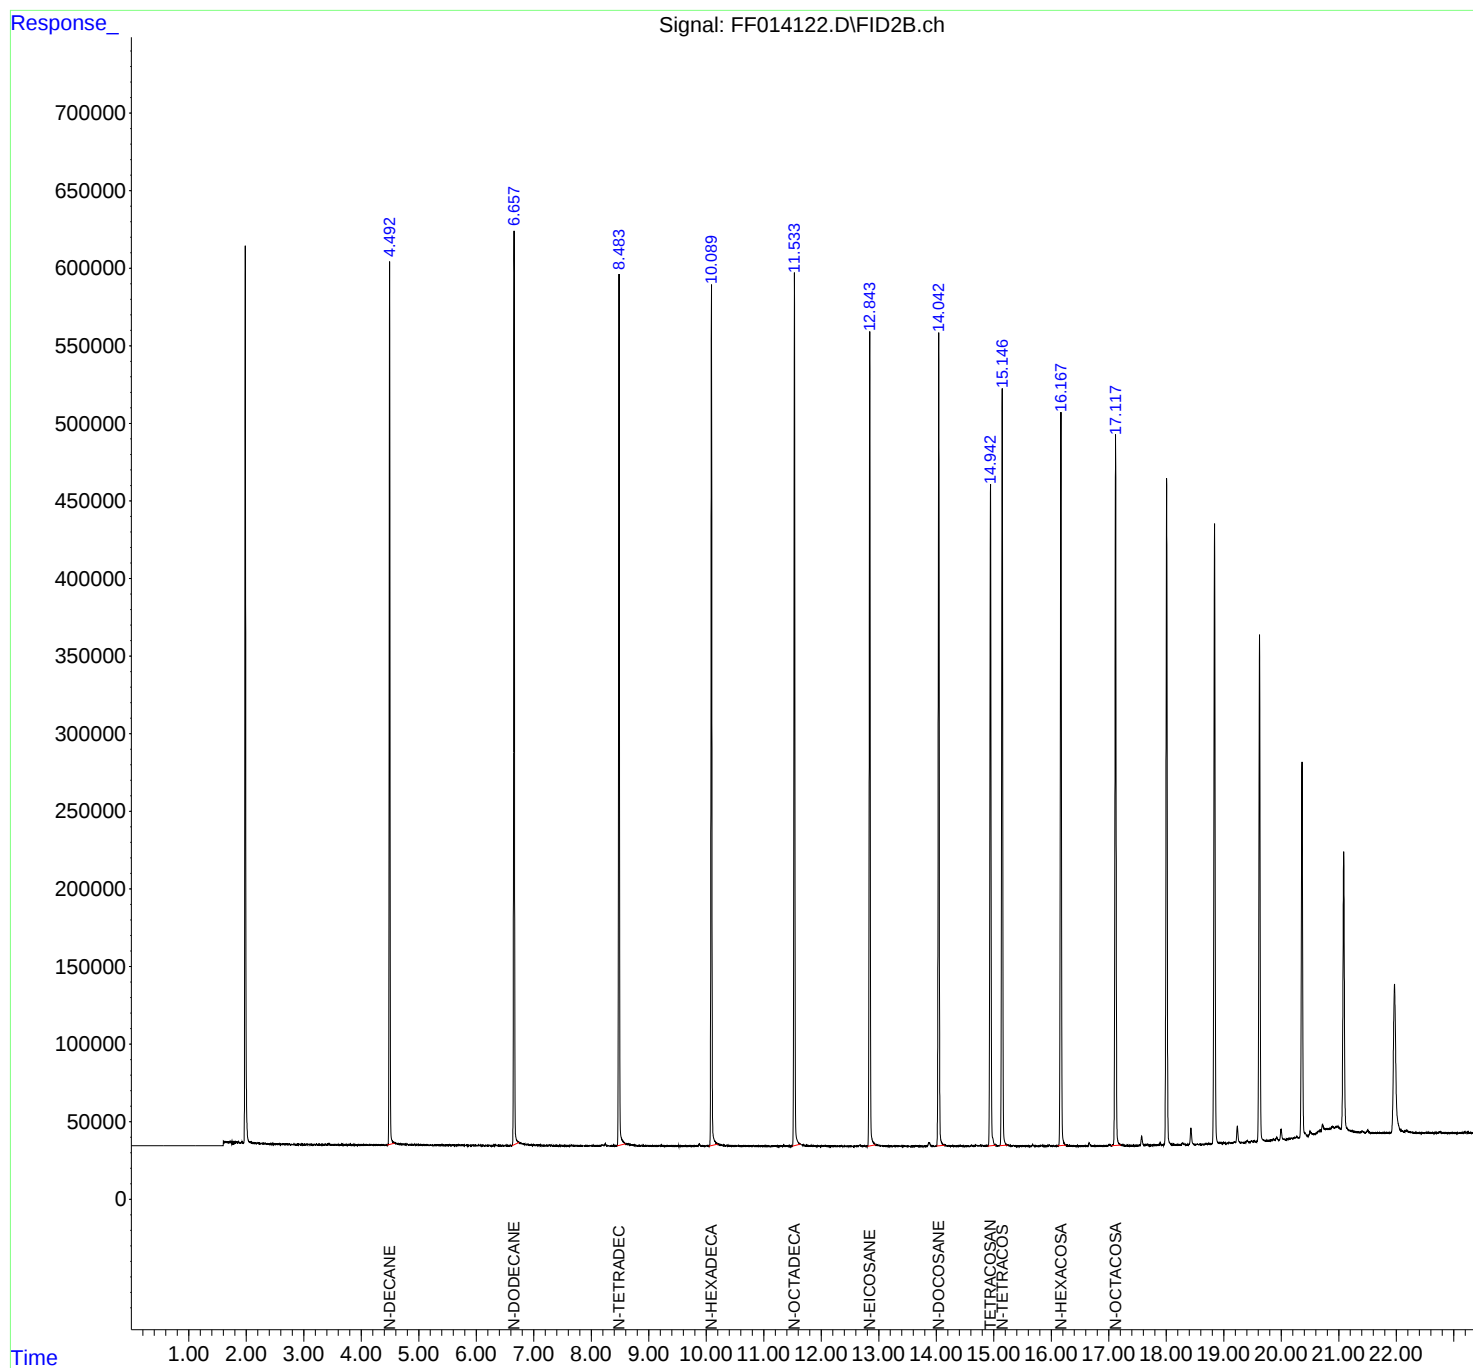


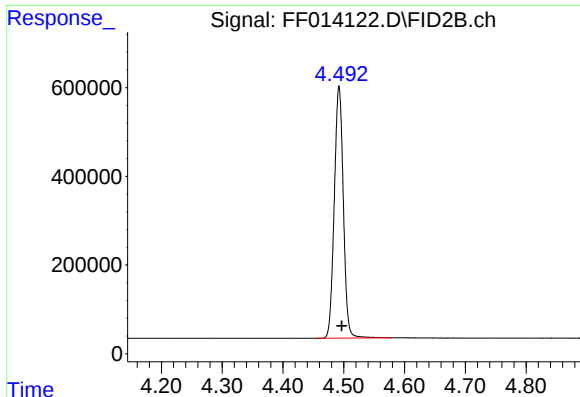

#2 N-DECANE


R.T.: 4.492 min
Delta R.T.: -0.004 min
Response: 5879325
Conc: 54.92 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

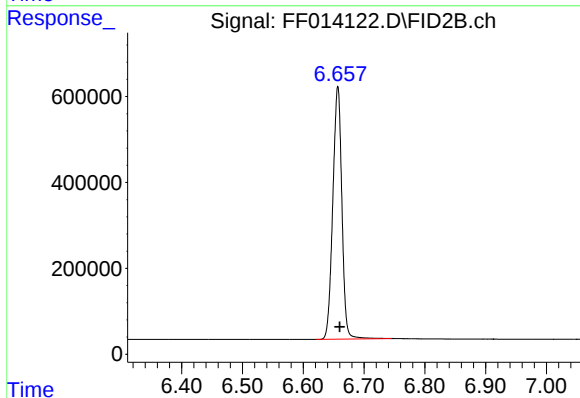


#3 N-DODECANE

R.T.: 6.657 min
Delta R.T.: -0.003 min
Response: 6111494
Conc: 56.89 ug/ml

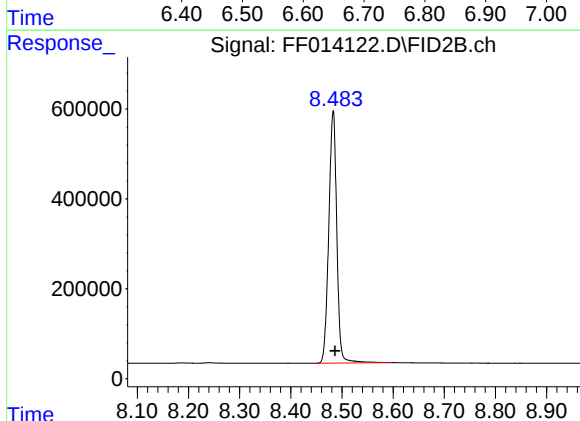


#4 N-TETRADECANE

R.T.: 8.483 min
Delta R.T.: -0.004 min
Response: 6118597
Conc: 55.02 ug/ml

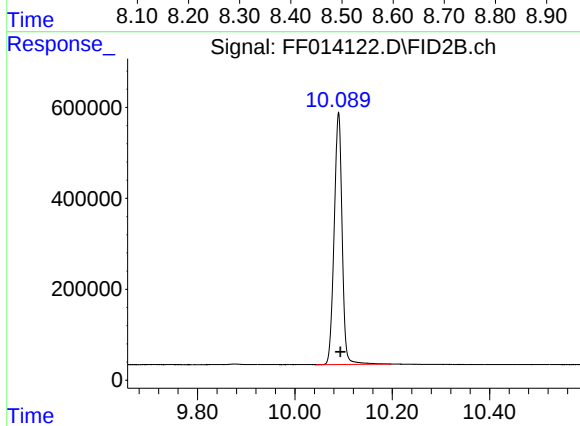

#5 N-HEXADECANE


R.T.: 10.090 min
Delta R.T.: -0.004 min
Response: 6280871
Conc: 54.41 ug/ml

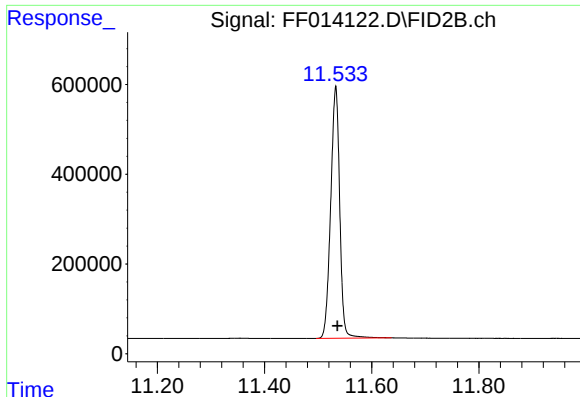

#6 N-OCTADECANE


R.T.: 11.533 min
Delta R.T.: -0.003 min
Response: 6546682
Conc: 54.85 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

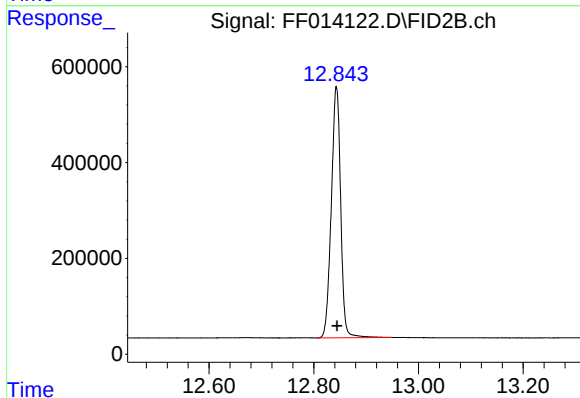


#7 N-EICOSANE

R.T.: 12.843 min
Delta R.T.: 0.000 min
Response: 6499653
Conc: 51.25 ug/ml

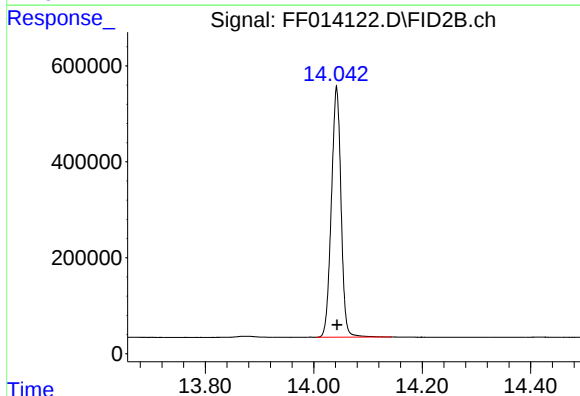


#8 N-DOCOSANE

R.T.: 14.042 min
Delta R.T.: -0.001 min
Response: 6450787
Conc: 52.39 ug/ml

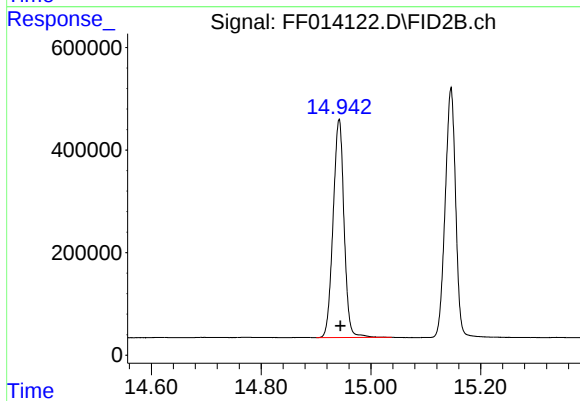

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.942 min
Delta R.T.: -0.002 min
Response: 5898827
Conc: 54.06 ug/ml

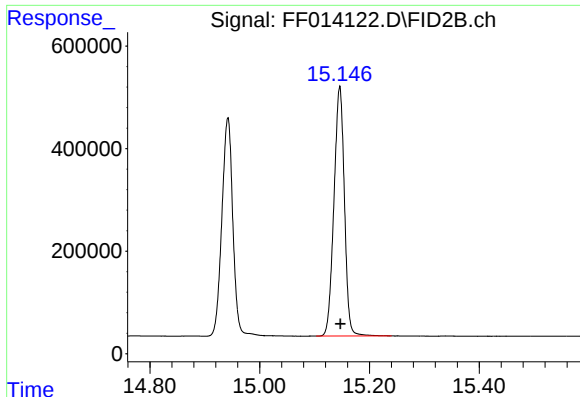


#10 N-TETRACOSANE

R.T.: 15.146 min
Delta R.T.: -0.001 min
Response: 6430263
Conc: 52.43 ug/ml

Instrument :


FID_F

ClientSampleId :
50 PPM TRPH STD

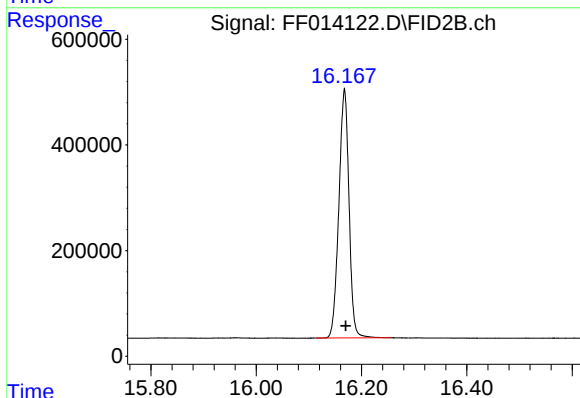

#11 N-HEXACOSANE

R.T.: 16.168 min
Delta R.T.: -0.002 min
Response: 6314076
Conc: 52.03 ug/ml

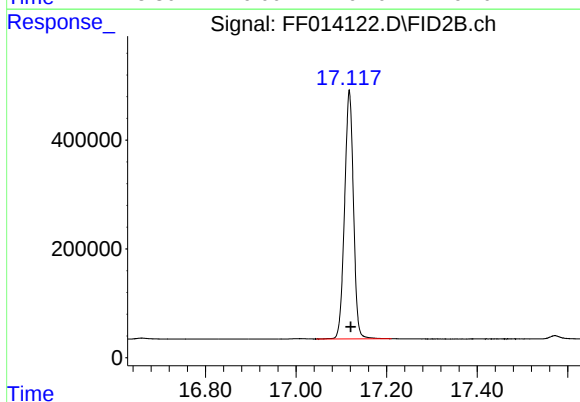

#12 N-OCTACOSANE

R.T.: 17.118 min
Delta R.T.: -0.004 min
Response: 6224430
Conc: 52.03 ug/ml