

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050922\
 Data File : FF010580.D
 Signal(s) : FID2B.ch
 Acq On : 09 May 2022 08:59
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 10 01:26:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	78753	0.642 ug/ml
Target Compounds			
7) N-EICOSANE	12.494	170841	1.220 ug/ml
8) N-DOCOSANE	13.698	869610	6.261 ug/ml
10) N-TETRACOSANE	14.784	9172190	66.388 ug/ml
11) N-HEXACOSANE	15.831	356199	2.632 ug/ml
12) N-OCTACOSANE	16.780	217269	1.652 ug/ml
13) N-TRIACONTANE	17.667	906593	7.133 ug/ml
14) N-DOTRIACONTANE	18.499	1523450	12.701 ug/ml
15) N-TETRATRIACONTANE	19.277	384234	3.620 ug/ml
17) N-OCTATRIACONTANE	20.728	917295	11.381 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050922\
Data File : FF010580.D
Signal(s) : FID2B.ch
Acq On : 09 May 2022 08:59
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 01:26:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

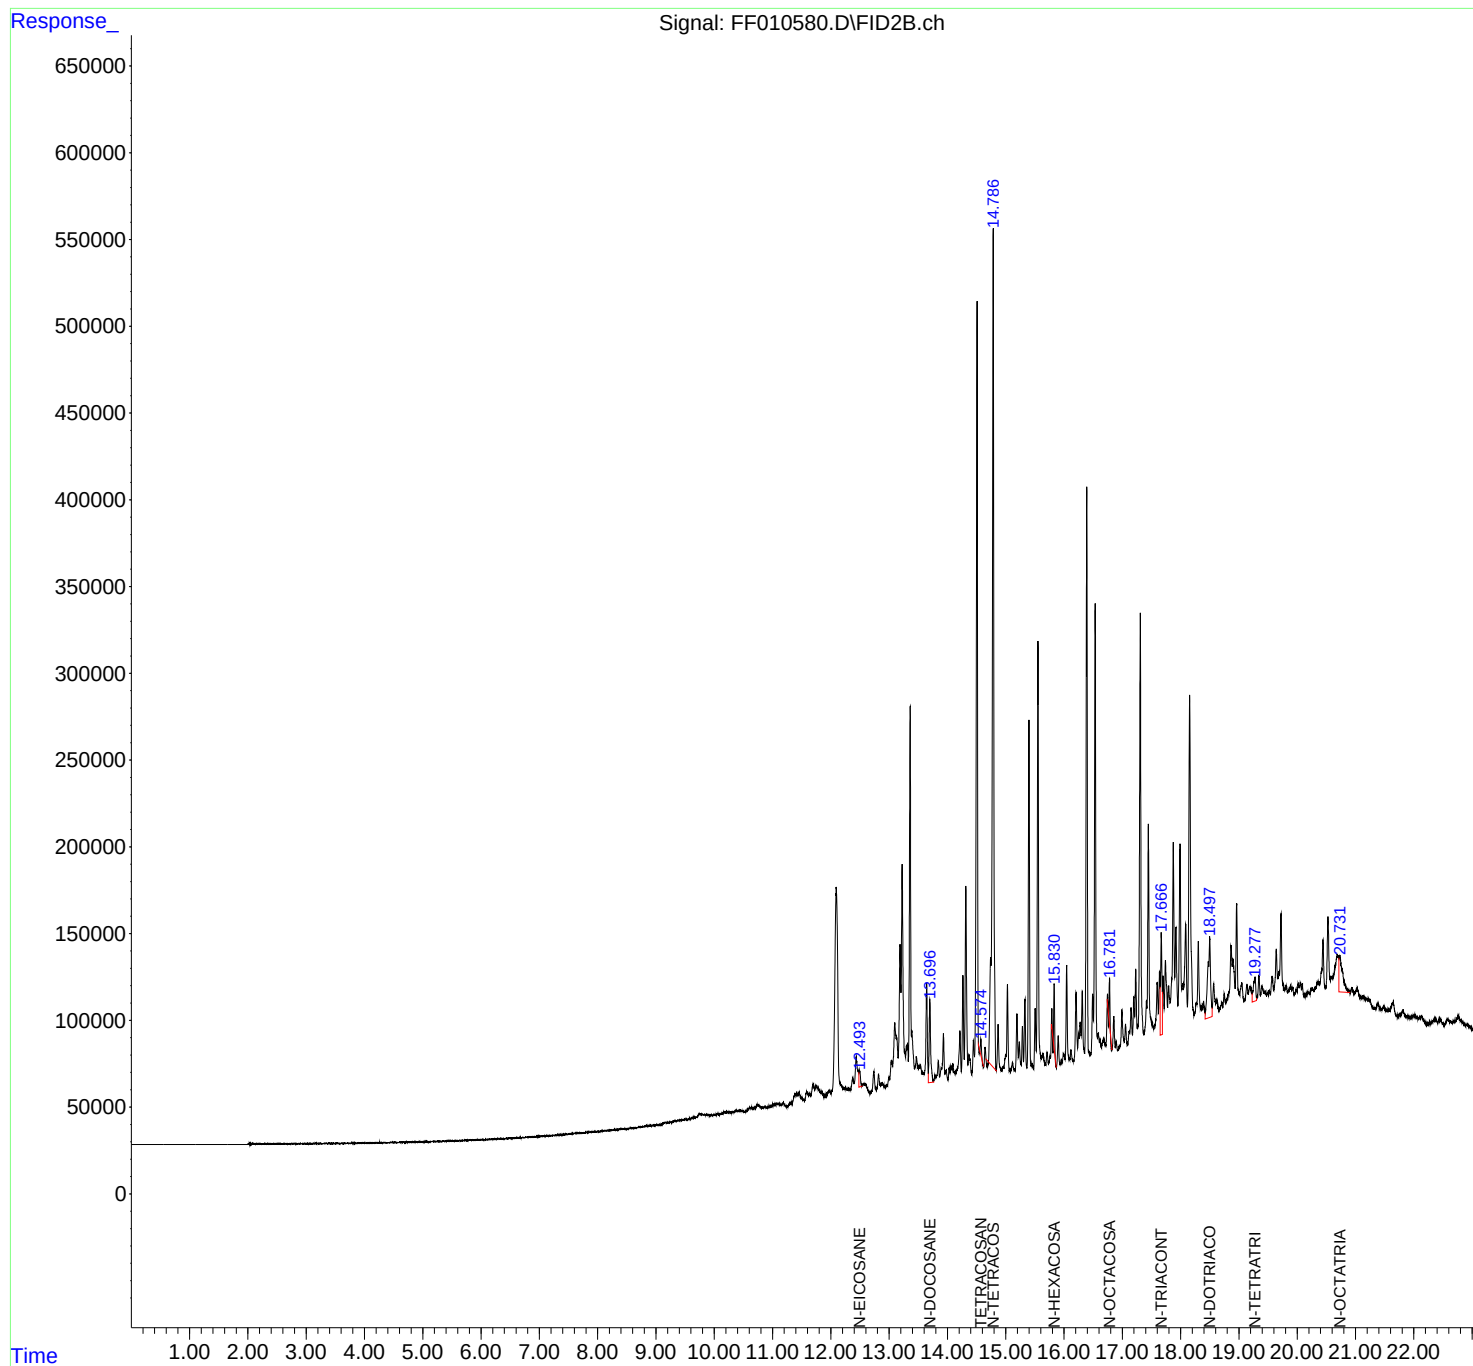


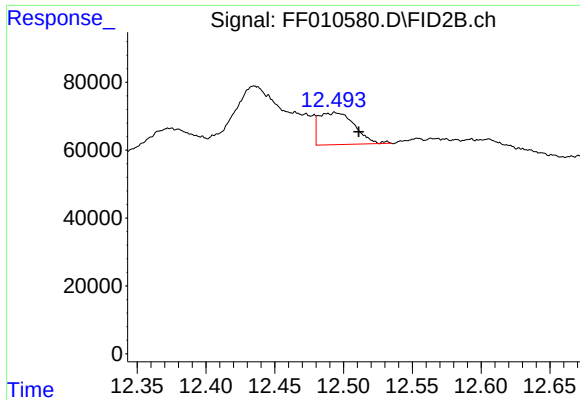

#7 N-EICOSANE


R.T.: 12.494 min
Delta R.T.: -0.017 min
Response: 170841
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :

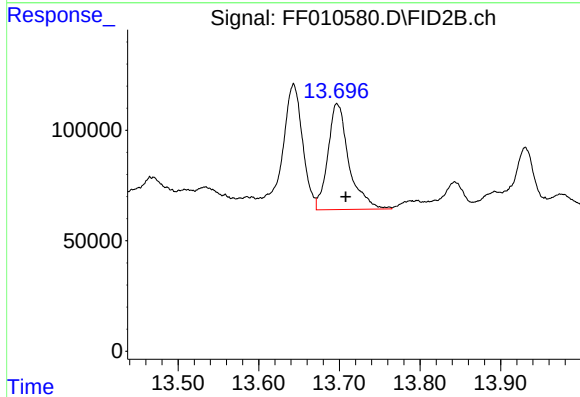


#8 N-DOCOSANE

R.T.: 13.698 min
Delta R.T.: -0.010 min
Response: 869610
Conc: 6.26 ug/ml

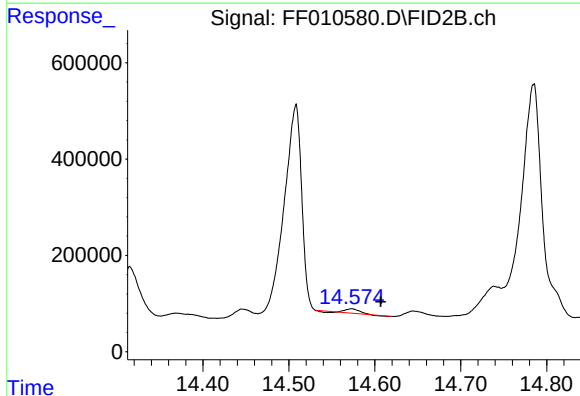


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.573 min
Delta R.T.: -0.034 min
Response: 78753
Conc: 0.64 ug/ml

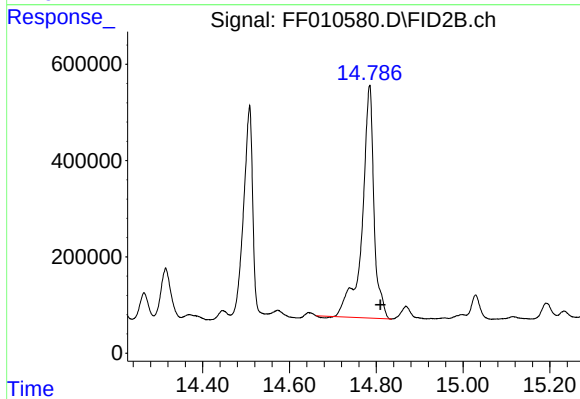

#10 N-TETRACOSANE


R.T.: 14.784 min
Delta R.T.: -0.025 min
Response: 9172190
Conc: 66.39 ug/ml

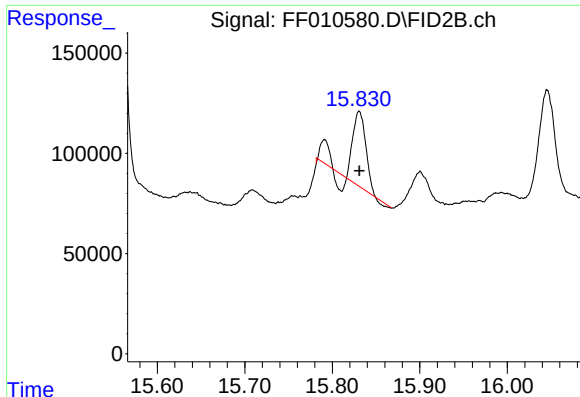

#11 N-HEXACOSANE


R.T.: 15.831 min
Delta R.T.: 0.000 min
Response: 356199
Conc: 2.63 ug/ml

Instrument :
FID_F
ClientSampleId :

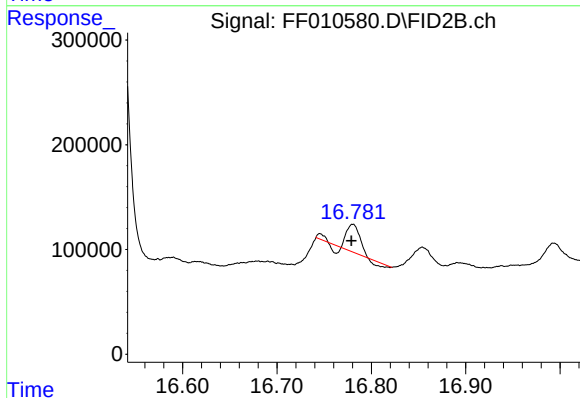


#12 N-OCTACOSANE

R.T.: 16.780 min
Delta R.T.: 0.001 min
Response: 217269
Conc: 1.65 ug/ml

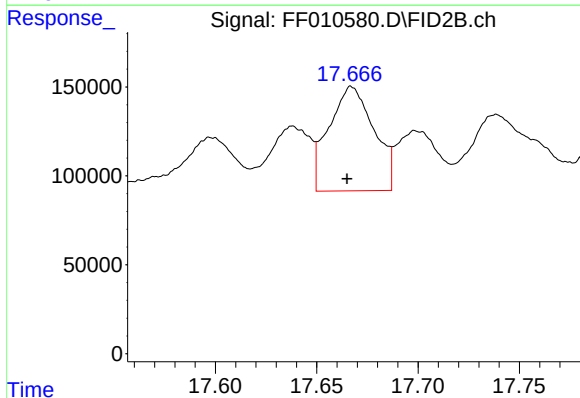


#13 N-TRIACONTANE

R.T.: 17.667 min
Delta R.T.: 0.002 min
Response: 906593
Conc: 7.13 ug/ml

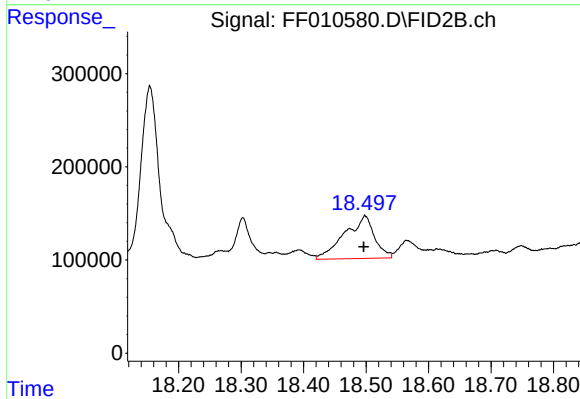

#14 N-DOTRIACONTANE


R.T.: 18.499 min
Delta R.T.: 0.003 min
Response: 1523450
Conc: 12.70 ug/ml

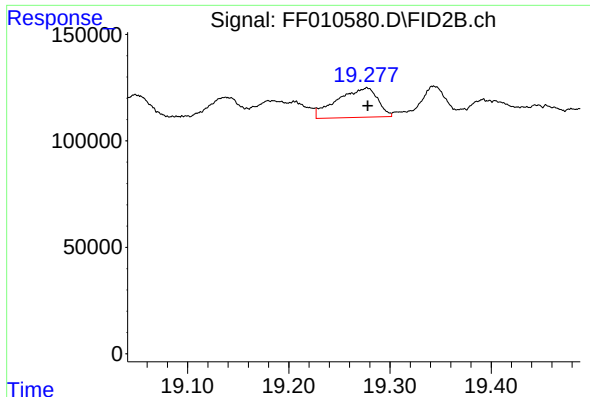

#15 N-TETRATRIACONTANE

R.T.: 19.277 min
Delta R.T.: -0.001 min
Response: 384234
Conc: 3.62 ug/ml

Instrument :
FID_F
ClientSampleId :

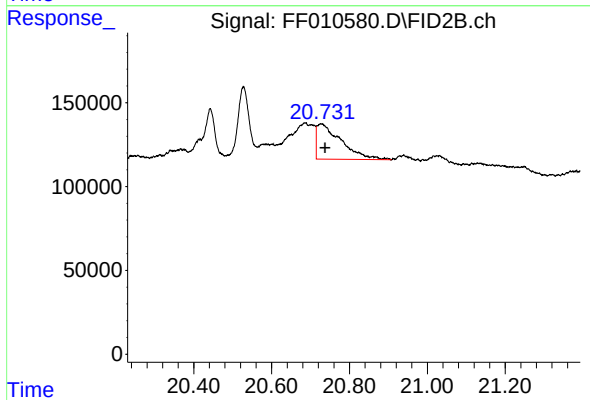

#17 N-OCTATRIACONTANE

R.T.: 20.728 min
Delta R.T.: -0.009 min
Response: 917295
Conc: 11.38 ug/ml