

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050922\
 Data File : FF010584.D
 Signal(s) : FID2B.ch
 Acq On : 09 May 2022 12:39
 Operator : AJ\MA
 Sample : N2706-01 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 10 01:27:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
 Quant Title :
 QLast Update : Fri Apr 29 04:08:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.605	5354671	43.662 ug/ml
Target Compounds			
6) N-OCTADECANE	11.172	274308	1.910 ug/ml
7) N-EICOSANE	12.515	538891	3.847 ug/ml
8) N-DOCOSANE	13.707	305588	2.200 ug/ml
10) N-TETRACOSANE	14.770	11501900	83.250 ug/ml
11) N-HEXACOSANE	15.833	583111	4.309 ug/ml
12) N-OCTACOSANE	16.785	743019	5.650 ug/ml
13) N-TRIACONTANE	17.671	2100316	16.525 ug/ml
14) N-DOTRIACONTANE	18.492	4341603	36.197 ug/ml
15) N-TETRATRIACONTANE	19.259	1779002	16.763 ug/ml
17) N-OCTATRIACONTANE	20.733	682130	8.463 ug/ml
18) N-TETRACONTANE	21.633	601322	7.639 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF050922\
Data File : FF010584.D
Signal(s) : FID2B.ch
Acq On : 09 May 2022 12:39
Operator : AJ\MA
Sample : N2706-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 10 01:27:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042922.M
Quant Title :
QLast Update : Fri Apr 29 04:08:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

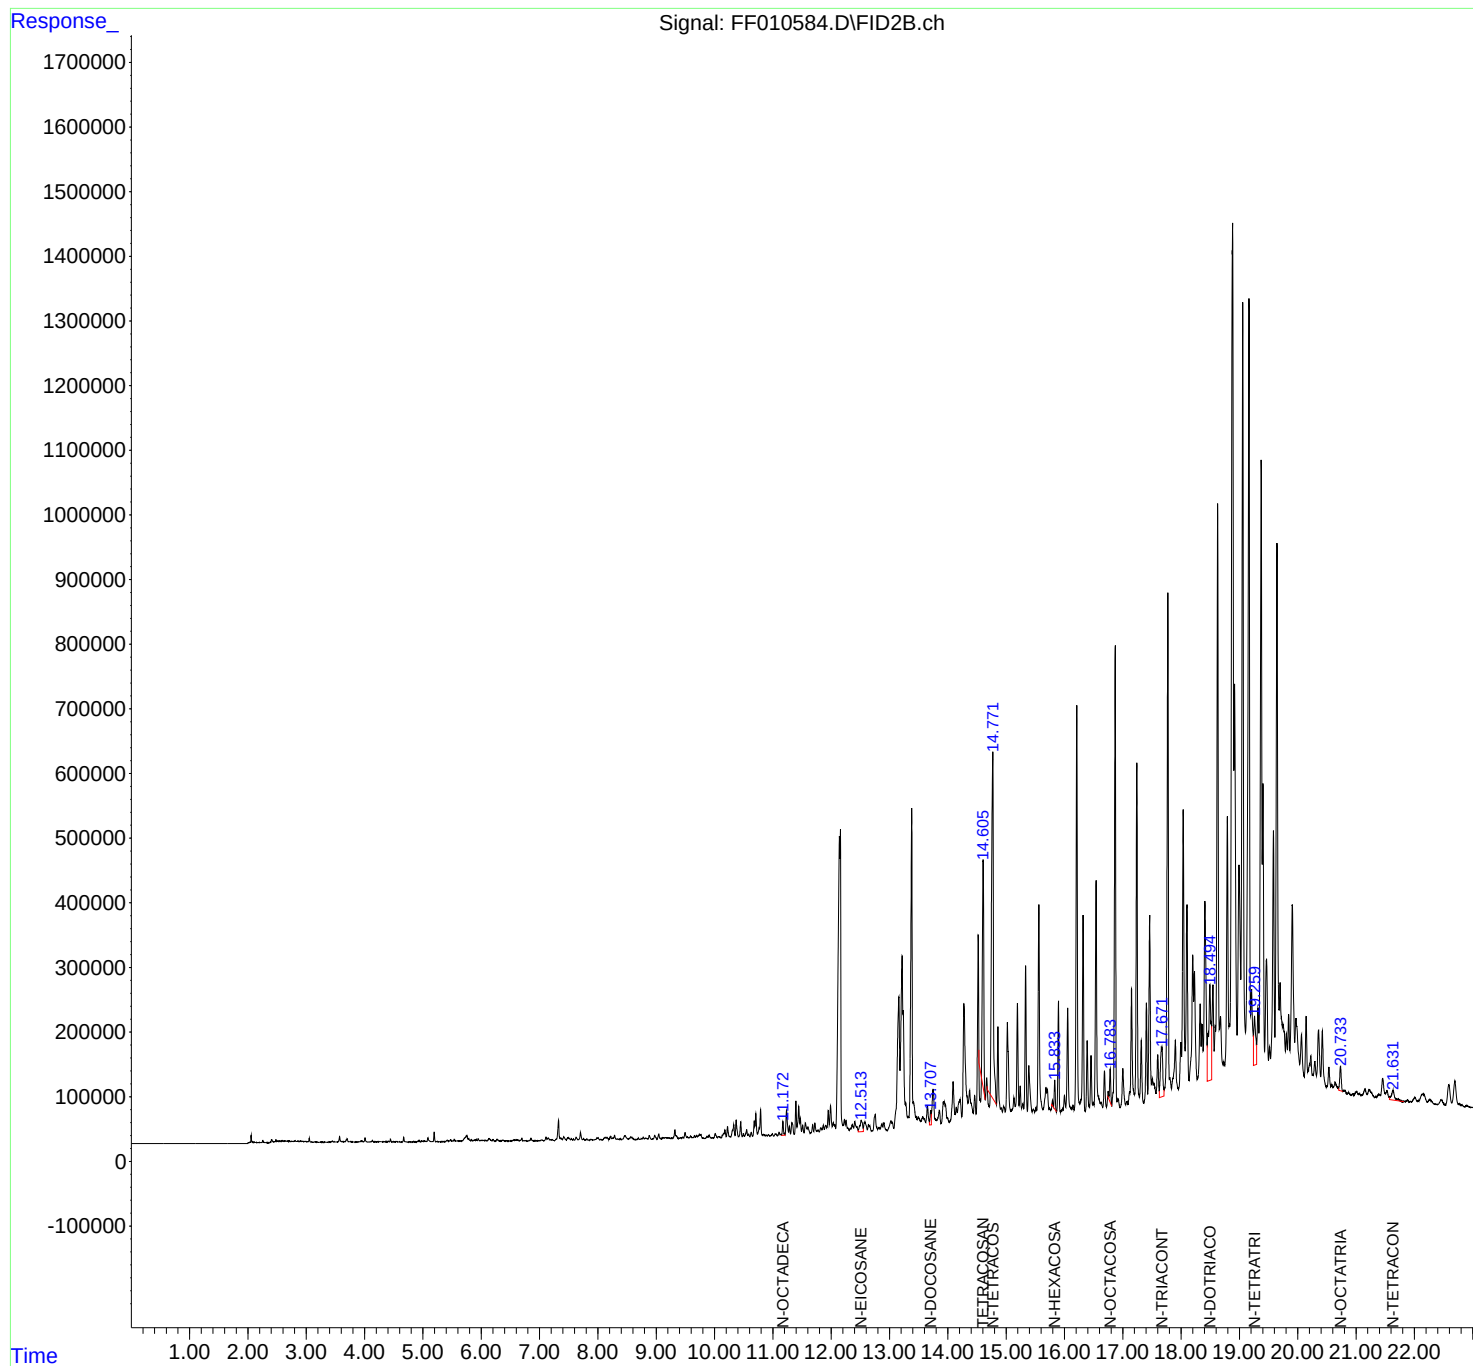


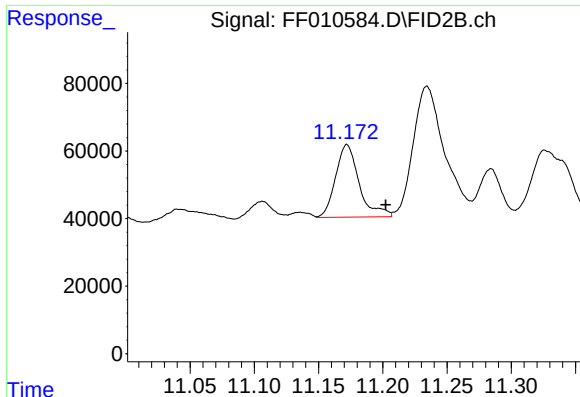

#6 N-OCTADECANE


R.T.: 11.172 min
Delta R.T.: -0.030 min
Response: 274308
Conc: 1.91 ug/ml

Instrument :
FID_F
ClientSampleId :

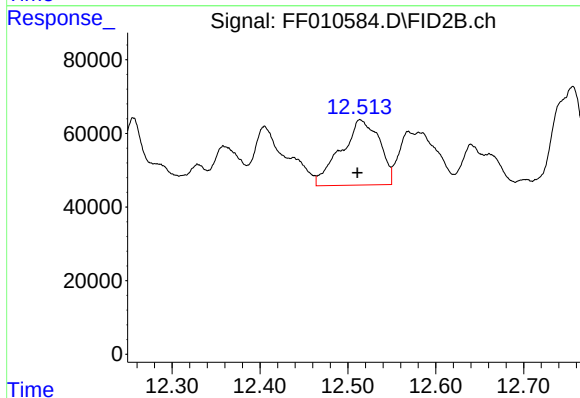


#7 N-EICOSANE

R.T.: 12.515 min
Delta R.T.: 0.004 min
Response: 538891
Conc: 3.85 ug/ml

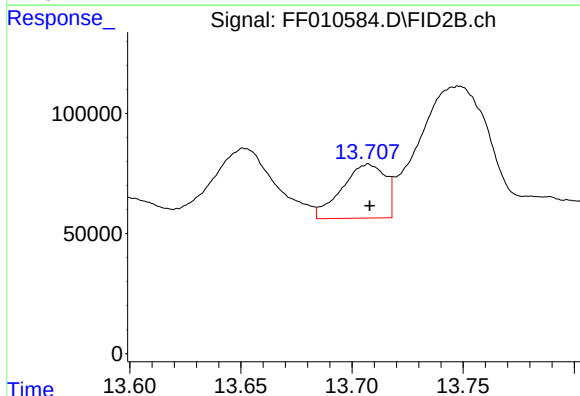


#8 N-DOCOSANE

R.T.: 13.707 min
Delta R.T.: 0.000 min
Response: 305588
Conc: 2.20 ug/ml

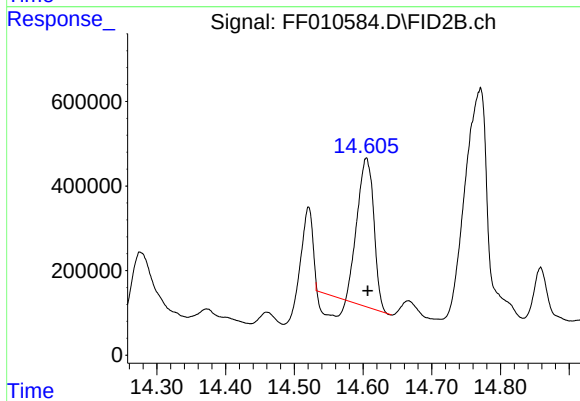

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.605 min
Delta R.T.: -0.002 min
Response: 5354671
Conc: 43.66 ug/ml

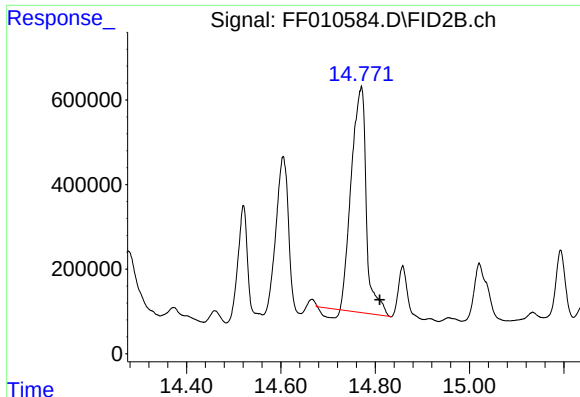

#10 N-TETRACOSANE


R.T.: 14.770 min
Delta R.T.: -0.040 min
Response: 11501900
Conc: 83.25 ug/ml

Instrument :
FID_F
ClientSampleId :

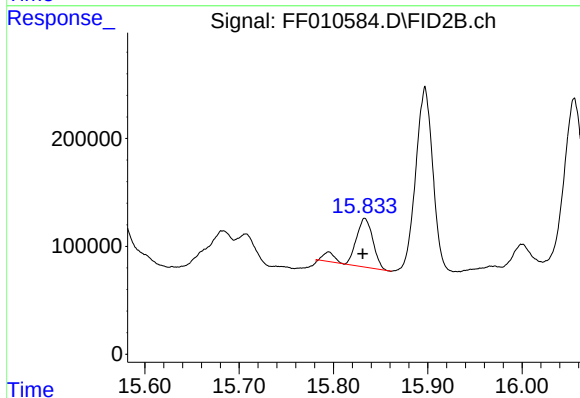


#11 N-HEXACOSANE

R.T.: 15.833 min
Delta R.T.: 0.002 min
Response: 583111
Conc: 4.31 ug/ml

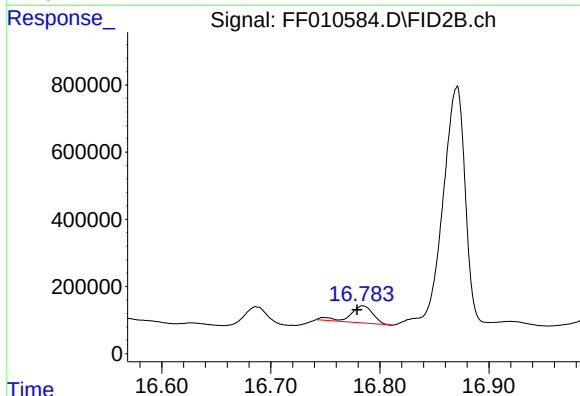


#12 N-OCTACOSANE

R.T.: 16.785 min
Delta R.T.: 0.006 min
Response: 743019
Conc: 5.65 ug/ml

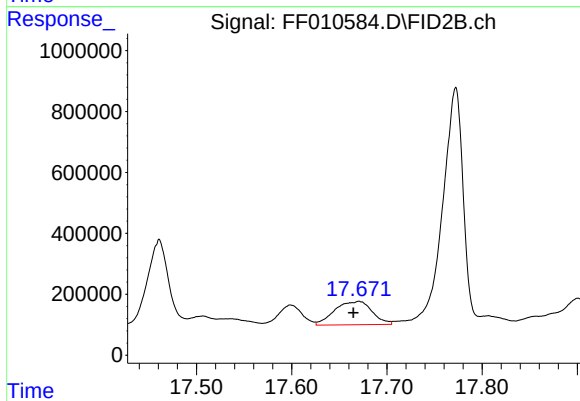

#13 N-TRIACONTANE


R.T.: 17.671 min
Delta R.T.: 0.006 min
Response: 2100316
Conc: 16.52 ug/ml

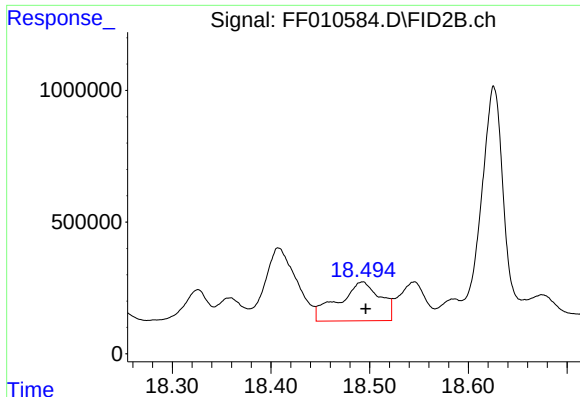

#14 N-DOTRIACONTANE


R.T.: 18.492 min
Delta R.T.: -0.004 min
Response: 4341603
Conc: 36.20 ug/ml

Instrument :
FID_F
ClientSampleId :

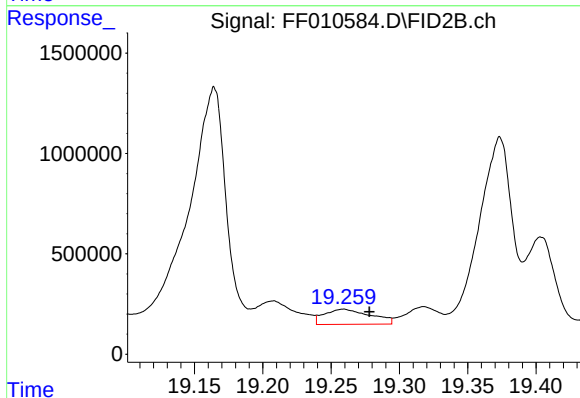


#15 N-TETRATRIACONTANE

R.T.: 19.259 min
Delta R.T.: -0.019 min
Response: 1779002
Conc: 16.76 ug/ml

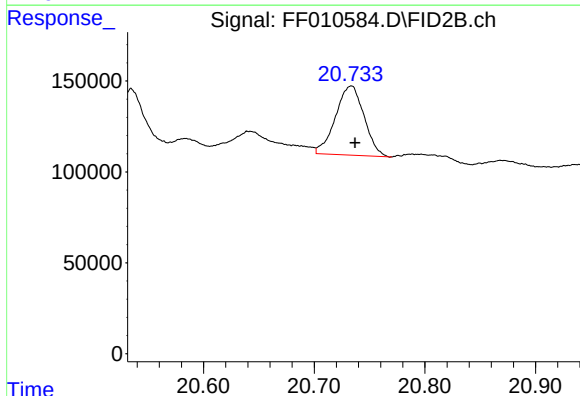

#17 N-OCTATRIACONTANE

R.T.: 20.733 min
Delta R.T.: -0.004 min
Response: 682130
Conc: 8.46 ug/ml

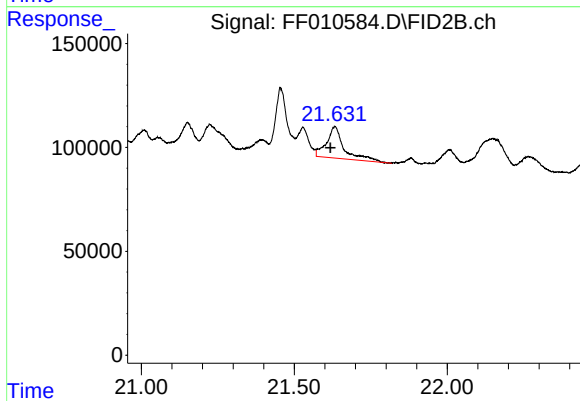

#18 N-TETRACONTANE

R.T.: 21.633 min
Delta R.T.: 0.015 min
Response: 601322
Conc: 7.64 ug/ml