

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051019\
 Data File : FF004513.D
 Signal(s) : FID2B.ch
 Acq On : 10 May 2019 15:44
 Operator : AJ\SJ
 Sample : K2801-07
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 10 23:08:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
 Quant Title :
 QLast Update : Thu May 09 09:32:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	1280830	12.781 ug/ml
Target Compounds			
4) N-TETRADECANE	8.292f	598866	4.407 ug/ml
7) N-EICOSANE	12.643f	277396	2.305 ug/ml
10) N-TETRACOSANE	14.861	168040	1.468 ug/ml
11) N-HEXACOSANE	15.914	122330	1.071 ug/ml
12) N-OCTACOSANE	16.866	247301	2.164 ug/ml
13) N-TRIACONTANE	17.756	249309	2.153 ug/ml
14) N-DOTRIACONTANE	18.610	561084	4.581 ug/ml
16) N-HEXATRIACONTANE	20.065	86965	0.807 ug/ml
18) N-TETRACONTANE	21.844f	347875	3.092 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051019\
Data File : FF004513.D
Signal(s) : FID2B.ch
Acq On : 10 May 2019 15:44
Operator : AJ\SJ
Sample : K2801-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 10 23:08:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
Quant Title :
QLast Update : Thu May 09 09:32:48 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

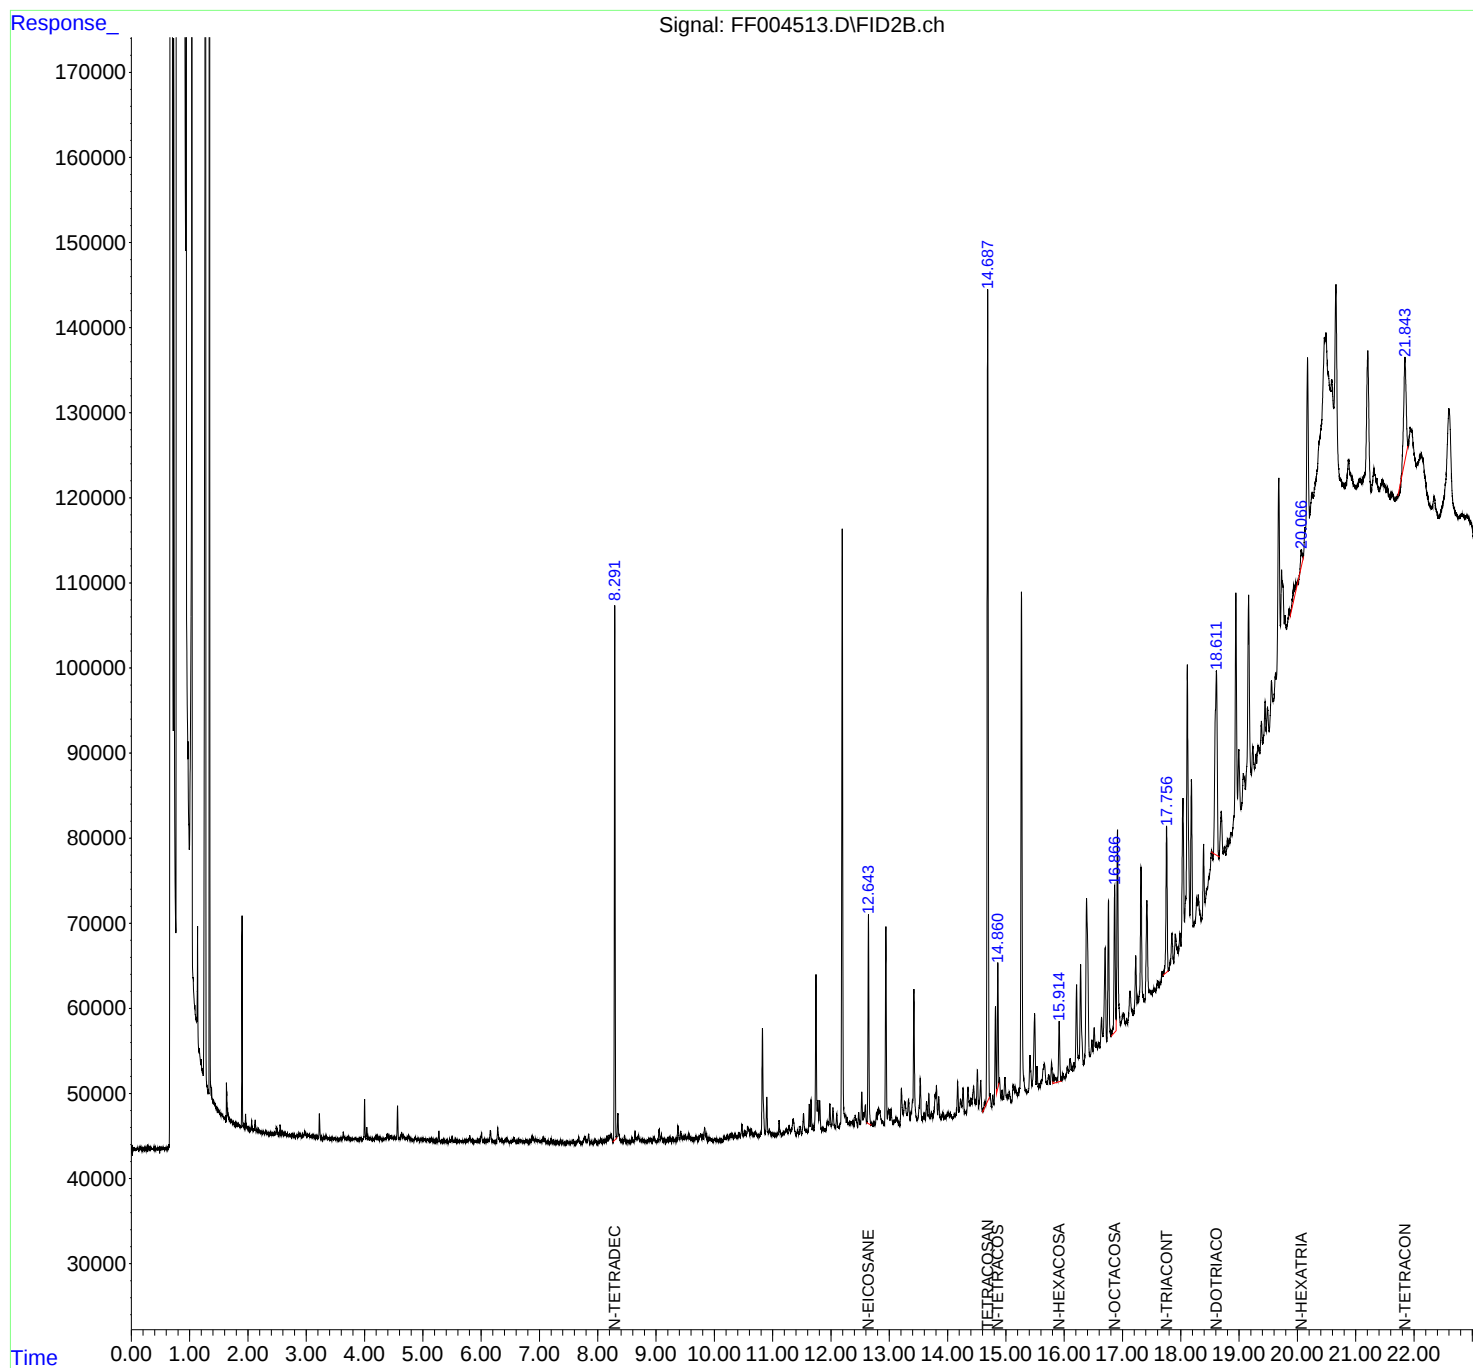

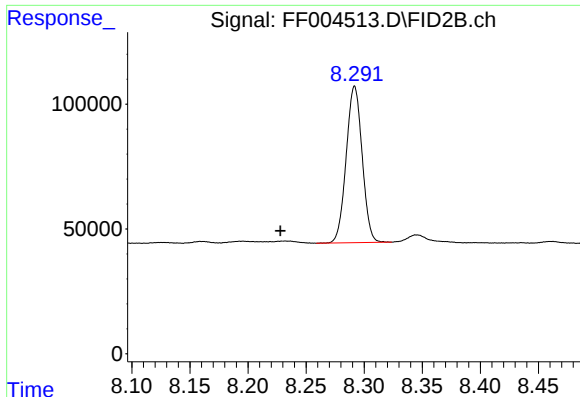


#4 N-TETRADECANE

R.T.: 8.292 min
Delta R.T.: 0.064 min
Response: 598866
Conc: 4.41 ug/ml

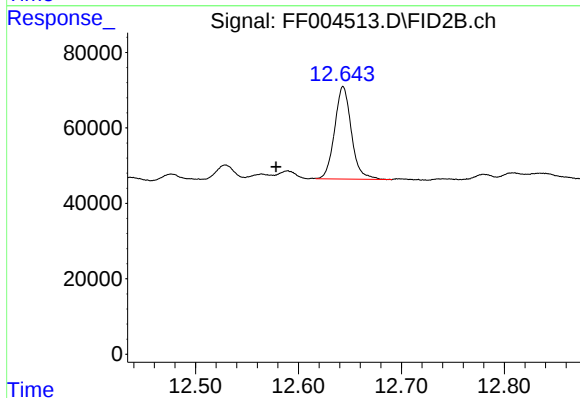


#7 N-EICOSANE

R.T.: 12.643 min
Delta R.T.: 0.065 min
Response: 277396
Conc: 2.31 ug/ml

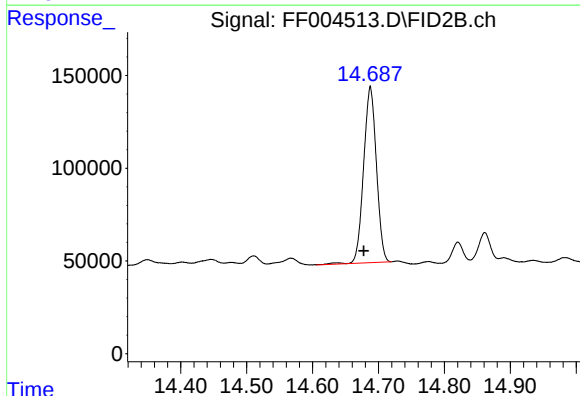


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: 0.010 min
Response: 1280830
Conc: 12.78 ug/ml

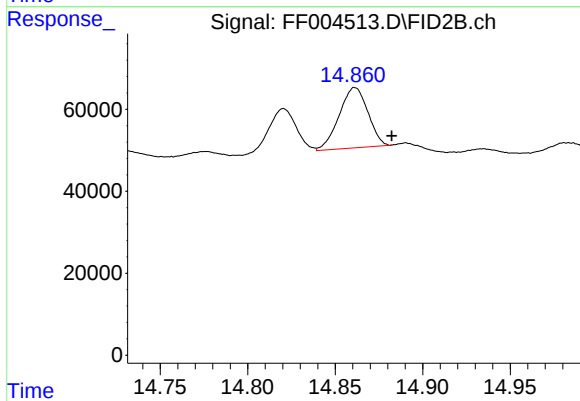


#10 N-TETRACOSANE

R.T.: 14.861 min
Delta R.T.: -0.021 min
Response: 168040
Conc: 1.47 ug/ml

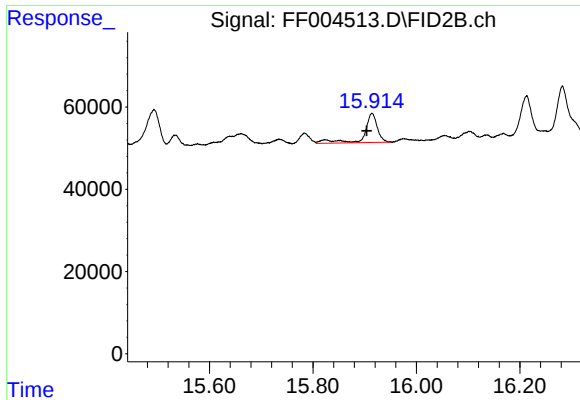


#11 N-HEXACOSANE

R.T.: 15.914 min
Delta R.T.: 0.010 min
Response: 122330
Conc: 1.07 ug/ml

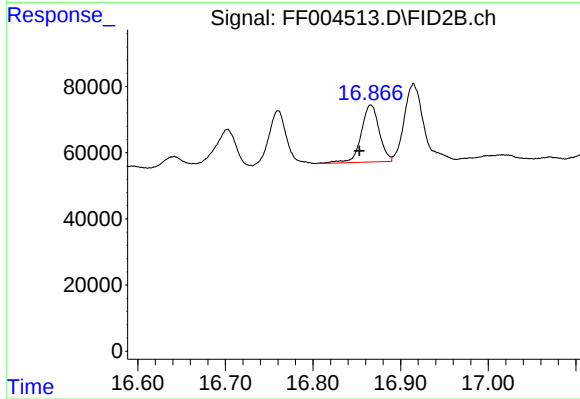


#12 N-OCTACOSANE

R.T.: 16.866 min
Delta R.T.: 0.013 min
Response: 247301
Conc: 2.16 ug/ml

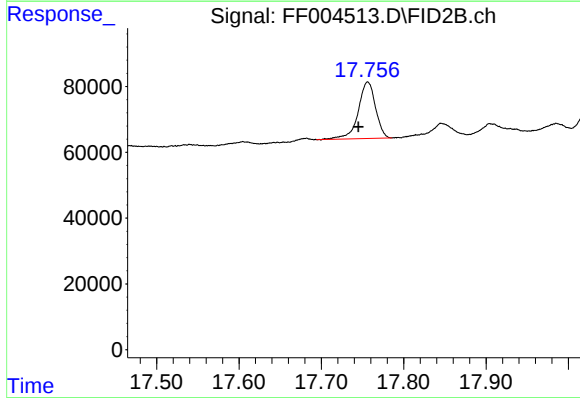


#13 N-TRIACONTANE

R.T.: 17.756 min
Delta R.T.: 0.011 min
Response: 249309
Conc: 2.15 ug/ml

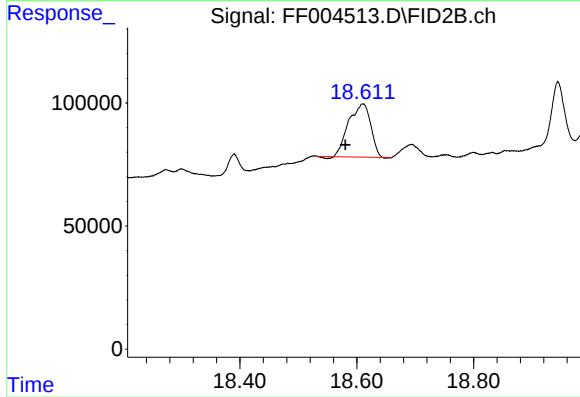


#14 N-DOTRIACONTANE

R.T.: 18.610 min
Delta R.T.: 0.030 min
Response: 561084
Conc: 4.58 ug/ml

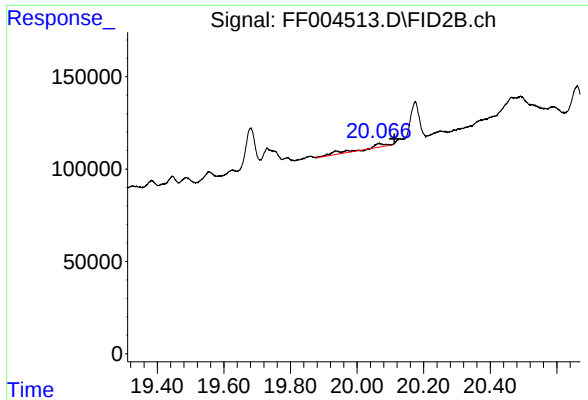

#16 N-HEXATRIACONTANE

R.T.: 20.065 min
Delta R.T.: -0.047 min
Response: 86965
Conc: 0.81 ug/ml

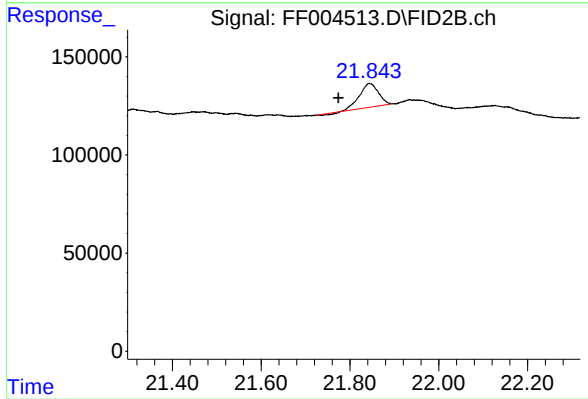

#18 N-TETRACONTANE

R.T.: 21.844 min
Delta R.T.: 0.070 min
Response: 347875
Conc: 3.09 ug/ml