

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051019\
 Data File : FF004509.D
 Signal(s) : FID2B.ch
 Acq On : 10 May 2019 13:48
 Operator : AJ\SJ
 Sample : PB119601BS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 10 14:18:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
 Quant Title :
 QLast Update : Thu May 09 09:32:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.690	2100772	20.963 ug/ml
Target Compounds			
2) N-DECANE	4.416	2838498	19.662 ug/ml
3) N-DODECANE	6.438	2745331	19.409 ug/ml
4) N-TETRADECANE	8.233	2631681	19.366 ug/ml
5) N-HEXADECANE	9.834	2563614	19.584 ug/ml
6) N-OCTADECANE	11.277	2462238	19.863 ug/ml
7) N-EICOSANE	12.589	2433848	20.224 ug/ml
8) N-DOCOSANE	13.789	2389629	20.592 ug/ml
10) N-TETRACOSANE	14.893	2400693	20.967 ug/ml
11) N-HEXACOSANE	15.916	2439636	21.368 ug/ml
12) N-OCTACOSANE	16.868	2507370	21.941 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051019\
Data File : FF004509.D
Signal(s) : FID2B.ch
Acq On : 10 May 2019 13:48
Operator : AJ\SJ
Sample : PB119601BS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 10 14:18:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
Quant Title :
QLast Update : Thu May 09 09:32:48 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

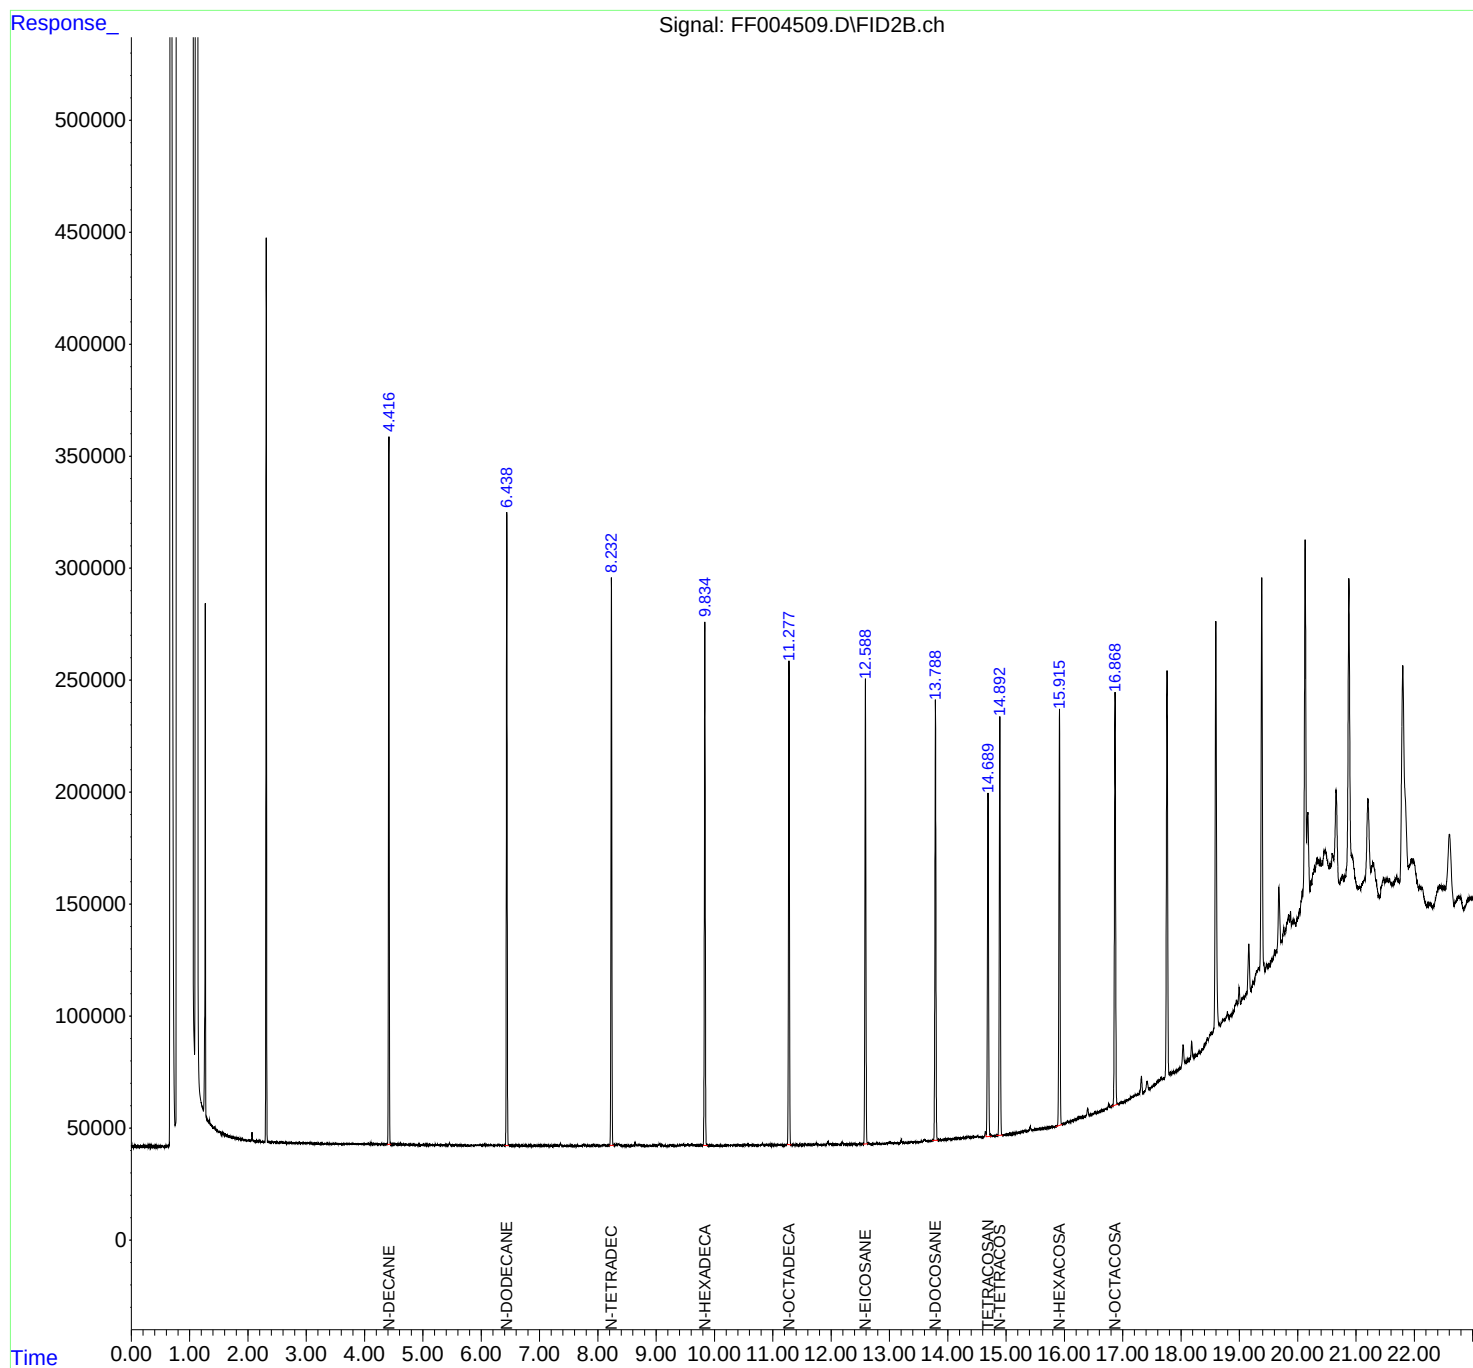

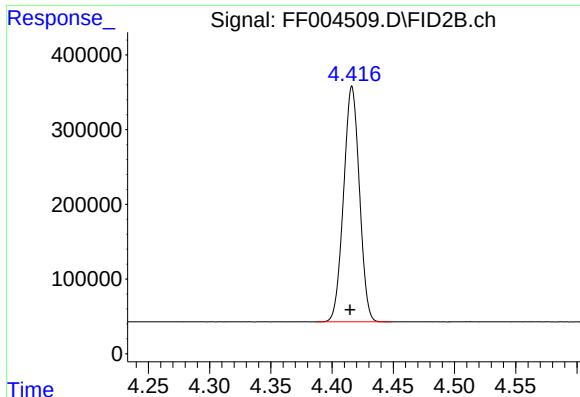


#2 N-DECANE

R.T.: 4.416 min
Delta R.T.: 0.002 min
Response: 2838498
Conc: 19.66 ug/ml

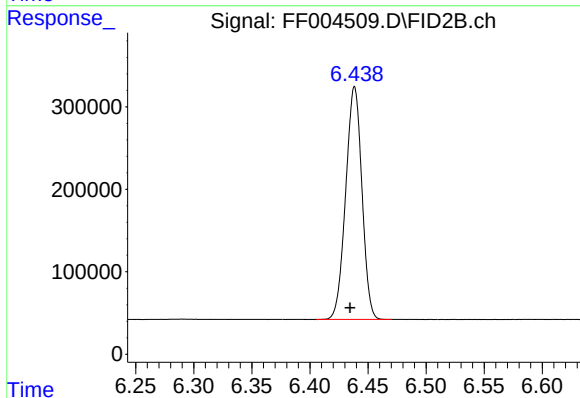


#3 N-DODECANE

R.T.: 6.438 min
Delta R.T.: 0.004 min
Response: 2745331
Conc: 19.41 ug/ml

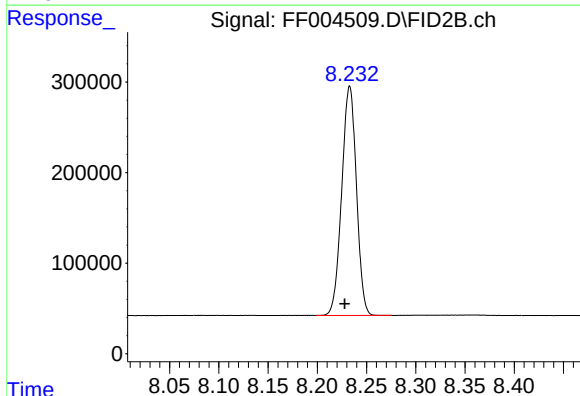


#4 N-TETRADECANE

R.T.: 8.233 min
Delta R.T.: 0.005 min
Response: 2631681
Conc: 19.37 ug/ml

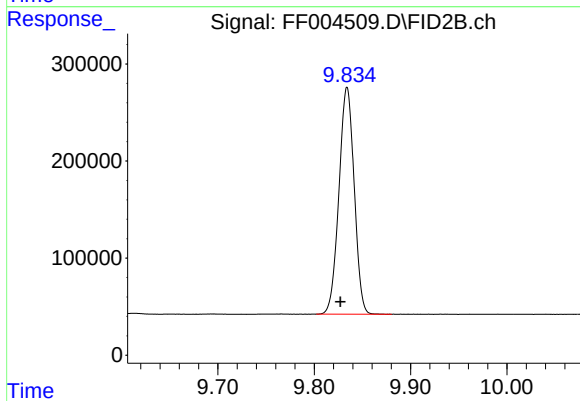


#5 N-HEXADECANE

R.T.: 9.834 min
Delta R.T.: 0.007 min
Response: 2563614
Conc: 19.58 ug/ml

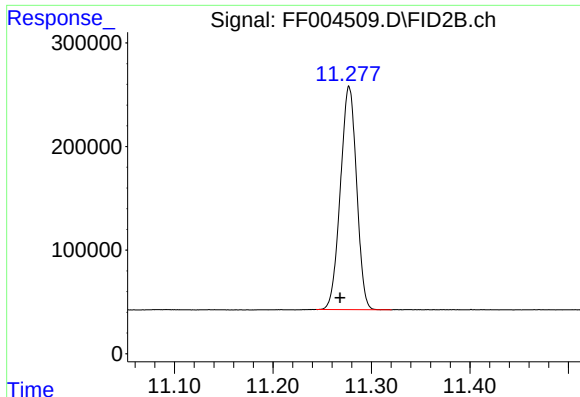


#6 N-OCTADECANE

R.T.: 11.277 min
Delta R.T.: 0.009 min
Response: 2462238
Conc: 19.86 ug/ml

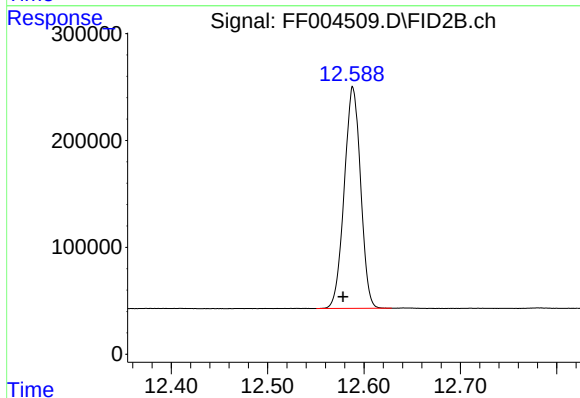


#7 N-EICOSANE

R.T.: 12.589 min
Delta R.T.: 0.010 min
Response: 2433848
Conc: 20.22 ug/ml

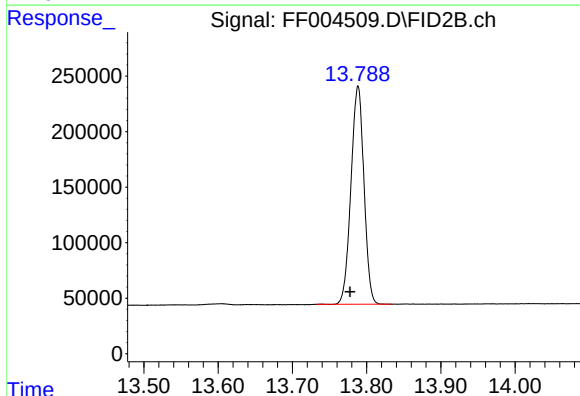


#8 N-DOCOSANE

R.T.: 13.789 min
Delta R.T.: 0.011 min
Response: 2389629
Conc: 20.59 ug/ml

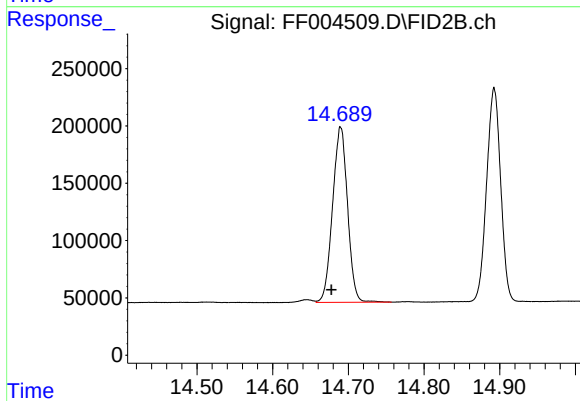


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.690 min
Delta R.T.: 0.012 min
Response: 2100772
Conc: 20.96 ug/ml

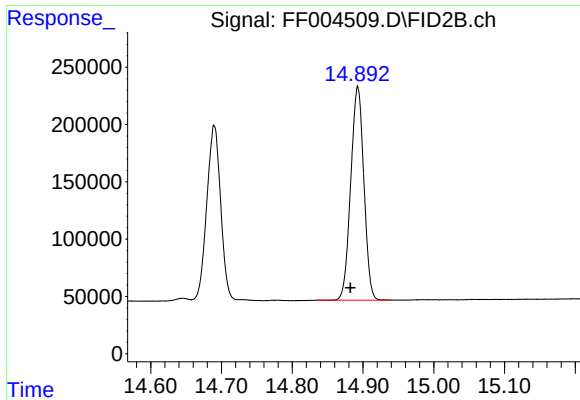


#10 N-TETRACOSANE

R.T.: 14.893 min
Delta R.T.: 0.010 min
Response: 2400693
Conc: 20.97 ug/ml

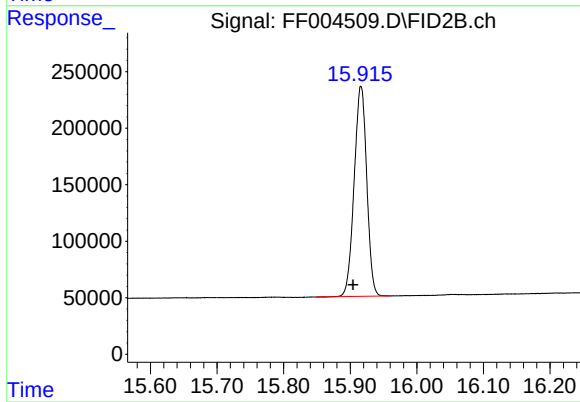

#11 N-HEXACOSANE

R.T.: 15.916 min
Delta R.T.: 0.012 min
Response: 2439636
Conc: 21.37 ug/ml

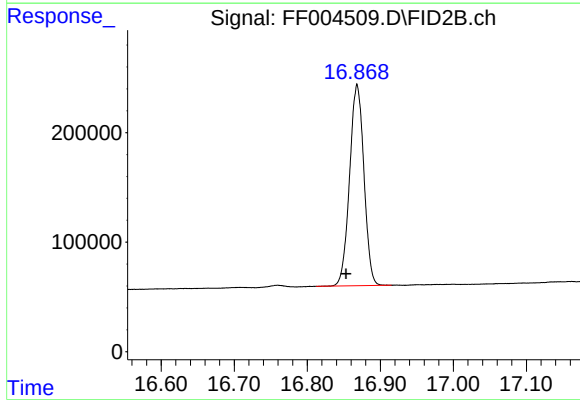

#12 N-OCTACOSANE

R.T.: 16.868 min
Delta R.T.: 0.015 min
Response: 2507370
Conc: 21.94 ug/ml