

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
 Data File : FF012597.D
 Signal(s) : FID2B.ch
 Acq On : 10 May 2023 14:45
 Operator : YP\AJ
 Sample : 02666-01 25X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 11 01:52:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
 Quant Title :
 QLast Update : Fri May 05 16:23:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.732	154801	1.185 ug/ml
4) N-TETRADECANE	8.556	336669	2.612 ug/ml
5) N-HEXADECANE	10.162	467061	3.465 ug/ml
6) N-OCTADECANE	11.604	327046	2.361 ug/ml
7) N-EICOSANE	12.912	223554	1.615 ug/ml
10) N-TETRACOSANE	15.209	236752	1.774 ug/ml
13) N-TRIACONTANE	18.066	72526	0.580 ug/ml
14) N-DOTRIACONTANE	18.900	129099	1.081 ug/ml
15) N-TETRATRIACONTANE	19.692	361361	3.285 ug/ml
16) N-HEXATRIACONTANE	20.410	239548	2.302 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
Data File : FF012597.D
Signal(s) : FID2B.ch
Acq On : 10 May 2023 14:45
Operator : YP\AJ
Sample : 02666-01 25X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 01:52:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

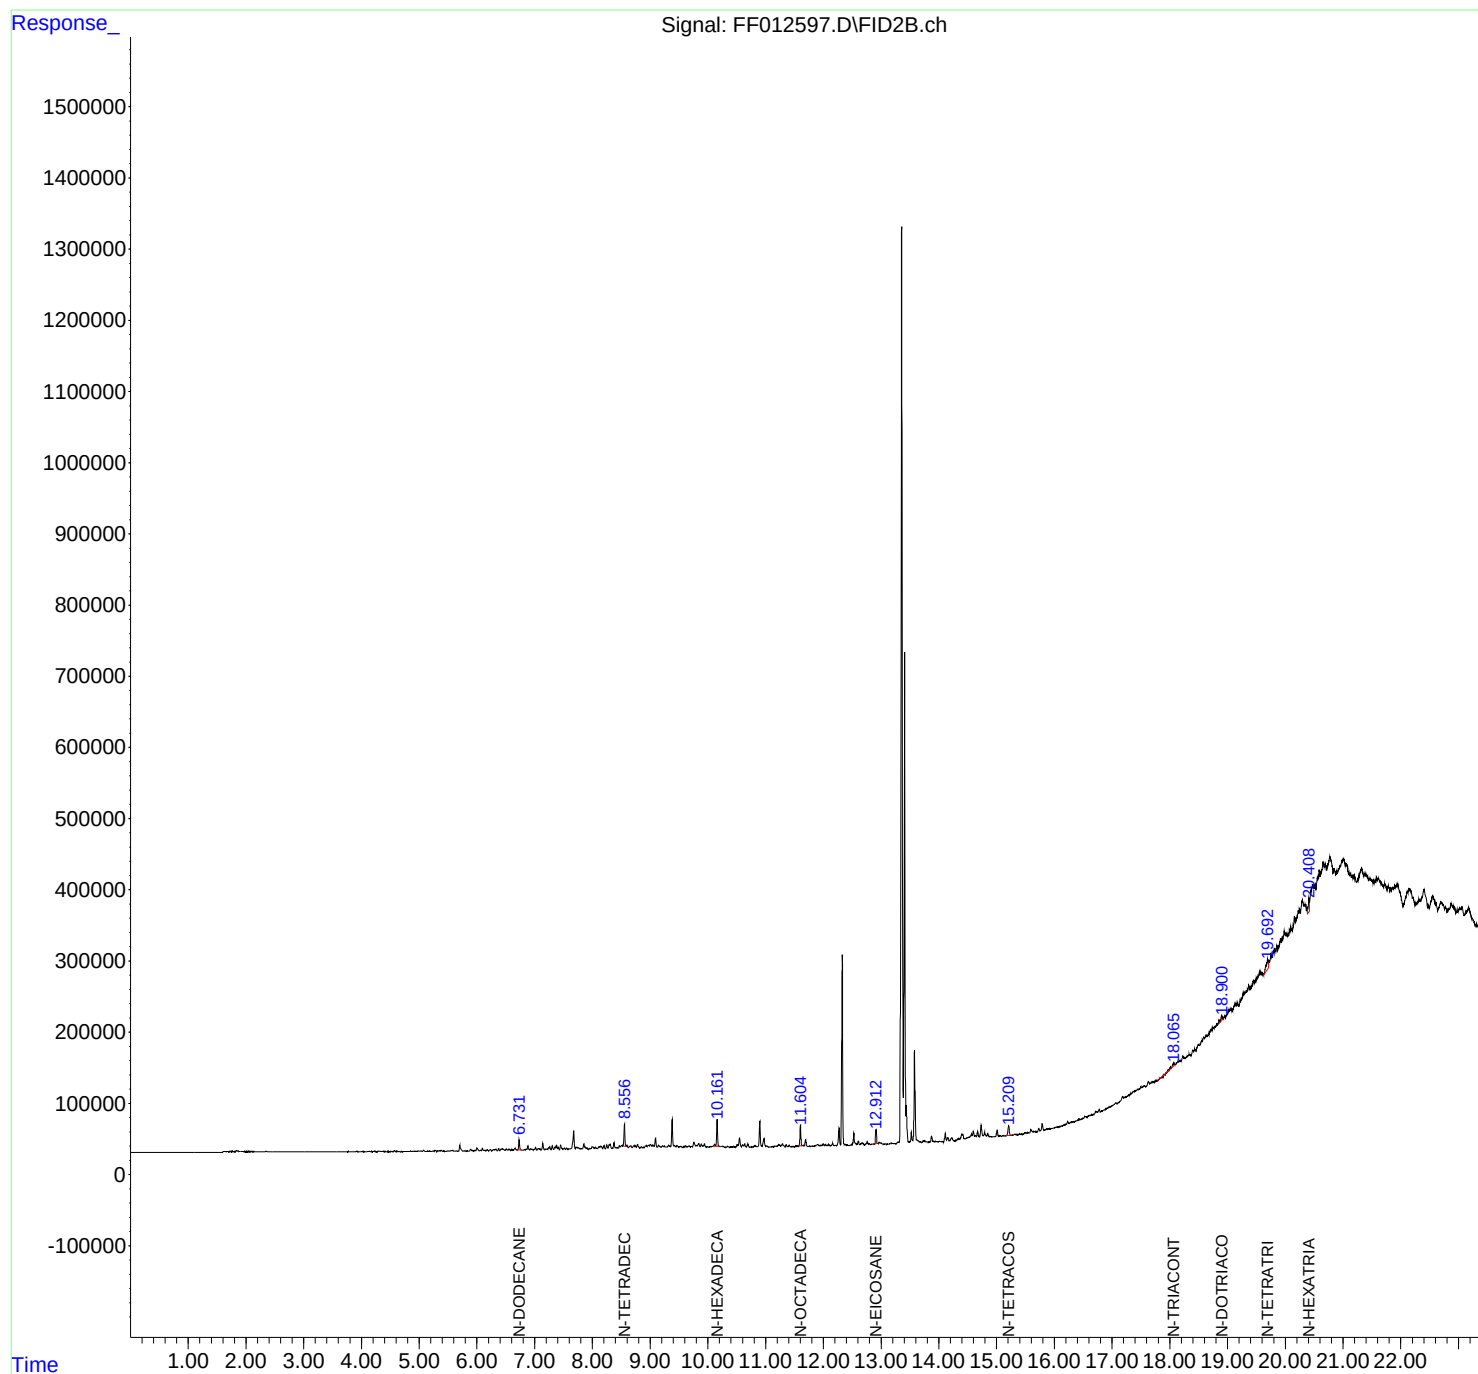


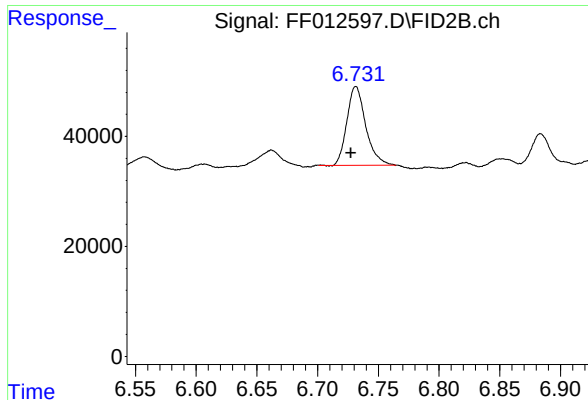

#3 N-DODECANE


R.T.: 6.732 min
Delta R.T.: 0.004 min
Response: 154801
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :

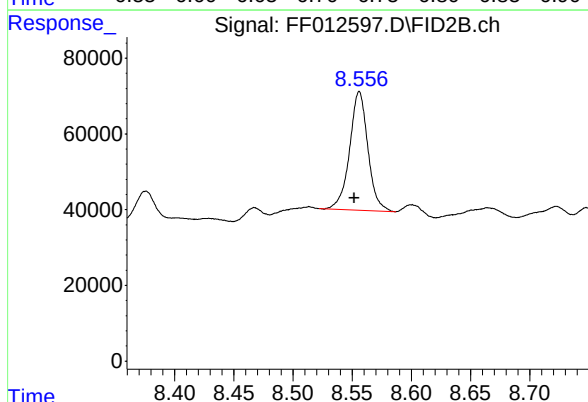


#4 N-TETRADECANE

R.T.: 8.556 min
Delta R.T.: 0.004 min
Response: 336669
Conc: 2.61 ug/ml

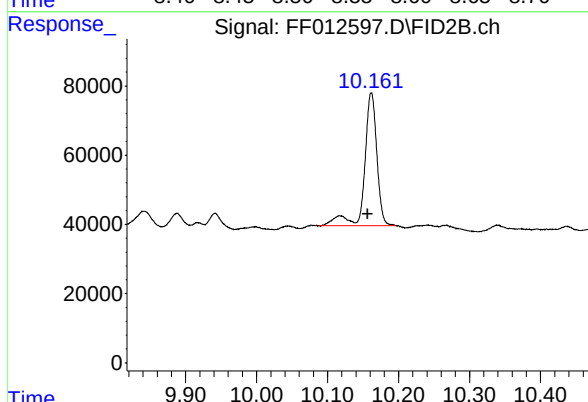


#5 N-HEXADECANE

R.T.: 10.162 min
Delta R.T.: 0.005 min
Response: 467061
Conc: 3.47 ug/ml

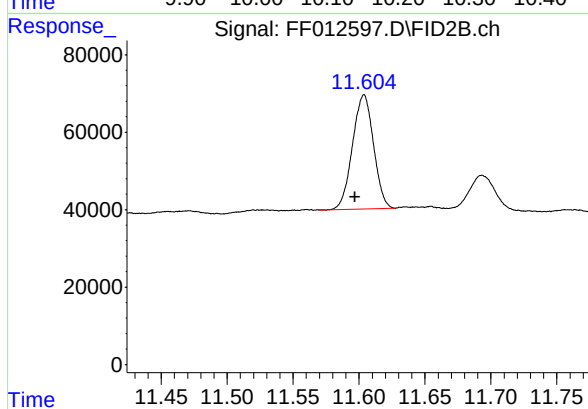

#6 N-OCTADECANE


R.T.: 11.604 min
Delta R.T.: 0.007 min
Response: 327046
Conc: 2.36 ug/ml

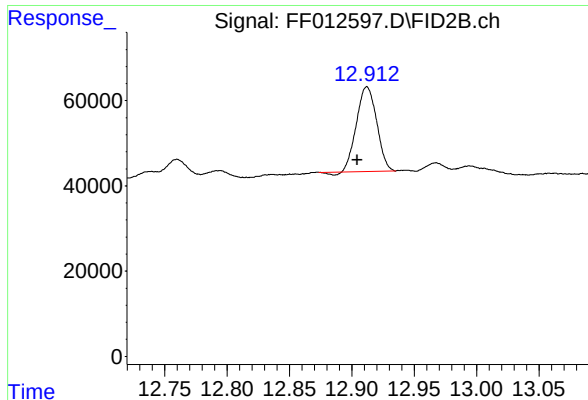

#7 N-EICOSANE


R.T.: 12.912 min
Delta R.T.: 0.008 min
Response: 223554
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :

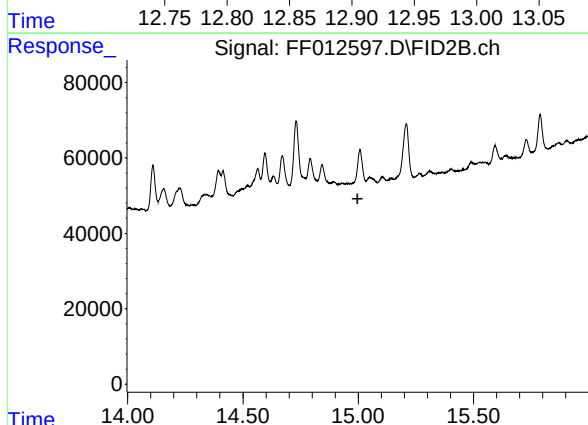


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.997 min
Response: 0
Conc: N.D.

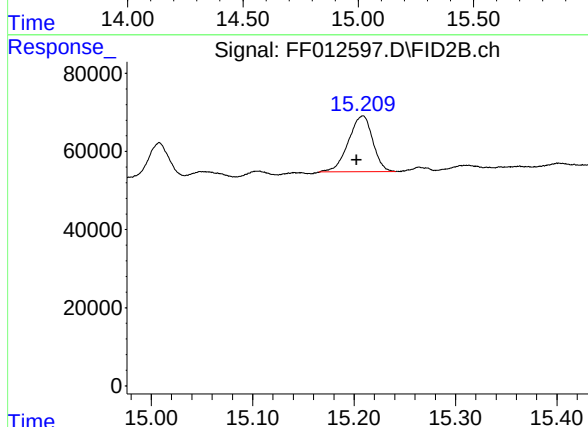


#10 N-TETRACOSANE

R.T.: 15.209 min
Delta R.T.: 0.006 min
Response: 236752
Conc: 1.77 ug/ml

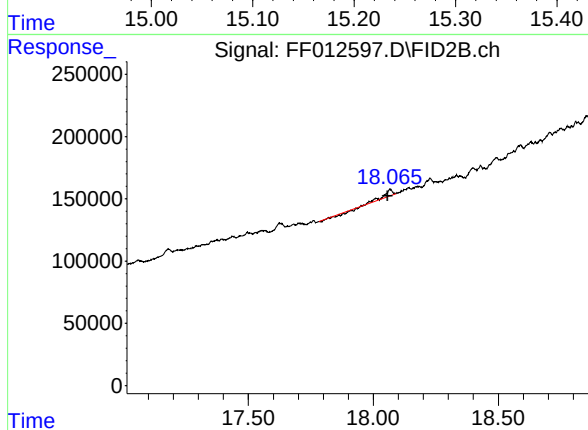

#13 N-TRIACONTANE


R.T.: 18.066 min
Delta R.T.: 0.009 min
Response: 72526
Conc: 0.58 ug/ml

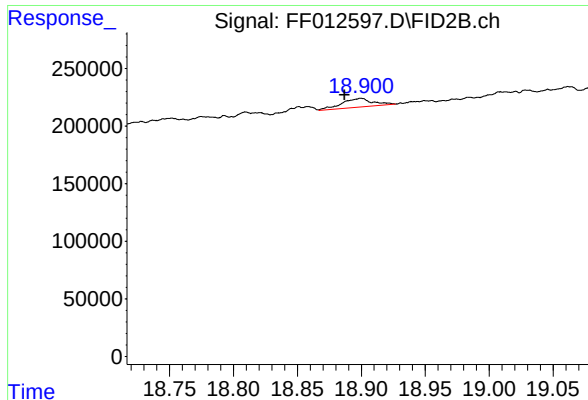

#14 N-DOTRIACONTANE


R.T.: 18.900 min
Delta R.T.: 0.013 min
Response: 129099
Conc: 1.08 ug/ml

Instrument :
FID_F
ClientSampleId :

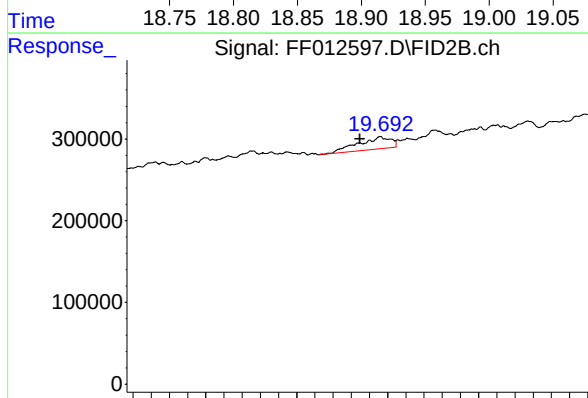

#15 N-TETRATRIACONTANE

R.T.: 19.692 min
Delta R.T.: 0.022 min
Response: 361361
Conc: 3.29 ug/ml

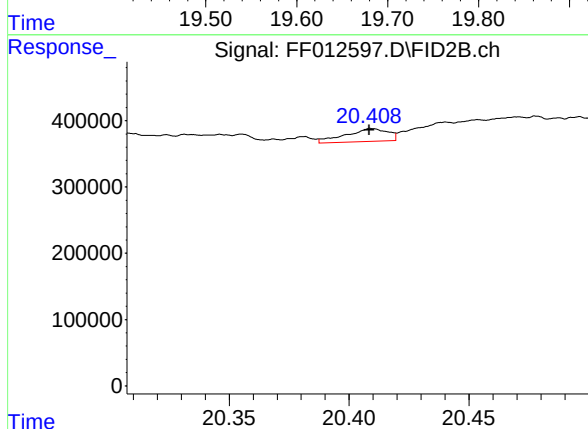

#16 N-HEXATRIACONTANE

R.T.: 20.410 min
Delta R.T.: 0.001 min
Response: 239548
Conc: 2.30 ug/ml