

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
Data File : FF012598.D
Signal(s) : FID2B.ch
Acq On : 10 May 2023 15:14
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 01:52:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.007	1689860	13.998 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.355f	114592	1.101 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
Data File : FF012598.D
Signal(s) : FID2B.ch
Acq On : 10 May 2023 15:14
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 01:52:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

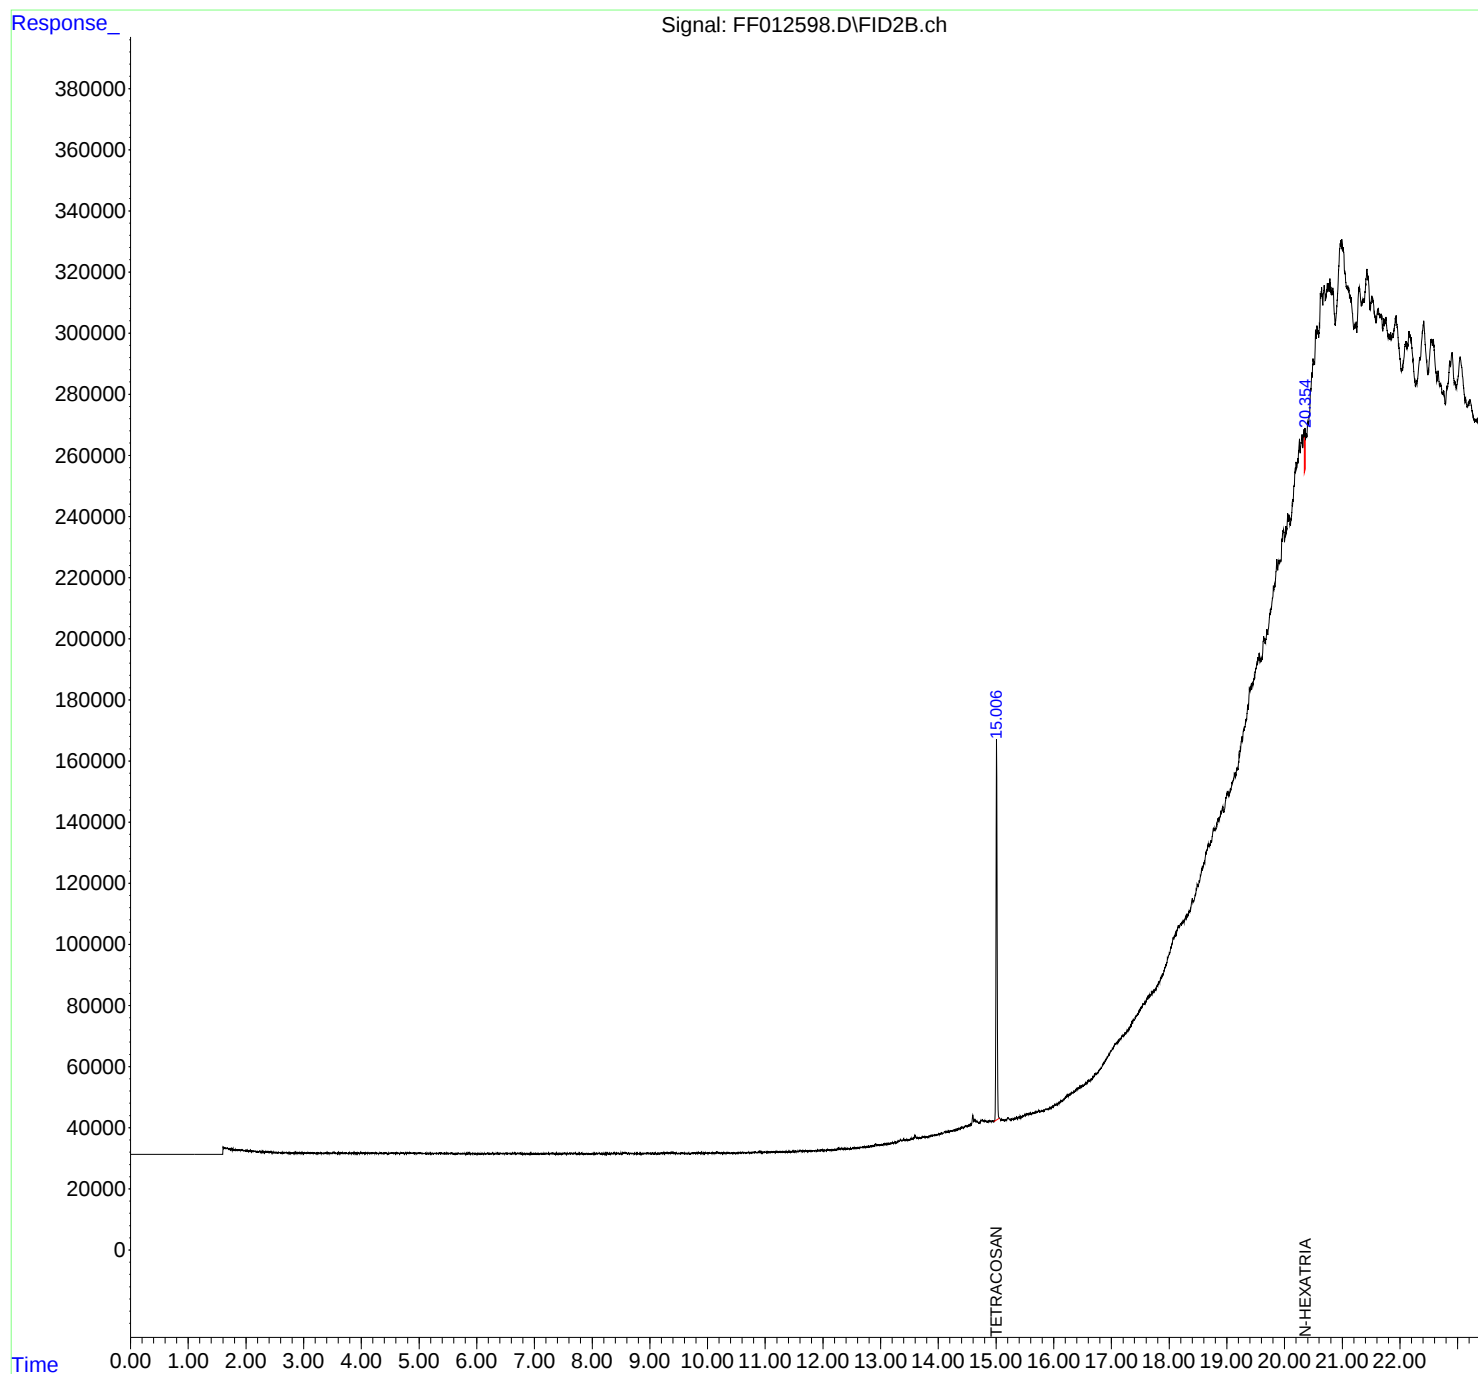


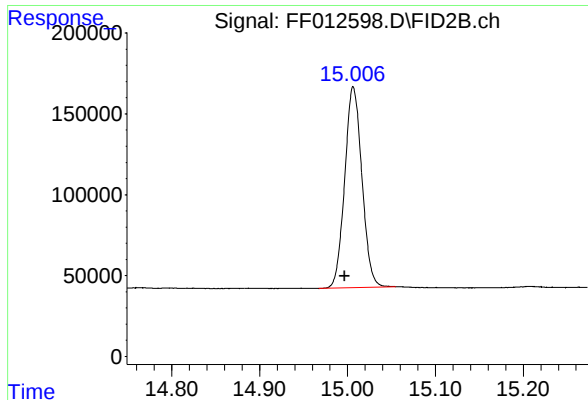

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.007 min
Delta R.T.: 0.010 min
Response: 1689860
Conc: 14.00 ug/ml

Instrument :
FID_F
ClientSampleId :

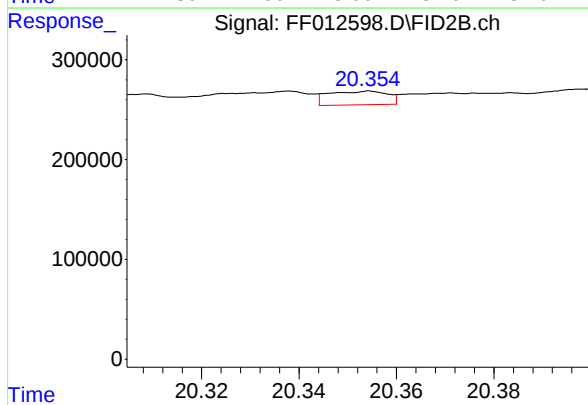

#16 N-HEXATRIACONTANE

R.T.: 20.355 min
Delta R.T.: -0.054 min
Response: 114592
Conc: 1.10 ug/ml