

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
Data File : FF012597.D
Signal(s) : FID2B.ch
Acq On : 10 May 2023 14:45
Operator : YP\AJ
Sample : 02666-01 25X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BU-02-050823

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/11/2023
Supervised By :Ankita Jodhani 05/11/2023

Integration File: autoint1.e
Quant Time: May 11 01:52:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.008	115026	0.953 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051023\
Data File : FF012597.D
Signal(s) : FID2B.ch
Acq On : 10 May 2023 14:45
Operator : YP\AJ
Sample : 02666-01 25X
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
BU-02-050823


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/11/2023
Supervised By :Ankita Jodhani 05/11/2023

Integration File: autoint1.e
Quant Time: May 11 01:52:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

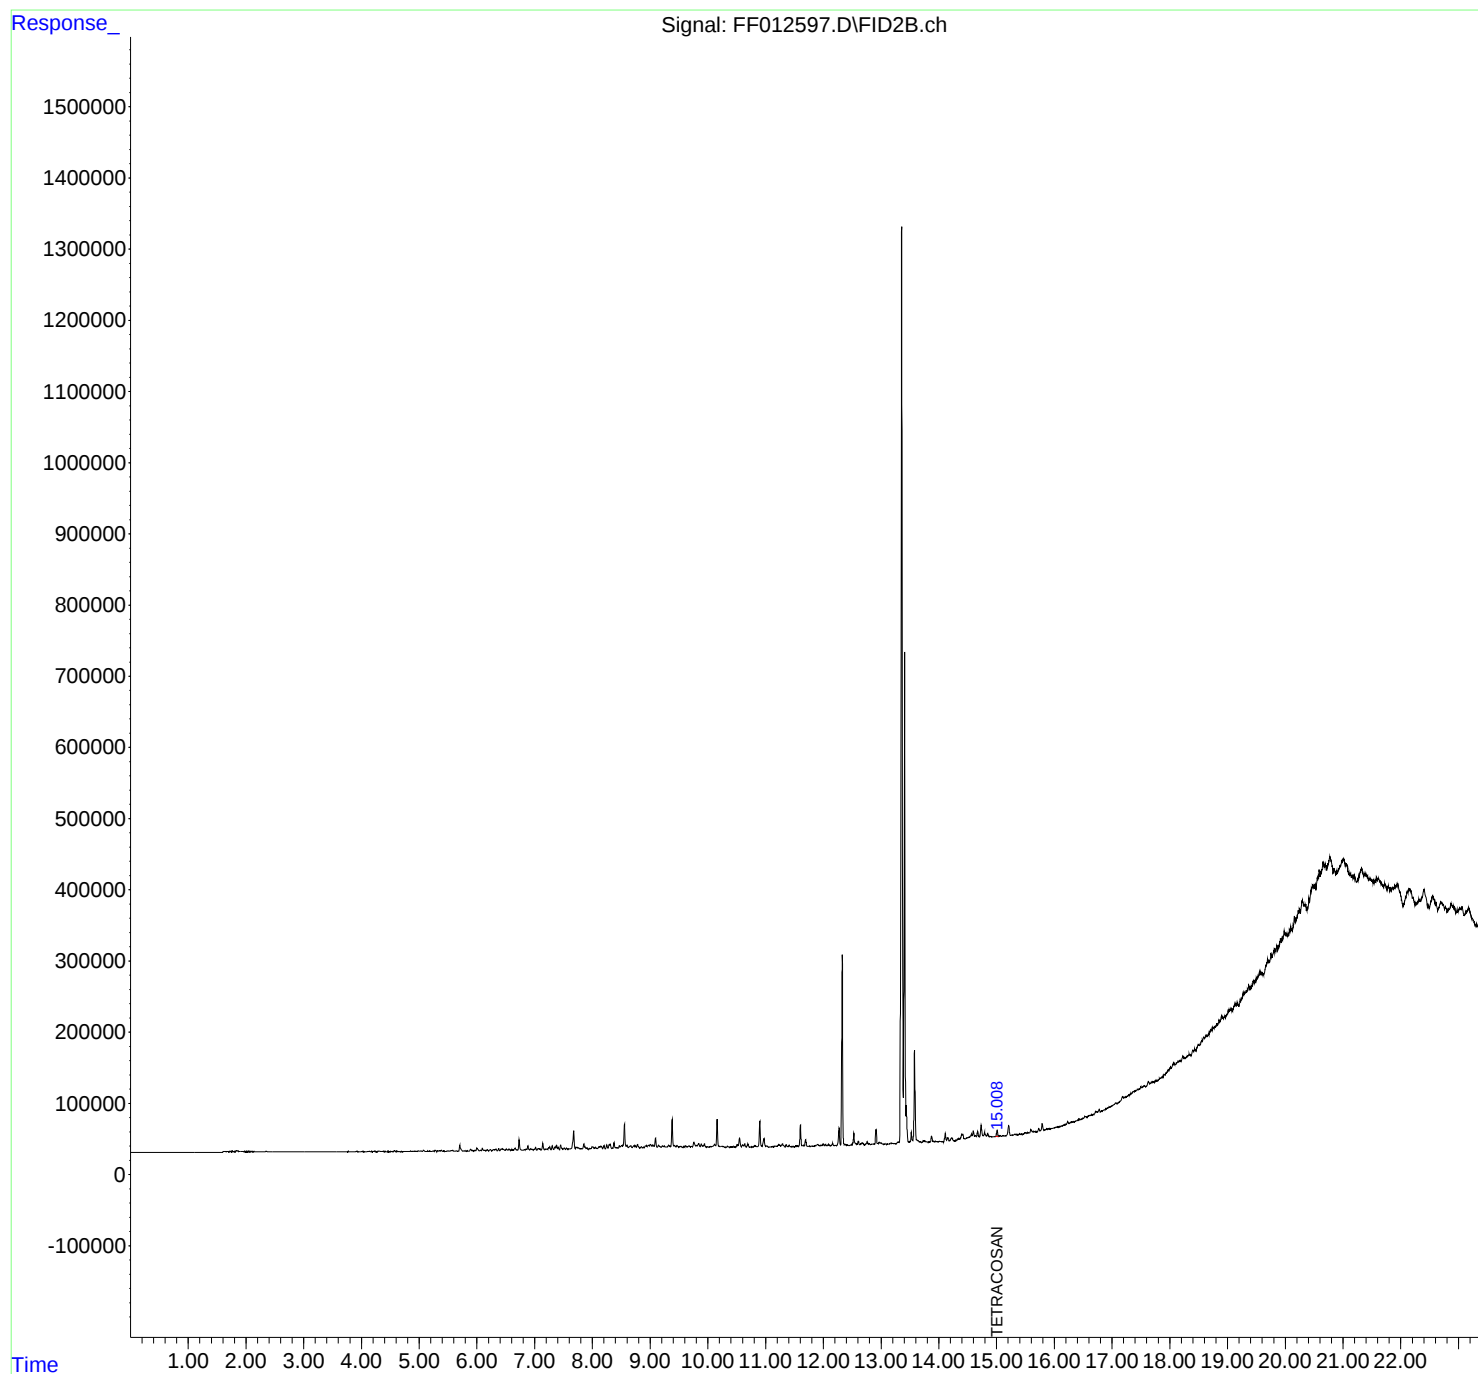

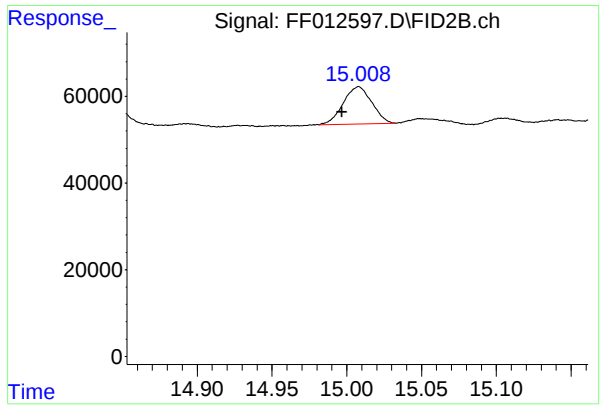

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.008 min
Delta R.T.: 0.011 min
Response: 115026
Conc: 0.95 ug/ml

Instrument :

FID_F

ClientSampleId :

BU-02-050823

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/11/2023

Supervised By :Ankita Jodhani 05/11/2023