

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
 Data File : FF014186.D
 Signal(s) : FID2B.ch
 Acq On : 10 May 2024 19:56
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 11 03:18:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
 Quant Title :
 QLast Update : Fri May 10 13:22:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.654	1891519	16.273 ug/ml
12) N-OCTACOSANE	17.116	1719241	15.671 ug/ml
13) N-TRIACONTANE	18.004	58932	0.540 ug/ml
14) N-DOTRIACONTANE	18.837	93528	0.733 ug/ml
15) N-TETRATRIACONTANE	19.620	69503	0.685 ug/ml
16) N-HEXATRIACONTANE	20.360	61347	0.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
Data File : FF014186.D
Signal(s) : FID2B.ch
Acq On : 10 May 2024 19:56
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 03:18:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

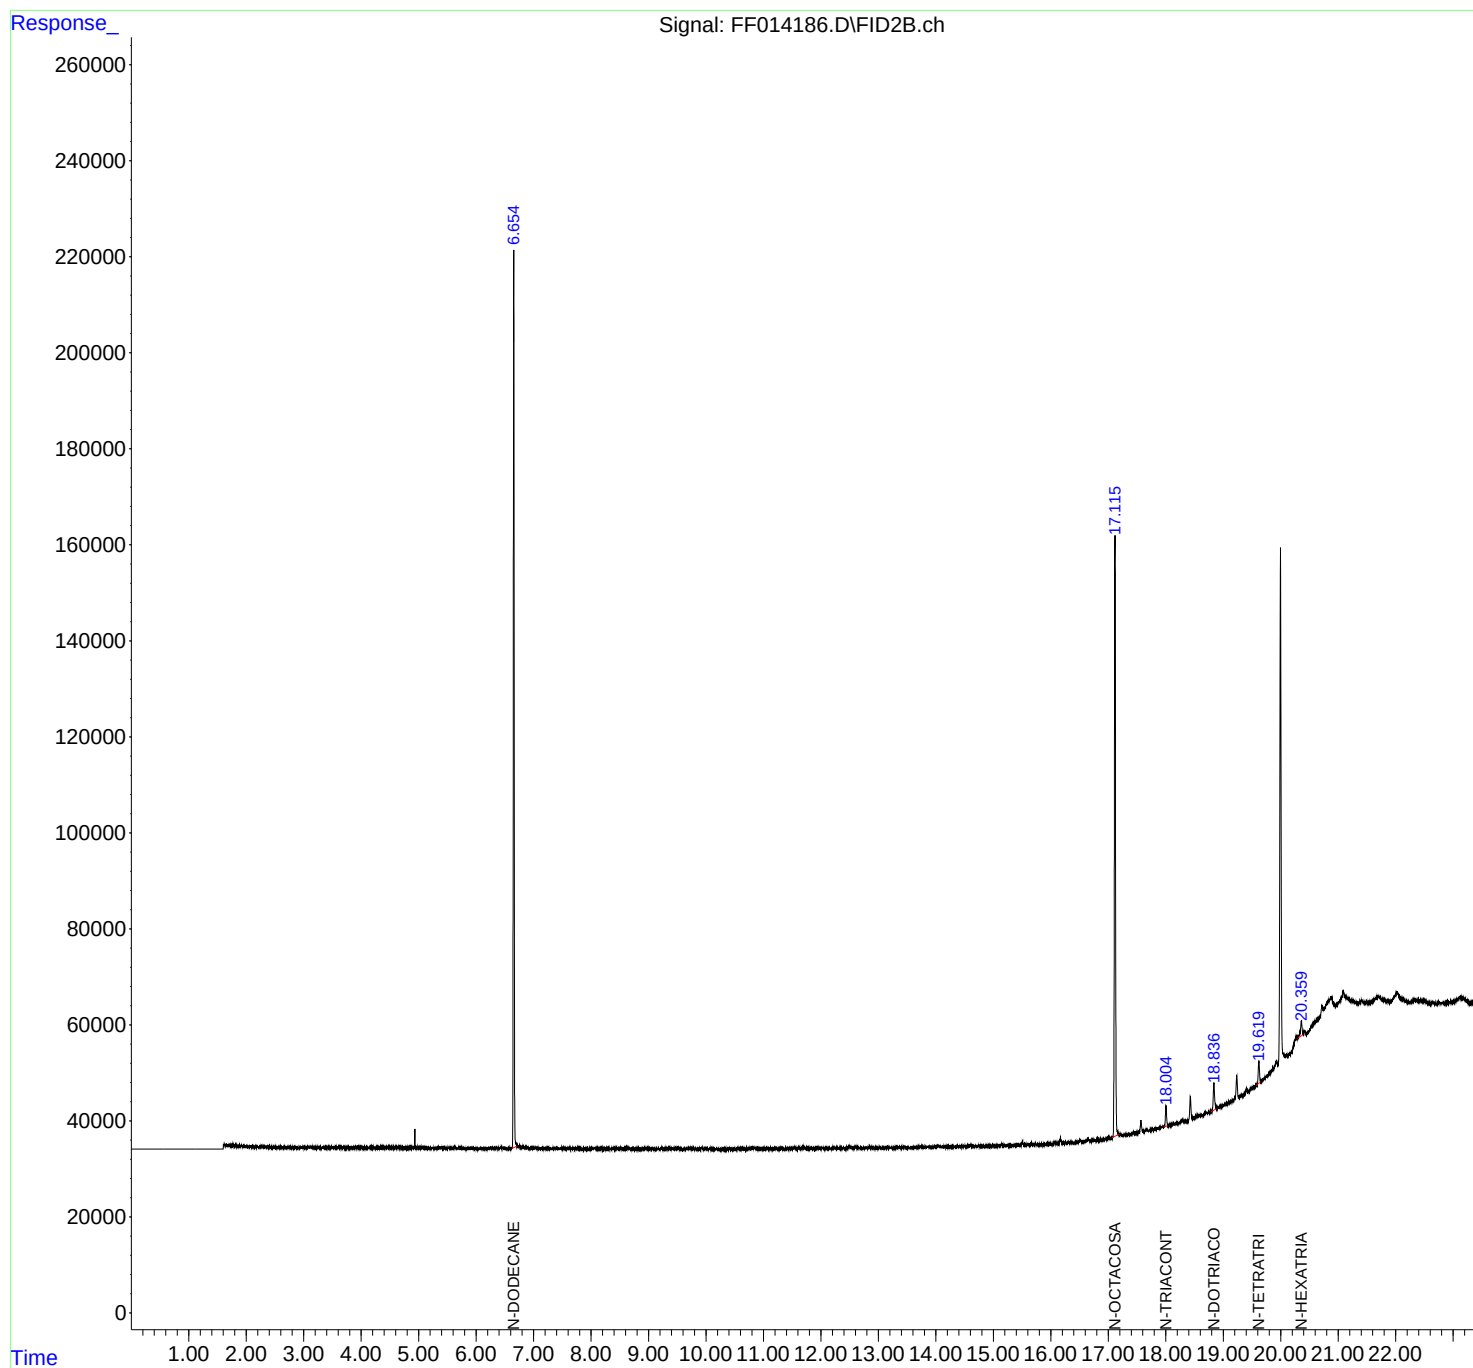


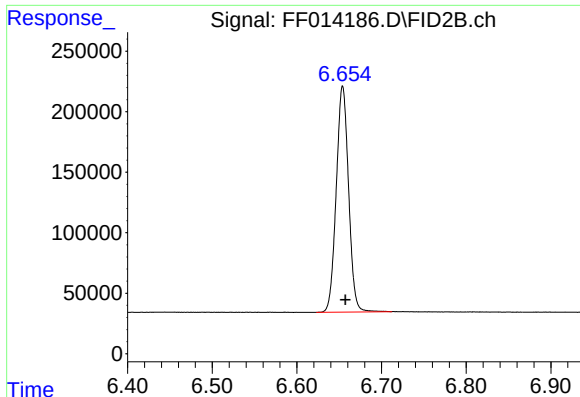

#3 N-DODECANE


R.T.: 6.654 min
Delta R.T.: -0.003 min
Response: 1891519
Conc: 16.27 ug/ml

Instrument :
FID_F
ClientSampleId :

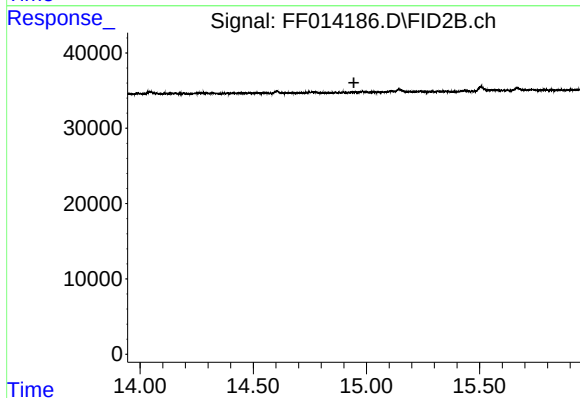


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.944 min
Response: 0
Conc: N.D.

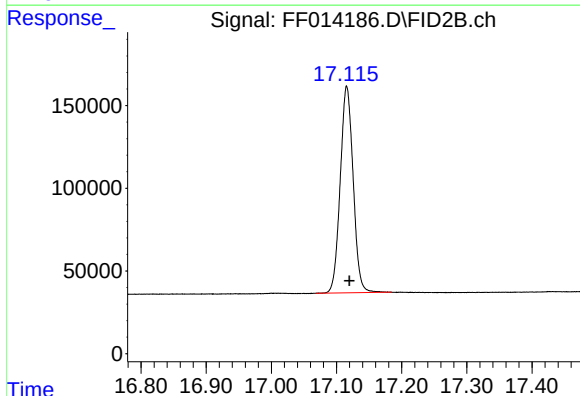


#12 N-OCTACOSANE

R.T.: 17.116 min
Delta R.T.: -0.004 min
Response: 1719241
Conc: 15.67 ug/ml

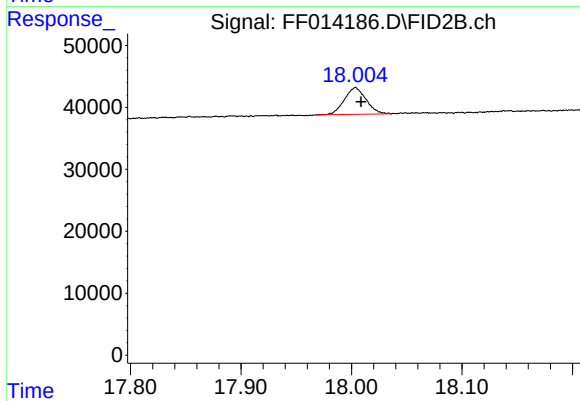

#13 N-TRIACONTANE


R.T.: 18.004 min
Delta R.T.: -0.005 min
Response: 58932
Conc: 0.54 ug/ml

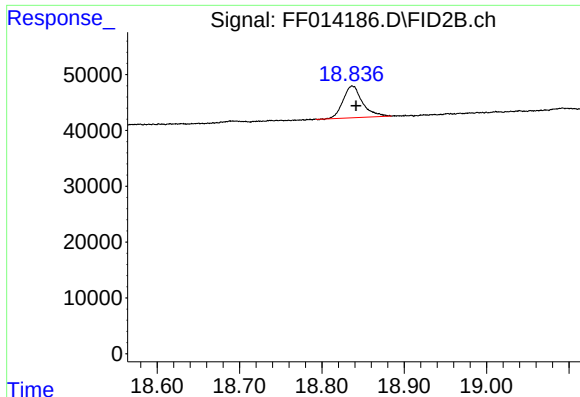

#14 N-DOTRIACONTANE


R.T.: 18.837 min
Delta R.T.: -0.004 min
Response: 93528
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :

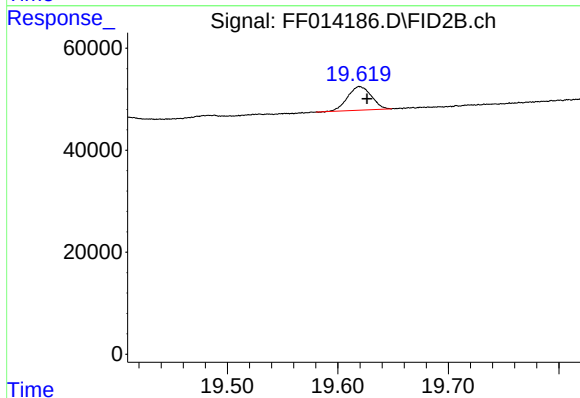

#15 N-TETRATRIACONTANE

R.T.: 19.620 min
Delta R.T.: -0.007 min
Response: 69503
Conc: 0.69 ug/ml

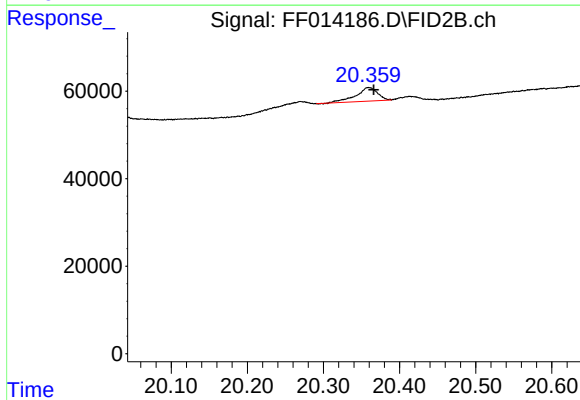

#16 N-HEXATRIACONTANE

R.T.: 20.360 min
Delta R.T.: -0.006 min
Response: 61347
Conc: 0.64 ug/ml