

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
Data File : FF014178.D
Signal(s) : FID2B.ch
Acq On : 10 May 2024 15:32
Operator : YP\AJ
Sample : PB160808BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB160808BL

Integration File: autoint1.e
Quant Time: May 11 03:16:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.943	1992011	19.932 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
Data File : FF014178.D
Signal(s) : FID2B.ch
Acq On : 10 May 2024 15:32
Operator : YP\AJ
Sample : PB160808BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB160808BL

Integration File: autoint1.e
Quant Time: May 11 03:16:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

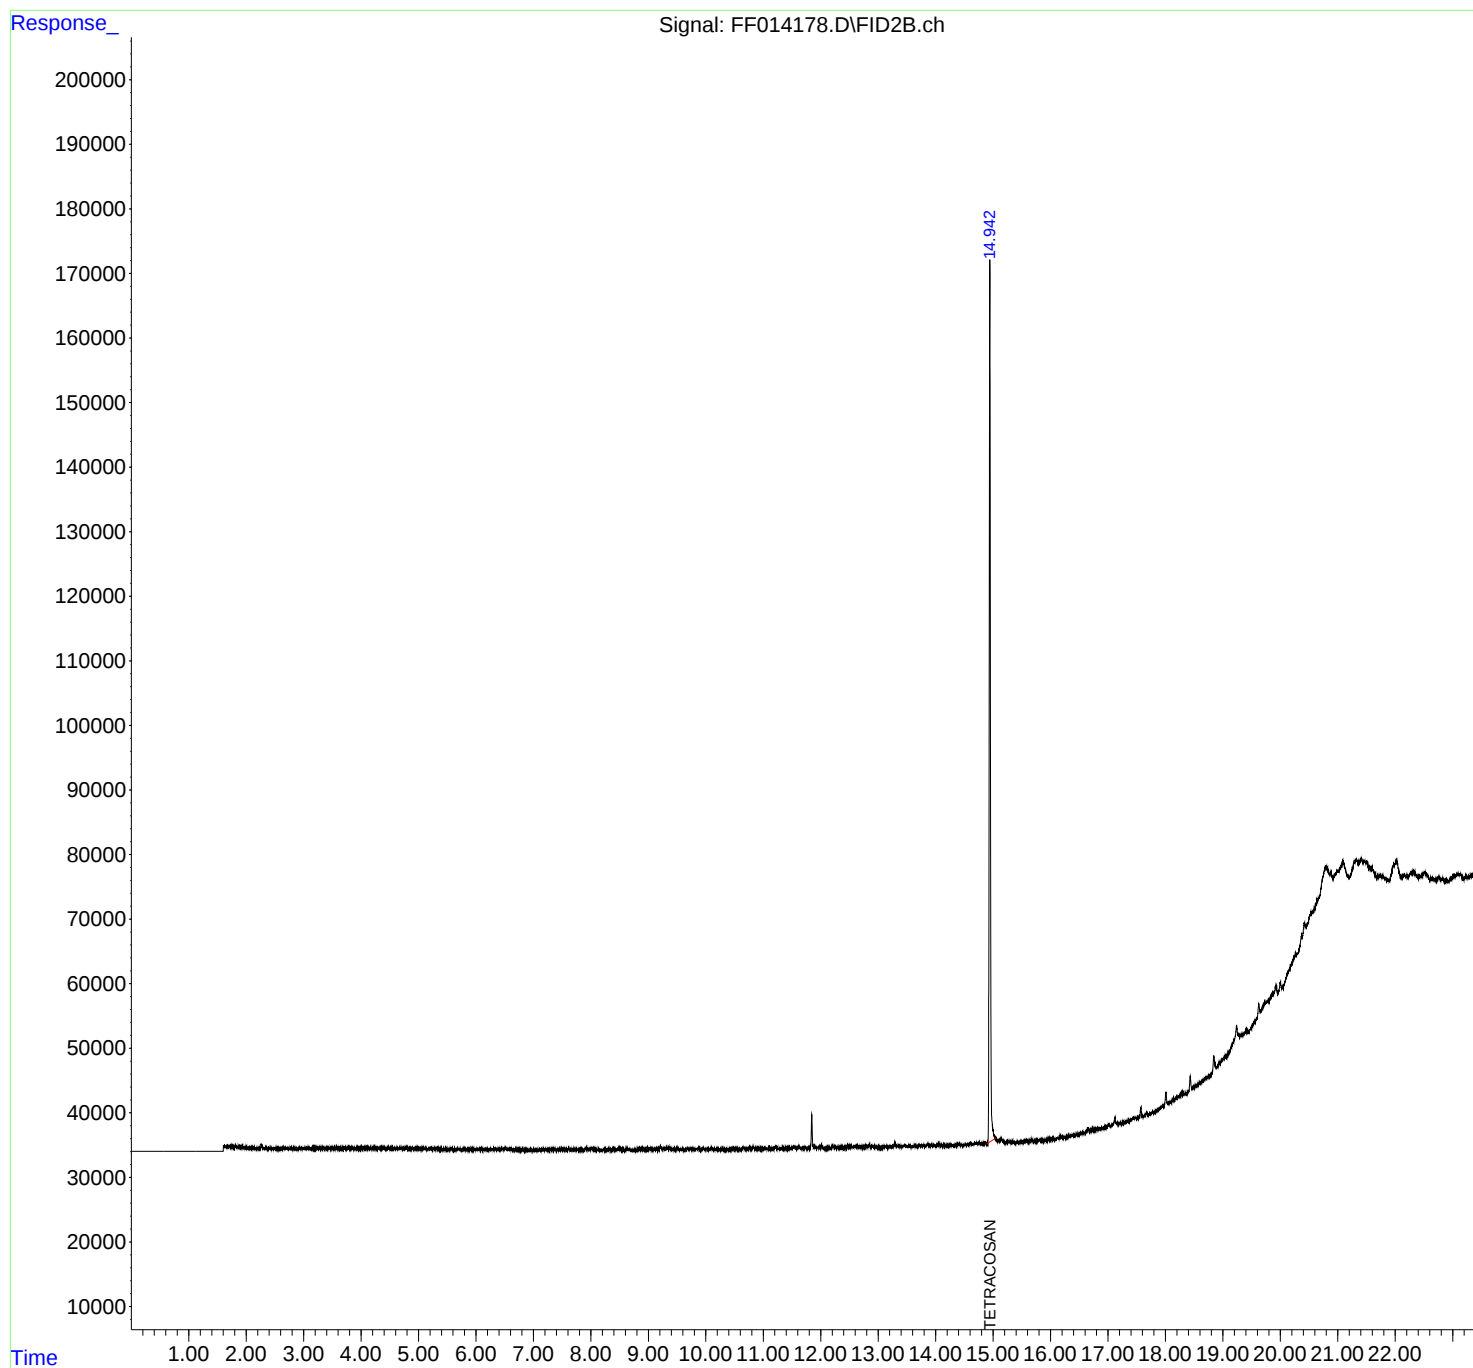

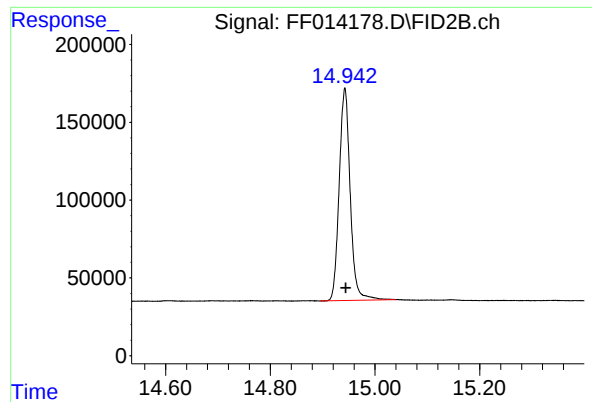

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.943 min
Delta R.T.: -0.002 min
Response: 1992011
Conc: 19.93 ug/ml

Instrument :

FID_F

ClientSampleId :

PB160808BL