

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
Data File : FF014188.D
Signal(s) : FID2B.ch
Acq On : 10 May 2024 20:55
Operator : YP\AJ
Sample : PB160787BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB160787BL

Integration File: autoint1.e
Quant Time: May 11 03:18:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.940	1952513	19.537 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051024\
Data File : FF014188.D
Signal(s) : FID2B.ch
Acq On : 10 May 2024 20:55
Operator : YP\AJ
Sample : PB160787BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB160787BL

Integration File: autoint1.e
Quant Time: May 11 03:18:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

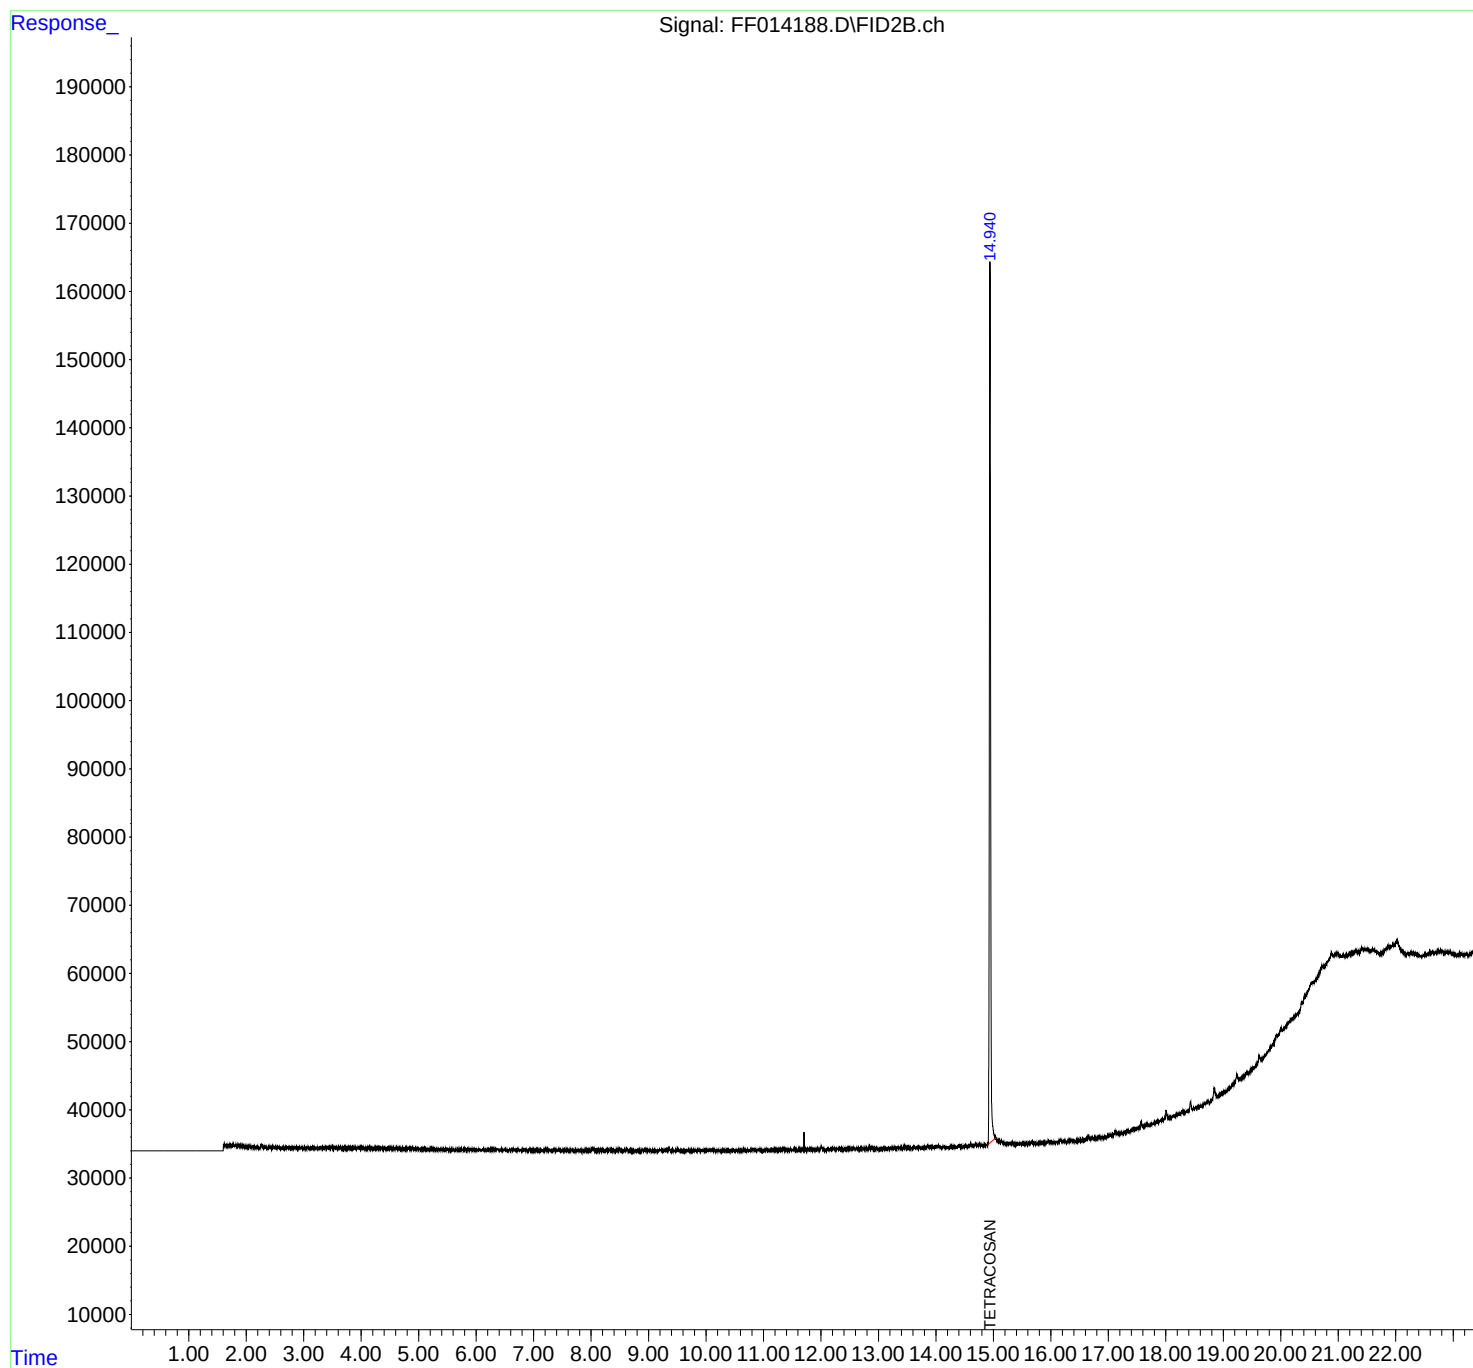

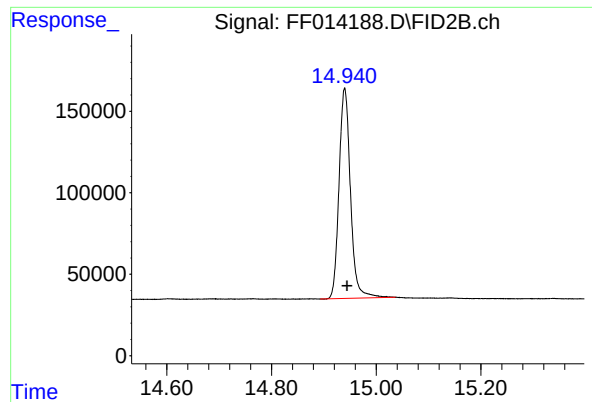

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.940 min
Delta R.T.: -0.005 min
Response: 1952513
Conc: 19.54 ug/ml

Instrument :

FID_F

ClientSampleId :

PB160787BL