

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051220\
Data File : FF006933.D
Signal(s) : FID2B.ch
Acq On : 12 May 2020 06:07
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: May 13 00:56:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	17.618	89116	0.574 ug/ml
14)	N-DOTRIACONTANE	18.446	107972	0.734 ug/ml
15)	N-TETRATRIACONTANE	19.226	131255	0.992 ug/ml
16)	N-HEXATRIACONTANE	19.976	105792	0.879 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051220\
Data File : FF006933.D
Signal(s) : FID2B.ch
Acq On : 12 May 2020 06:07
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: May 13 00:56:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

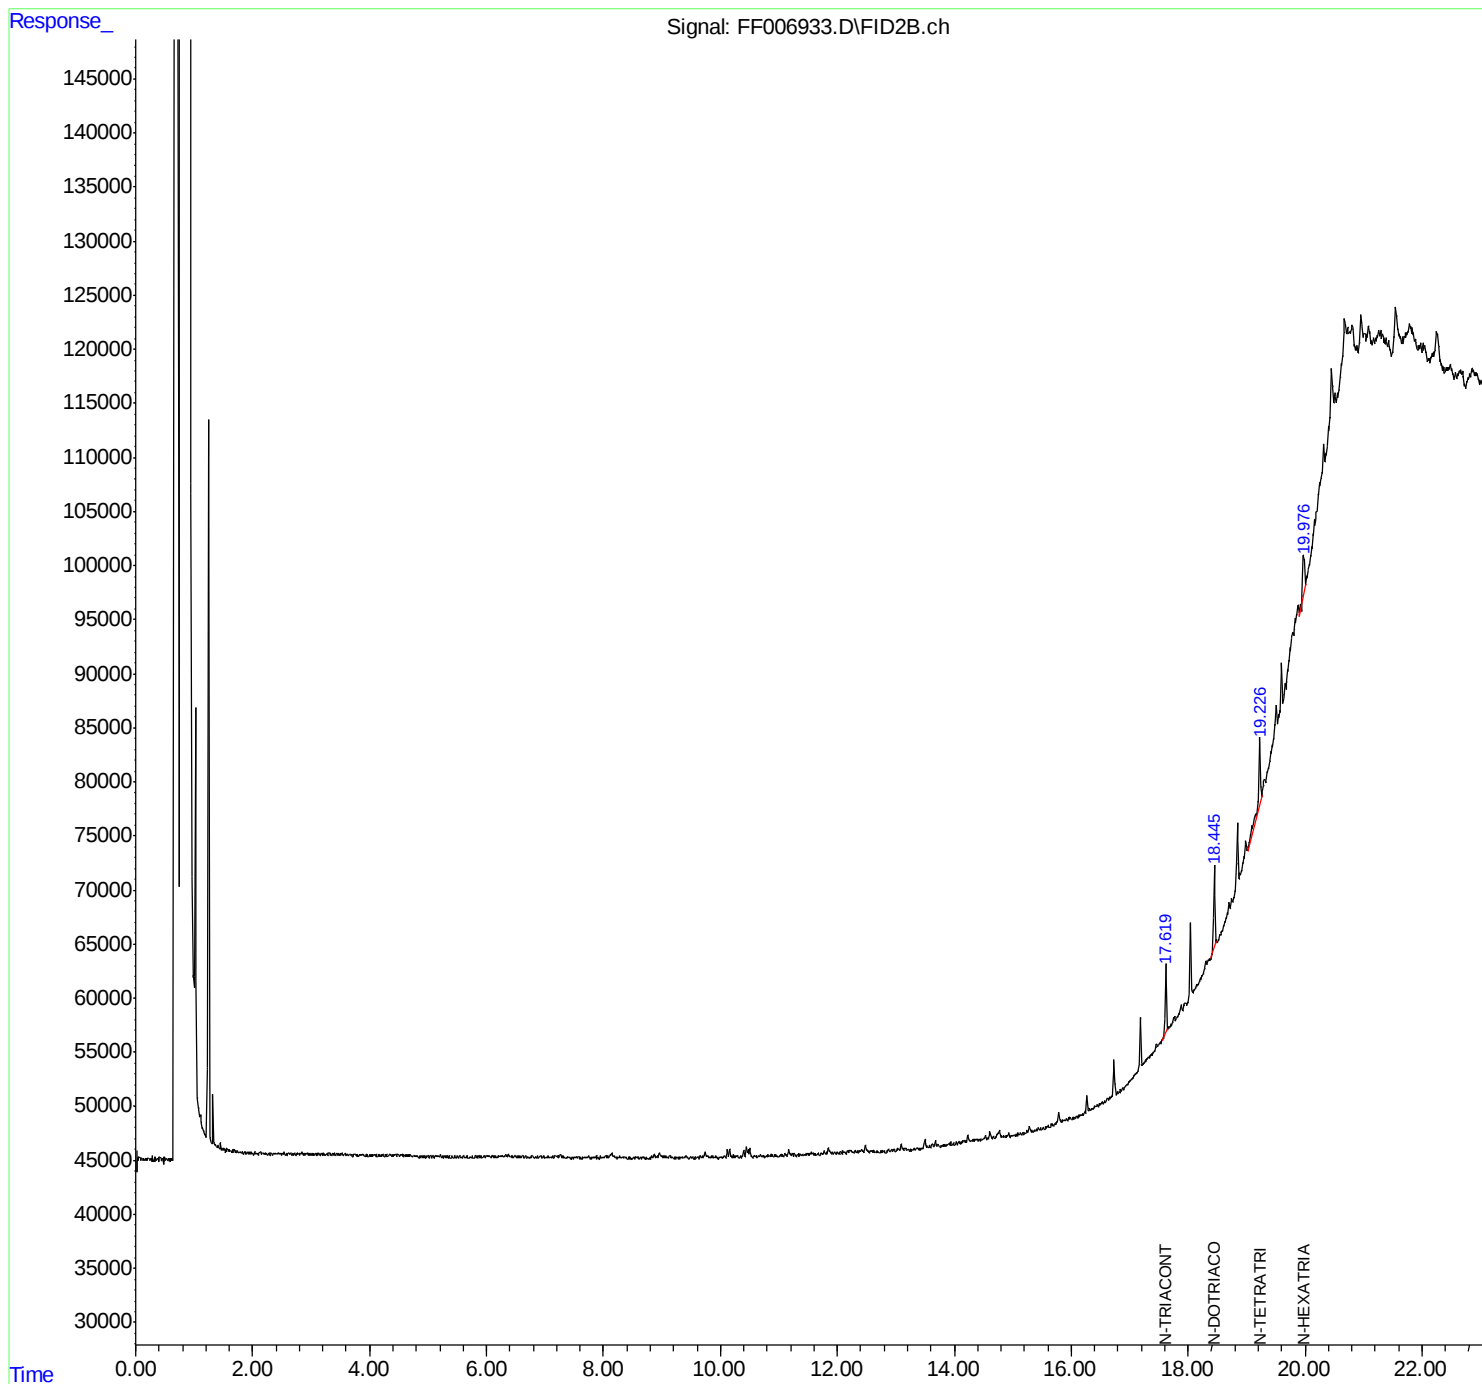


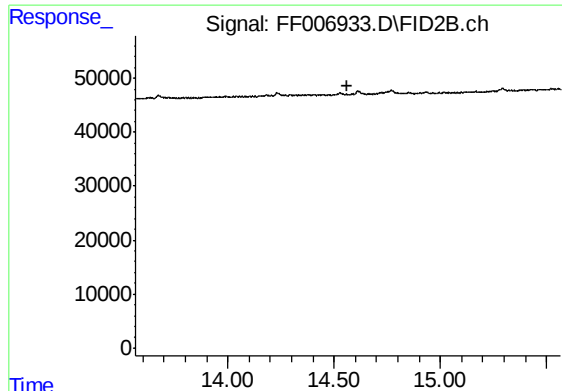

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.565 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

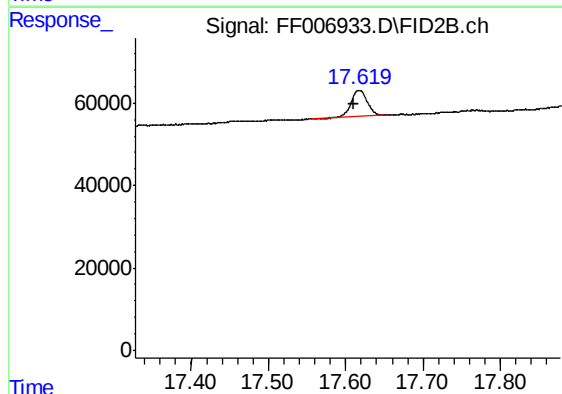


#13 N-TRIACONTANE

R.T.: 17.618 min
Delta R.T.: 0.007 min
Response: 89116
Conc: 0.57 ug/ml

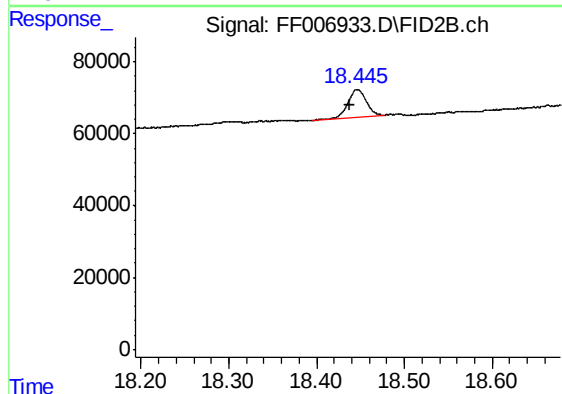


#14 N-DOTRIACONTANE

R.T.: 18.446 min
Delta R.T.: 0.008 min
Response: 107972
Conc: 0.73 ug/ml

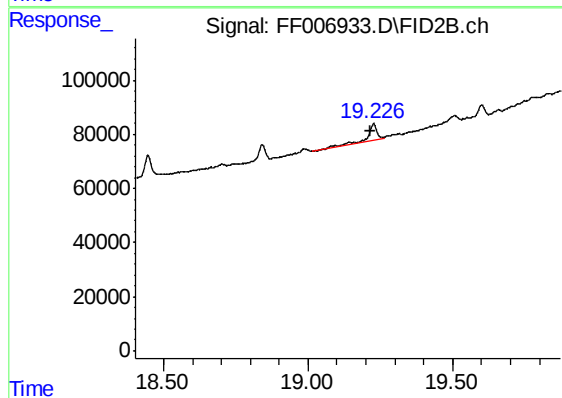

#15 N-TETRATRIACONTANE

R.T.: 19.226 min
Delta R.T.: 0.009 min
Response: 131255
Conc: 0.99 ug/ml

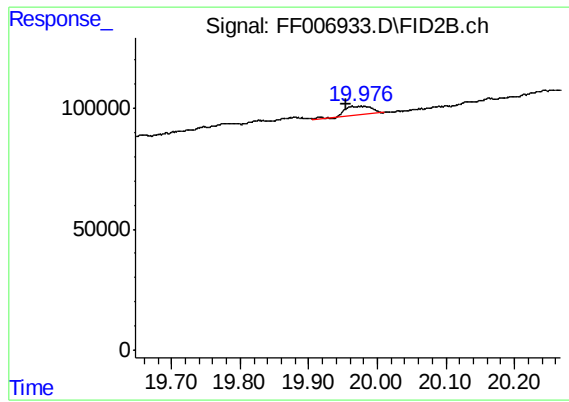

#16 N-HEXATRIACONTANE

R.T.: 19.976 min
Delta R.T.: 0.022 min
Response: 105792
Conc: 0.88 ug/ml

Instrument :
FID_F
ClientSampleId :
MECL2