

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051220\
Data File : FF006934.D
Signal(s) : FID2B.ch
Acq On : 12 May 2020 06:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 13 00:56:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.570	2002006	14.737 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.985	249582	2.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051220\
Data File : FF006934.D
Signal(s) : FID2B.ch
Acq On : 12 May 2020 06:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 13 00:56:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

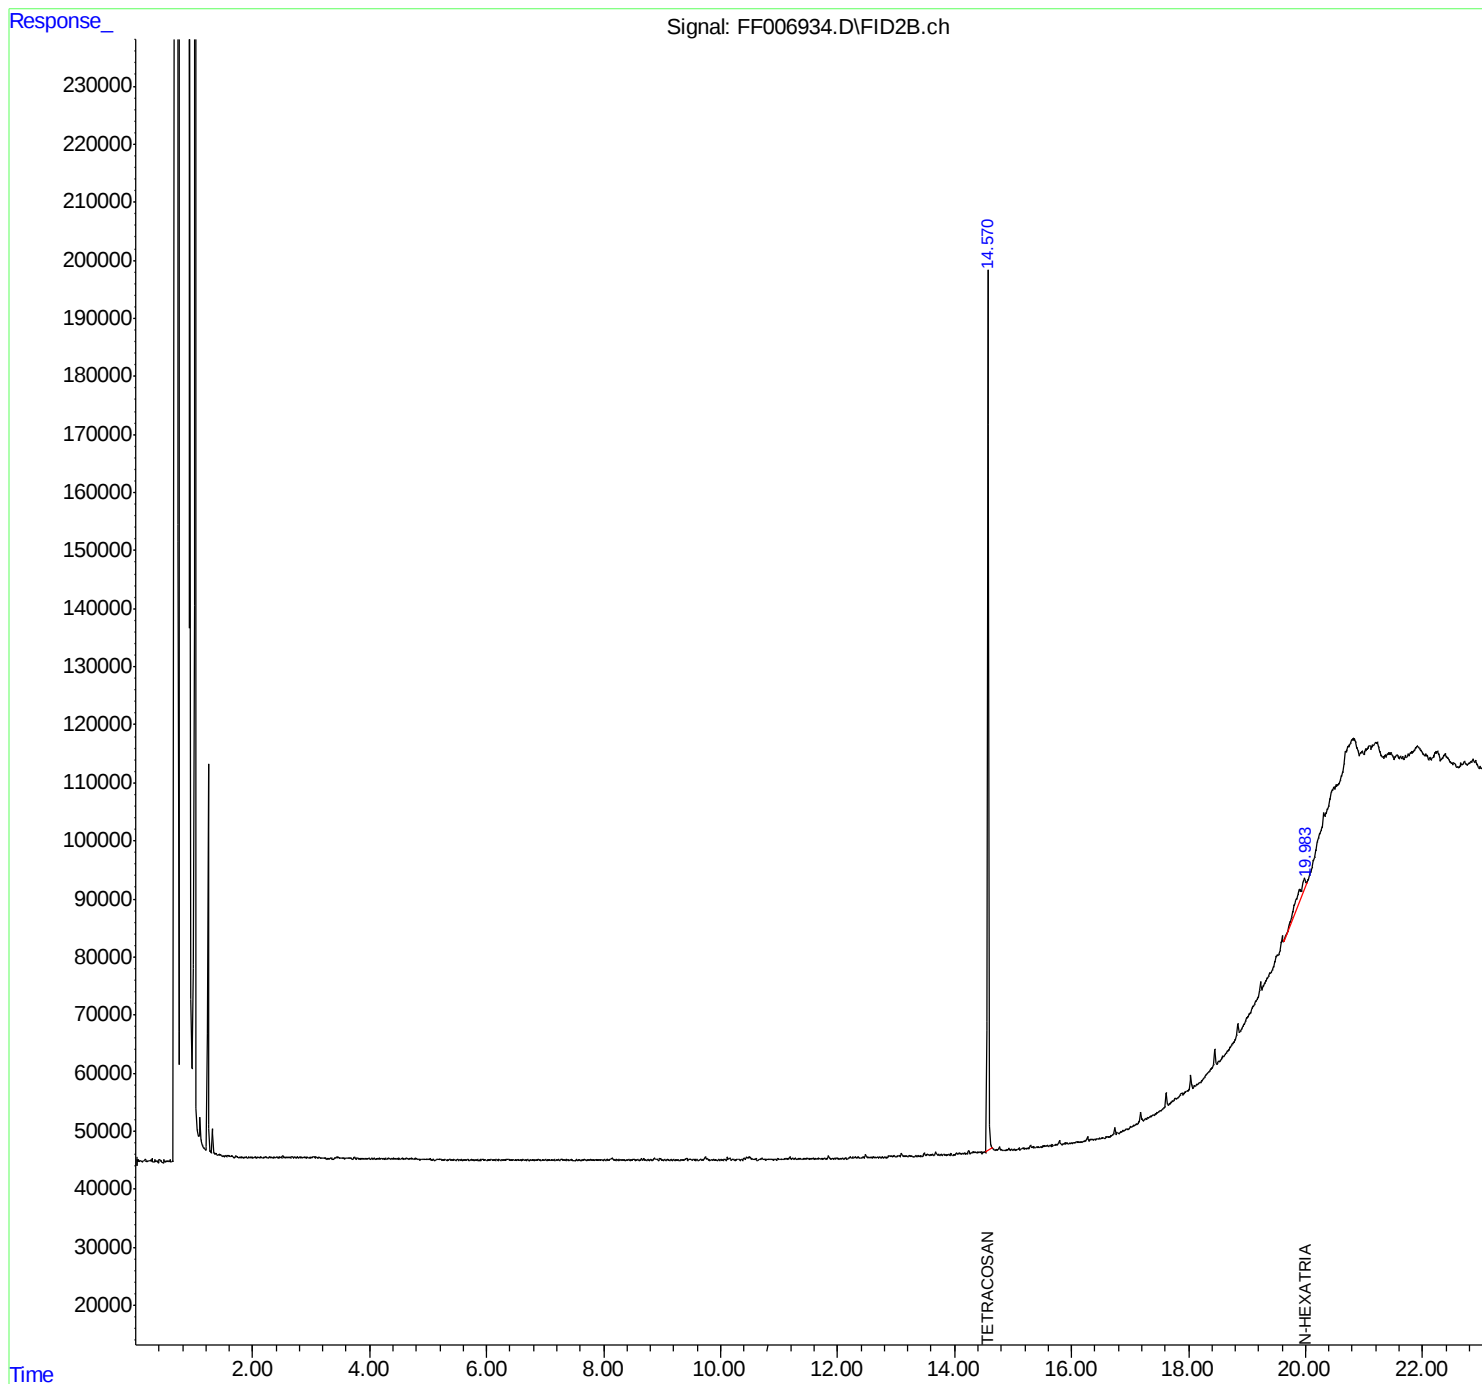


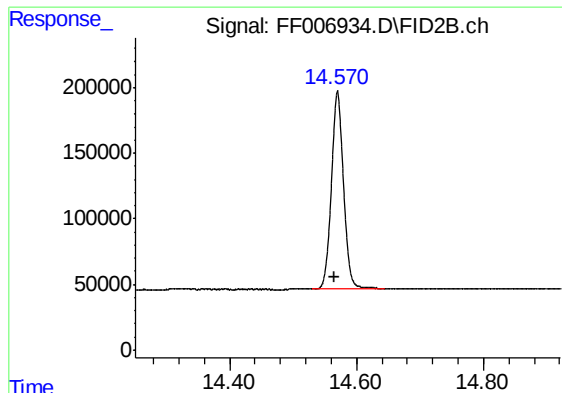

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.570 min
Delta R.T.: 0.005 min
Response: 2002006
Conc: 14.74 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

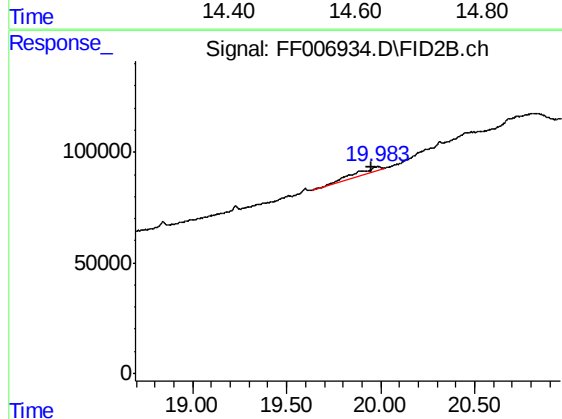

#16 N-HEXATRIACONTANE

R.T.: 19.985 min
Delta R.T.: 0.031 min
Response: 249582
Conc: 2.07 ug/ml