

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006955.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 08:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:11:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.567	2147937	15.812 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	19.958	72206	0.600 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006955.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 08:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:11:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

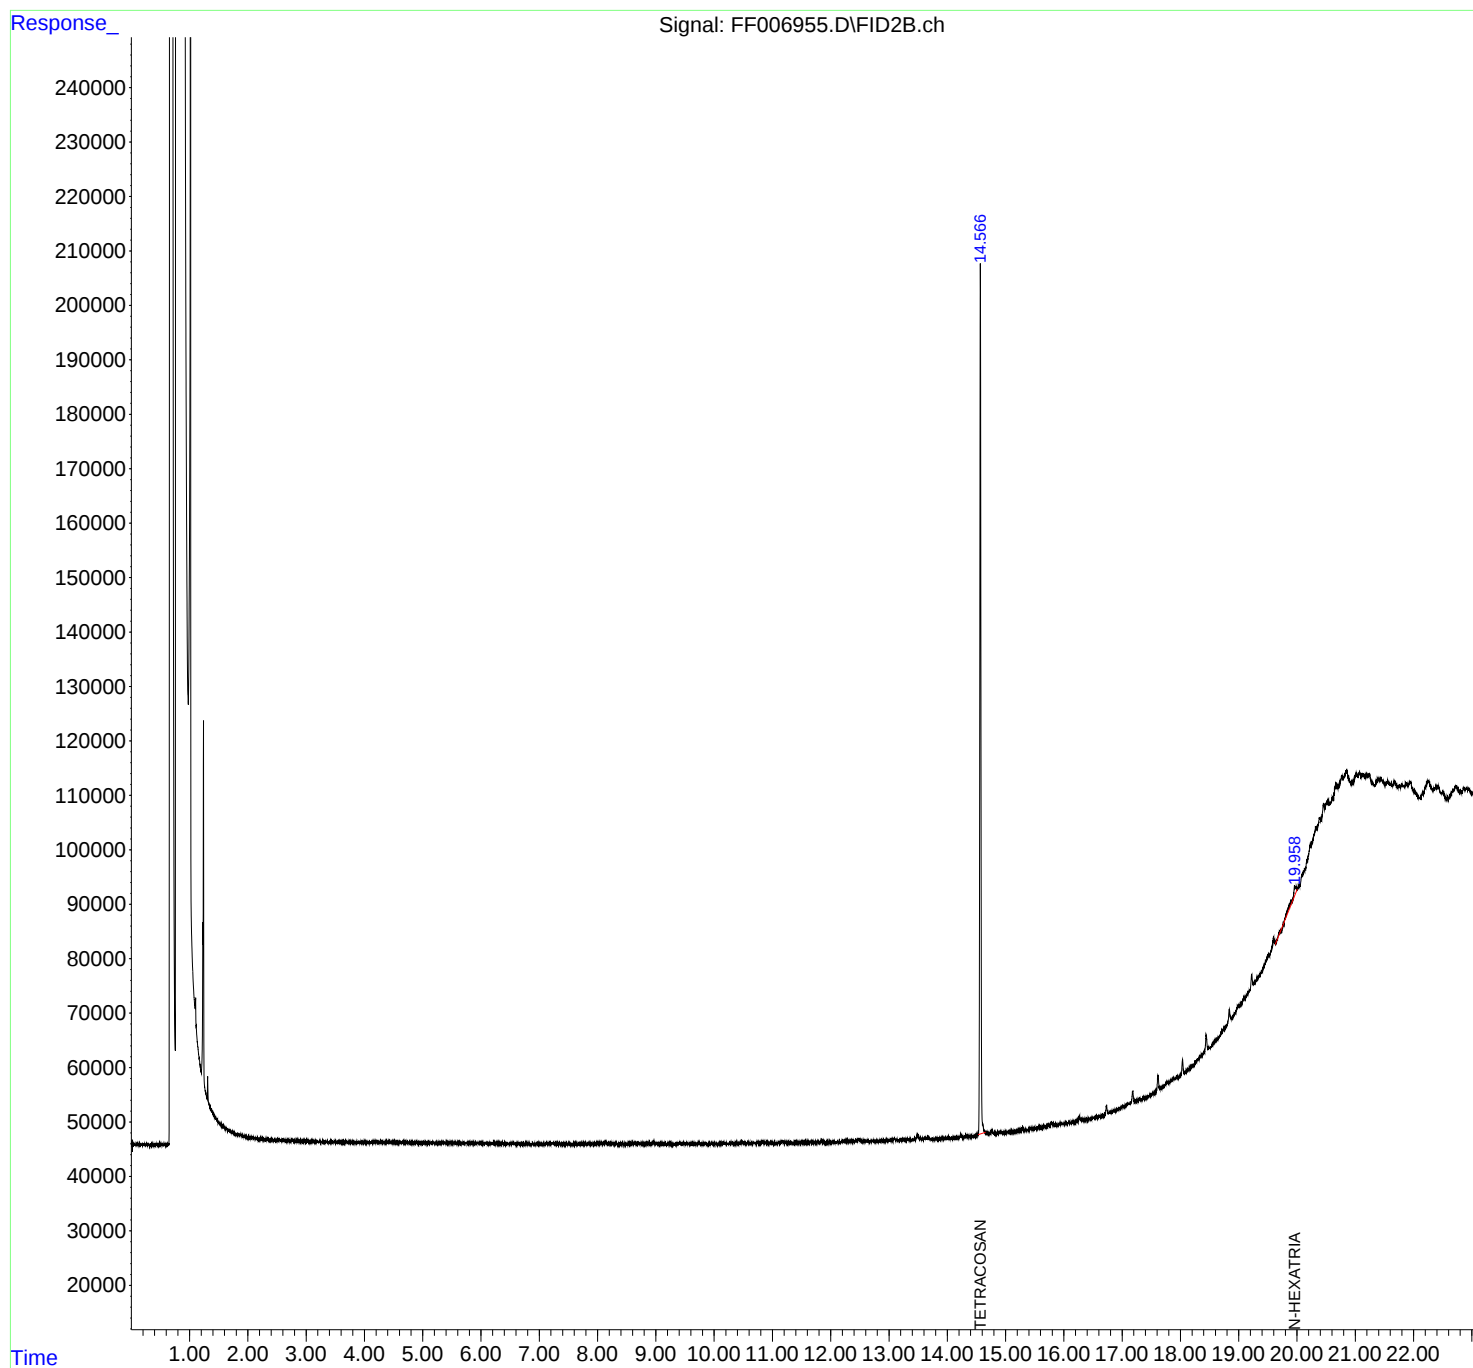


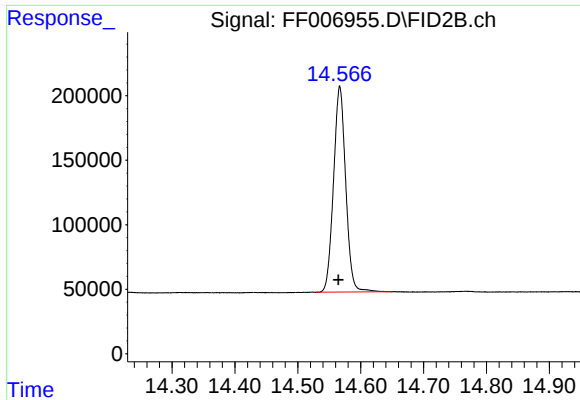

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.567 min
Delta R.T.: 0.002 min
Response: 2147937
Conc: 15.81 ug/ml

Instrument :
FID_F
ClientSampleId :

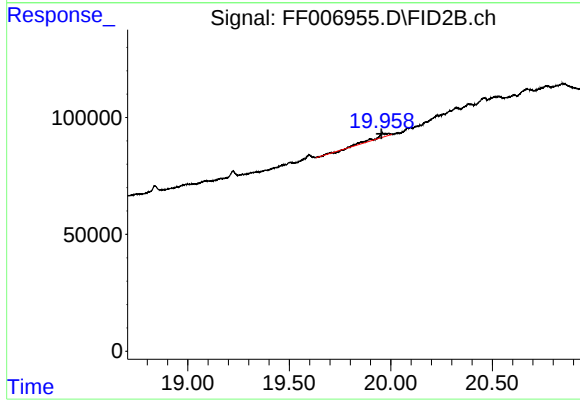

#16 N-HEXATRIACONTANE

R.T.: 19.958 min
Delta R.T.: 0.005 min
Response: 72206
Conc: 0.60 ug/ml