

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
 Data File : FF006957.D
 Signal(s) : FID2B.ch
 Acq On : 13 May 2020 09:35
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 14 05:12:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.346	2796334	19.612 ug/ml
12) N-OCTACOSANE	16.732	2697203	17.499 ug/ml
13) N-TRIACONTANE	17.613	105246	0.678 ug/ml
14) N-DOTRIACONTANE	18.441	147514	1.003 ug/ml
15) N-TETRATRIACONTANE	19.220	78800	0.596 ug/ml
16) N-HEXATRIACONTANE	19.984	194368	1.614 ug/ml
18) N-TETRACONTANE	21.546	246163	2.350 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006957.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 09:35
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:12:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

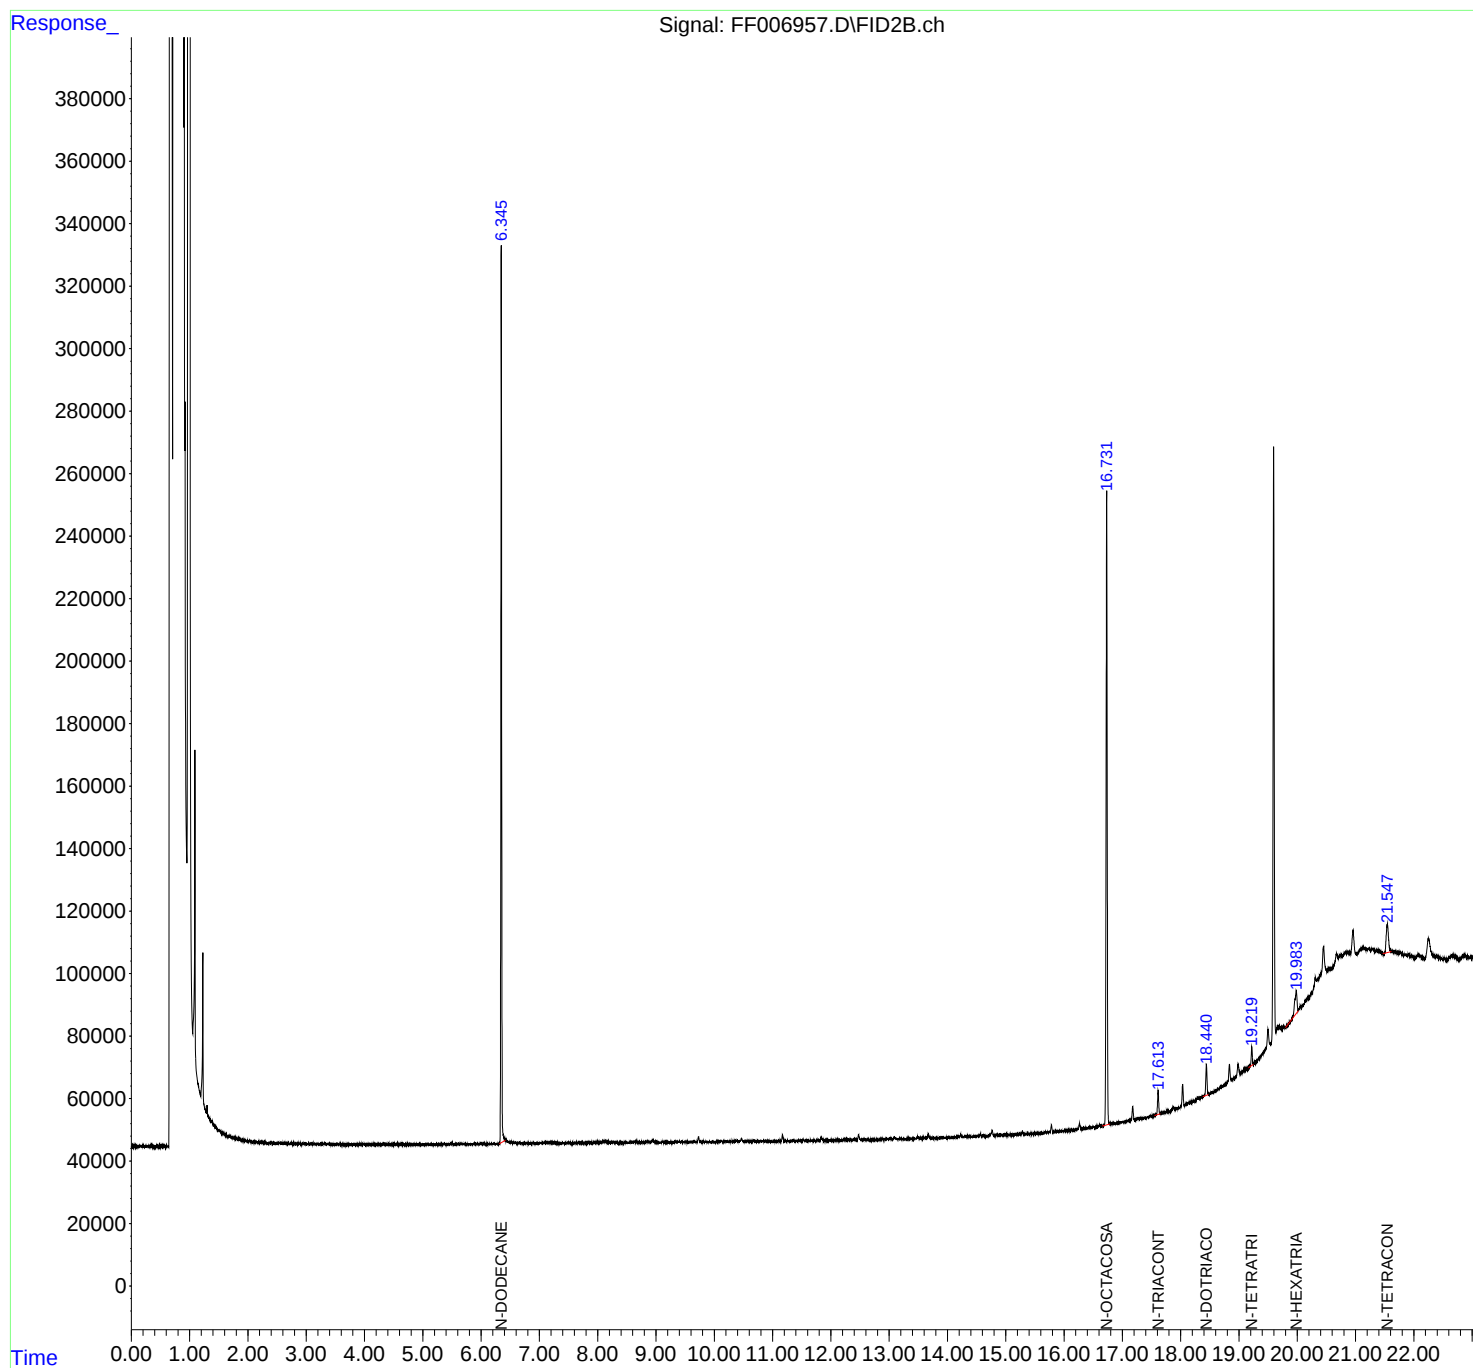


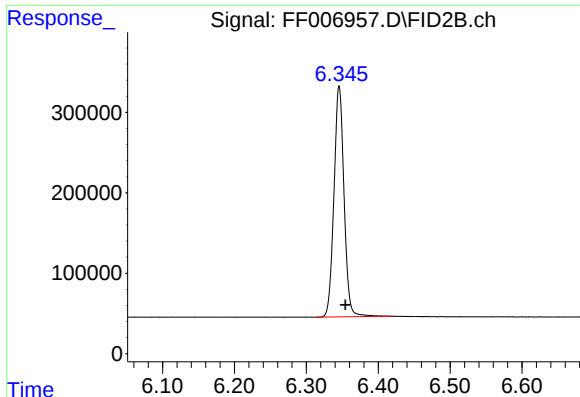

#3 N-DODECANE


R.T.: 6.346 min
Delta R.T.: -0.009 min
Response: 2796334
Conc: 19.61 ug/ml

Instrument :
FID_F
ClientSampleId :

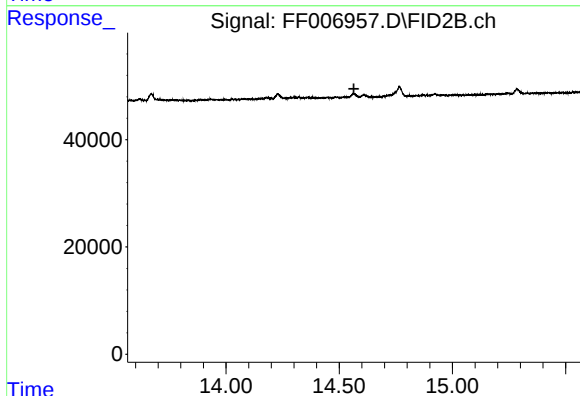


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.565 min
Response: 0
Conc: N.D.

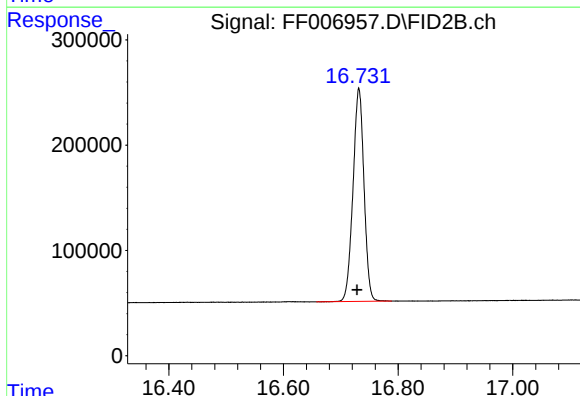


#12 N-OCTACOSANE

R.T.: 16.732 min
Delta R.T.: 0.003 min
Response: 2697203
Conc: 17.50 ug/ml

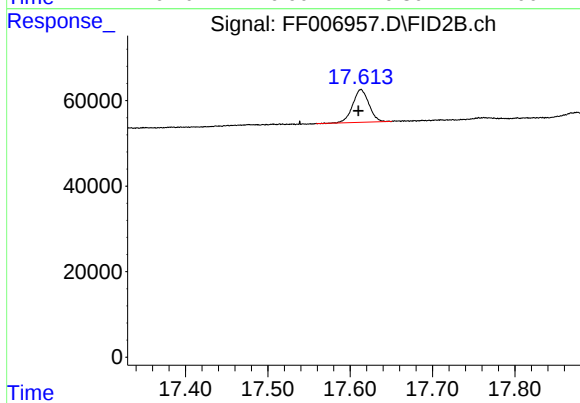

#13 N-TRIACONTANE


R.T.: 17.613 min
Delta R.T.: 0.003 min
Response: 105246
Conc: 0.68 ug/ml

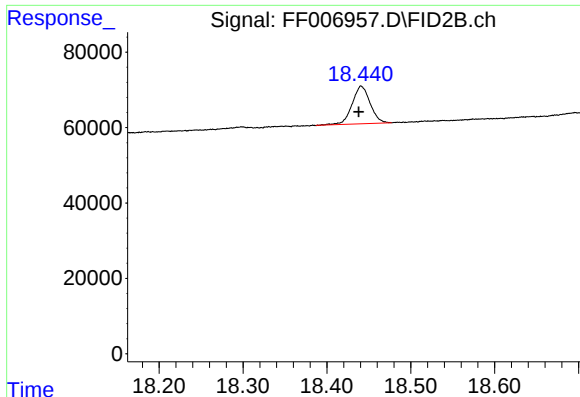

#14 N-DOTRIACONTANE


R.T.: 18.441 min
Delta R.T.: 0.003 min
Response: 147514
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :

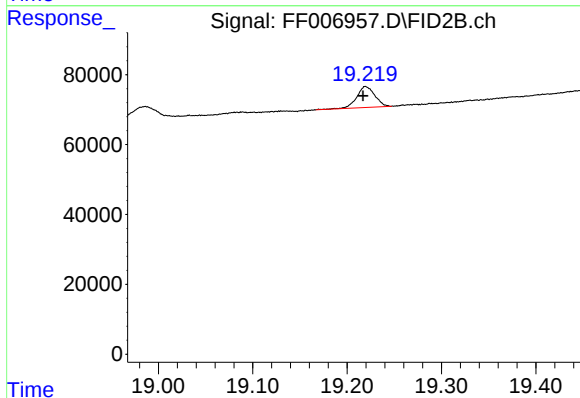


#15 N-TETRATRIACONTANE

R.T.: 19.220 min
Delta R.T.: 0.003 min
Response: 78800
Conc: 0.60 ug/ml

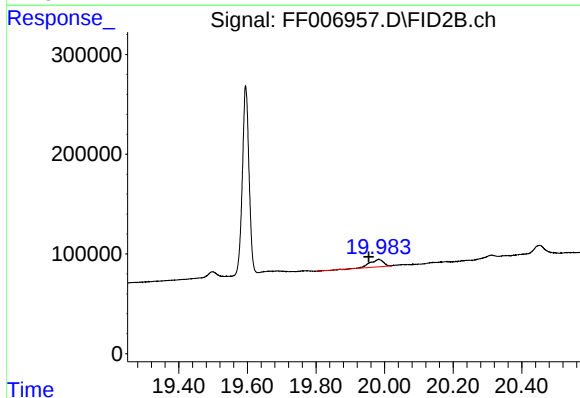

#16 N-HEXATRIACONTANE

R.T.: 19.984 min
Delta R.T.: 0.030 min
Response: 194368
Conc: 1.61 ug/ml

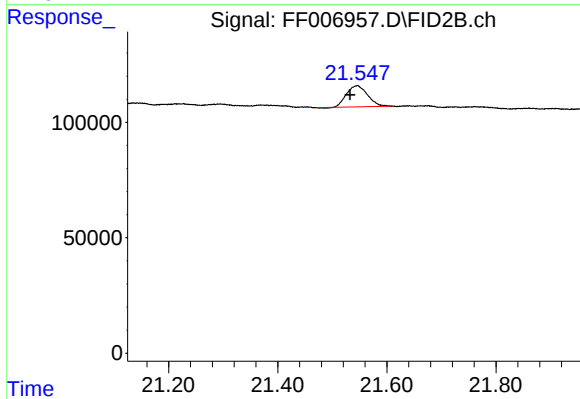

#18 N-TETRACONTANE

R.T.: 21.546 min
Delta R.T.: 0.013 min
Response: 246163
Conc: 2.35 ug/ml