

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
 Data File : FF006961.D
 Signal(s) : FID2B.ch
 Acq On : 13 May 2020 14:52
 Operator : DD\AJ
 Sample : L2500-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 14 05:13:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.566	176111	1.296 ug/ml
Target Compounds			
7) N-EICOSANE	12.474	163373	1.057 ug/ml
10) N-TETRACOSANE	14.768	464099	2.978 ug/ml
12) N-OCTACOSANE	16.730	73826	0.479 ug/ml
13) N-TRIACONTANE	17.614	283152	1.825 ug/ml
14) N-DOTRIACONTANE	18.442	271702	1.847 ug/ml
15) N-TETRATRIACONTANE	19.222	62637	0.473 ug/ml
16) N-HEXATRIACONTANE	19.959	160836	1.336 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006961.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 14:52
Operator : DD\AJ
Sample : L2500-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:13:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

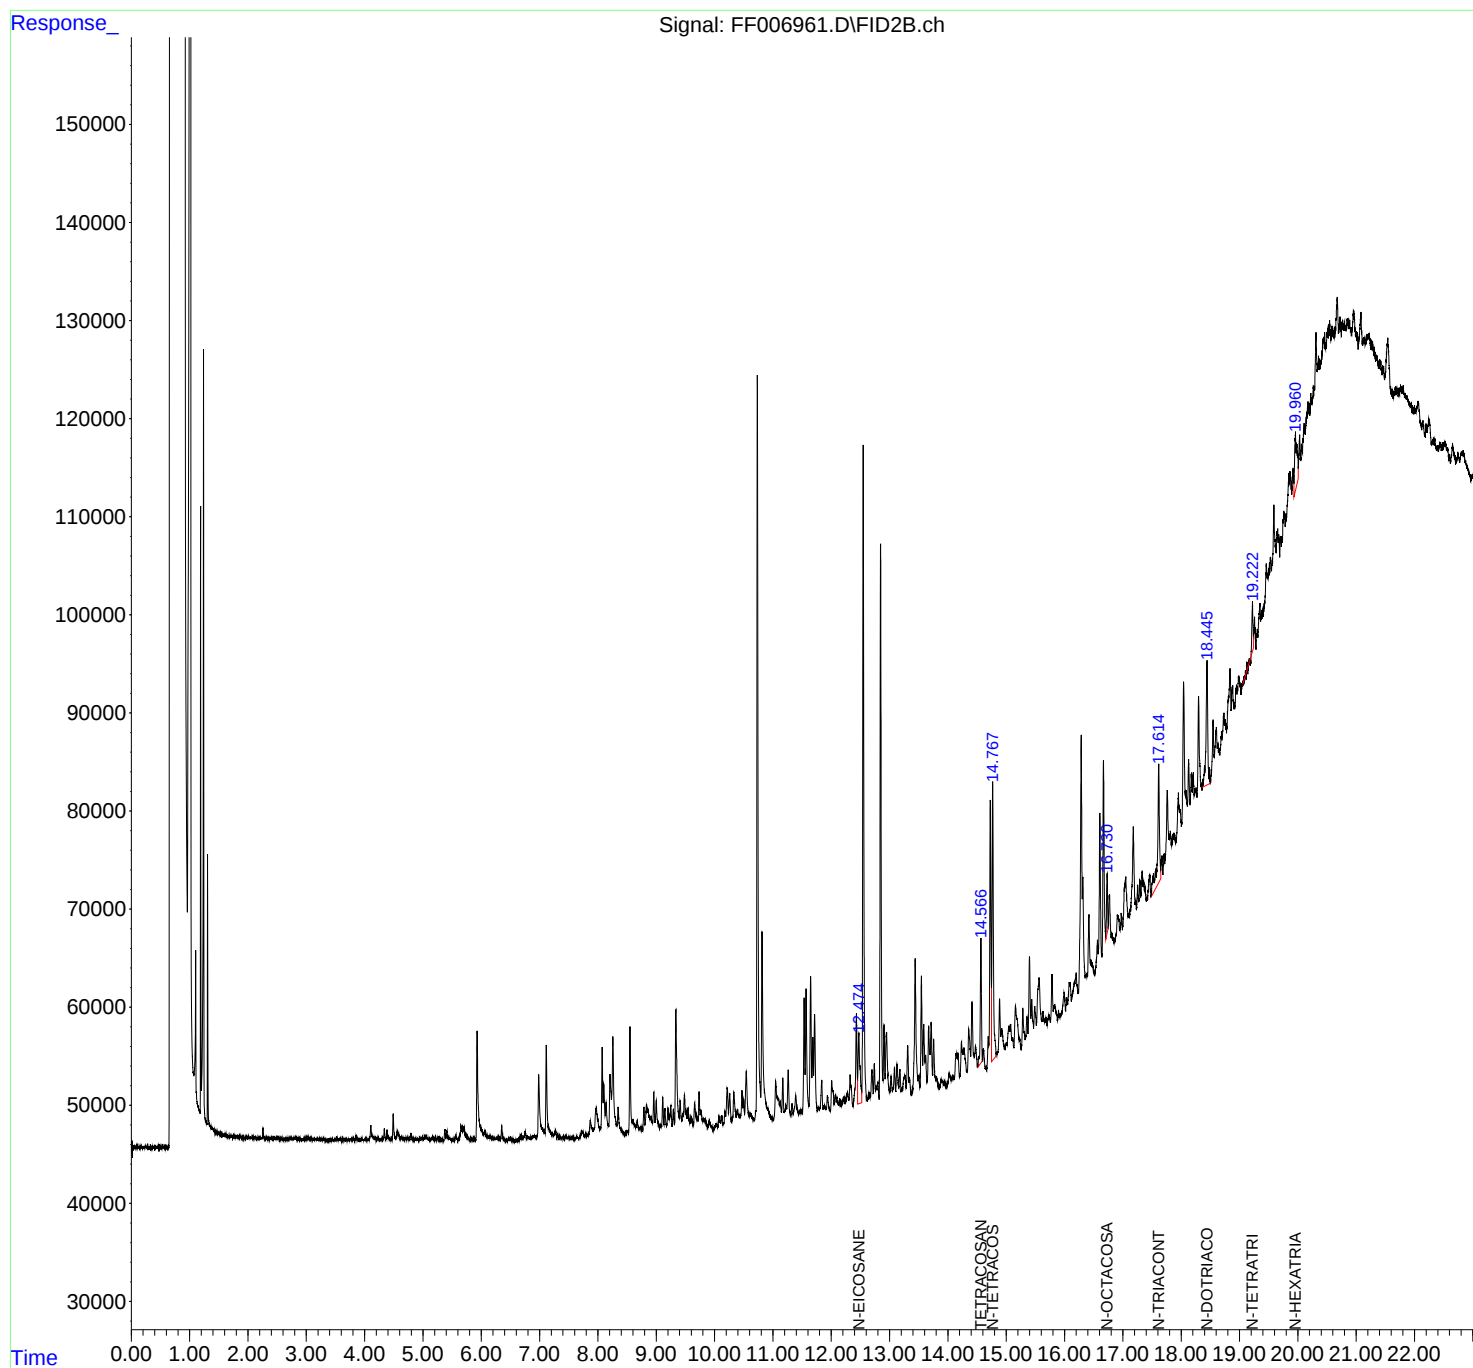


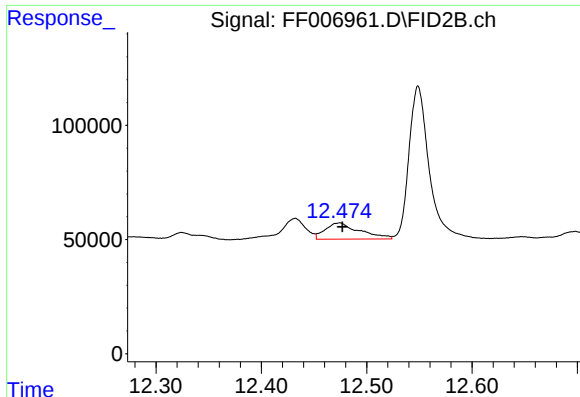

#7 N-EICOSANE


R.T.: 12.474 min
Delta R.T.: -0.003 min
Response: 163373
Conc: 1.06 ug/ml

Instrument :
FID_F
ClientSampleId :

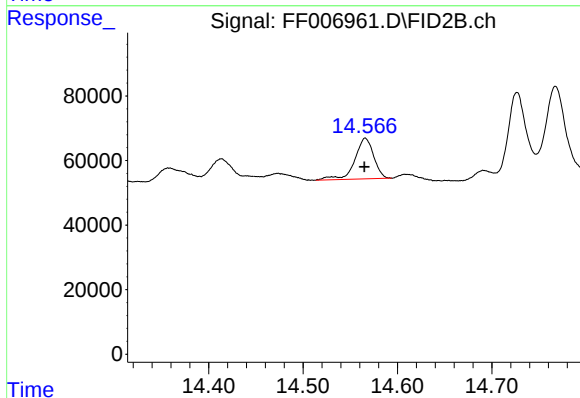


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.566 min
Delta R.T.: 0.001 min
Response: 176111
Conc: 1.30 ug/ml

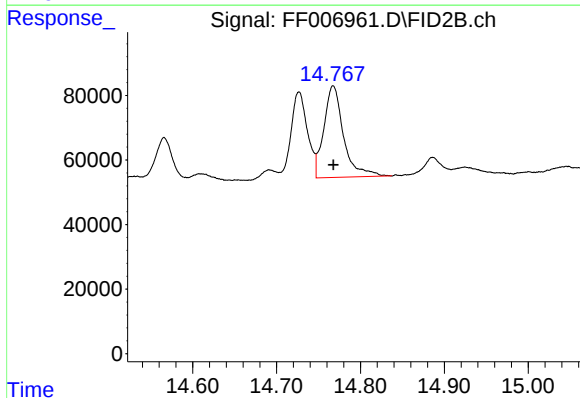


#10 N-TETRACOSANE

R.T.: 14.768 min
Delta R.T.: 0.000 min
Response: 464099
Conc: 2.98 ug/ml

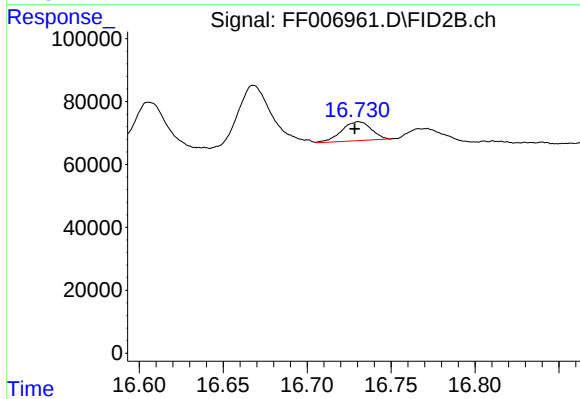

#12 N-OCTACOSANE


R.T.: 16.730 min
Delta R.T.: 0.002 min
Response: 73826
Conc: 0.48 ug/ml

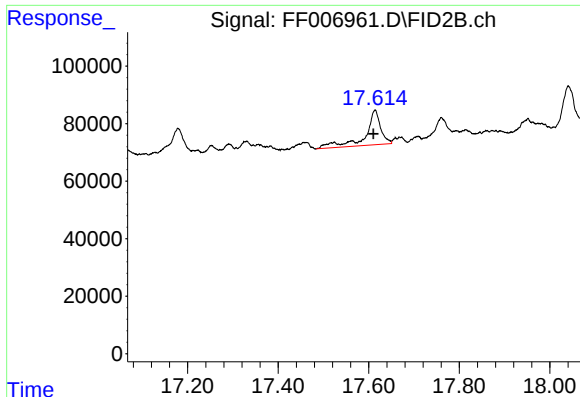

#13 N-TRIACONTANE


R.T.: 17.614 min
Delta R.T.: 0.004 min
Response: 283152
Conc: 1.82 ug/ml

Instrument :
FID_F
ClientSampleId :

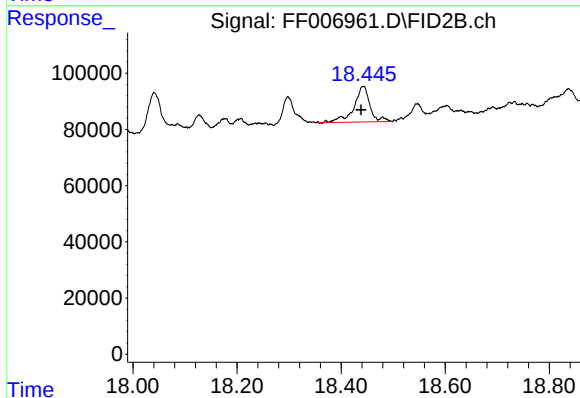


#14 N-DOTRIACONTANE

R.T.: 18.442 min
Delta R.T.: 0.004 min
Response: 271702
Conc: 1.85 ug/ml

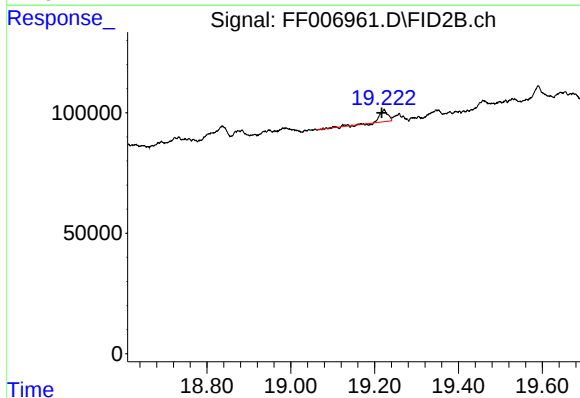

#15 N-TETRATRIACONTANE

R.T.: 19.222 min
Delta R.T.: 0.005 min
Response: 62637
Conc: 0.47 ug/ml

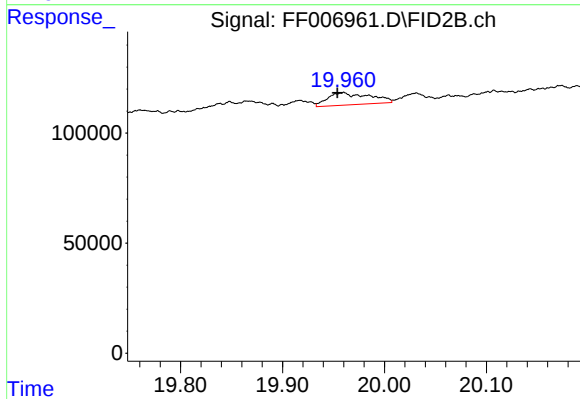

#16 N-HEXATRIACONTANE

R.T.: 19.959 min
Delta R.T.: 0.005 min
Response: 160836
Conc: 1.34 ug/ml