

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
 Data File : FF006962.D
 Signal(s) : FID2B.ch
 Acq On : 13 May 2020 15:22
 Operator : DD\AJ
 Sample : L2505-01 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 14 05:13:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.566	151297	1.114 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.769	180890	1.161 ug/ml
12) N-OCTACOSANE	16.731	79260	0.514 ug/ml
13) N-TRIACONTANE	17.615	148887	0.959 ug/ml
14) N-DOTRIACONTANE	18.441	222717	1.514 ug/ml
15) N-TETRATRIACONTANE	19.220	53898	0.407 ug/ml
16) N-HEXATRIACONTANE	19.960	87682	0.728 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006962.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 15:22
Operator : DD\AJ
Sample : L2505-01 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:13:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

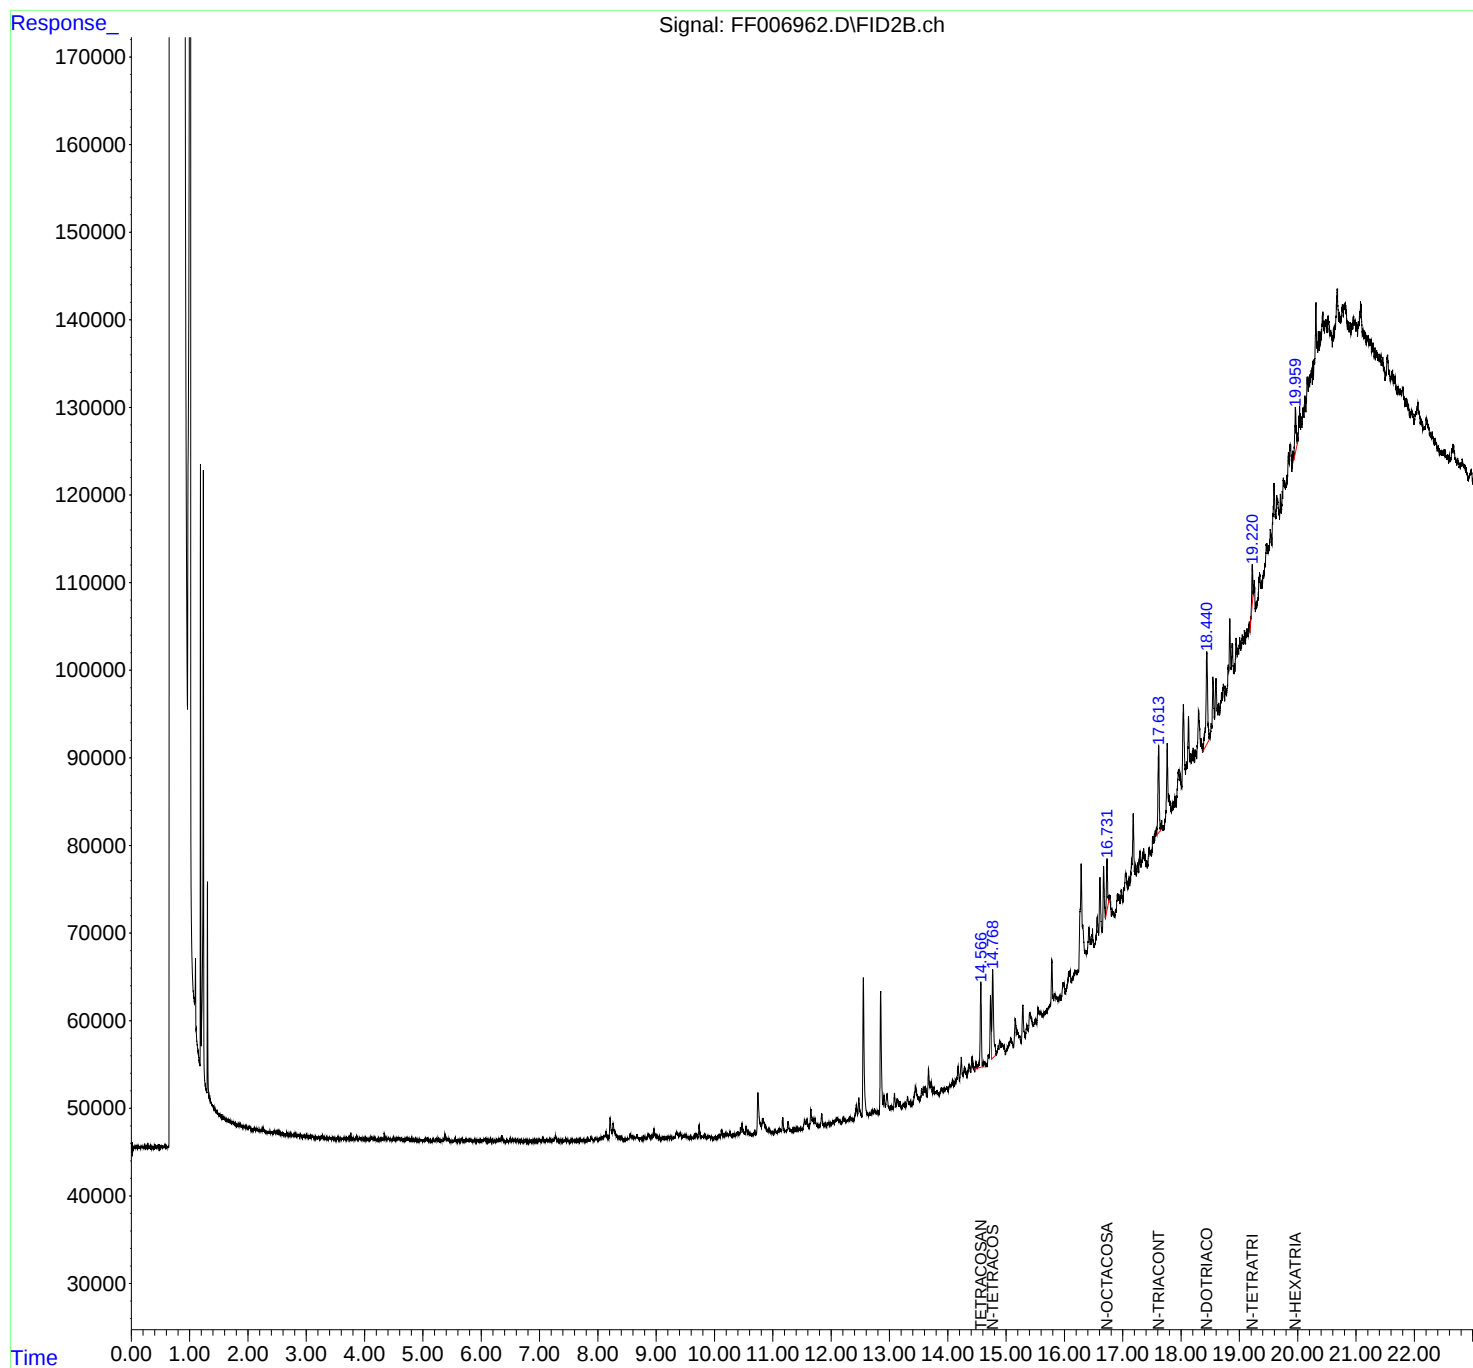


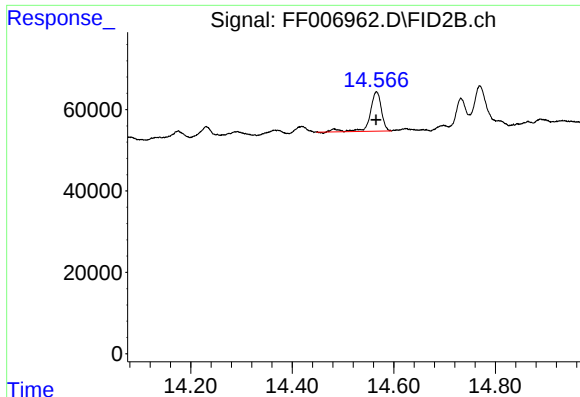

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.566 min
Delta R.T.: 0.000 min
Response: 151297
Conc: 1.11 ug/ml

Instrument :
FID_F
ClientSampleId :

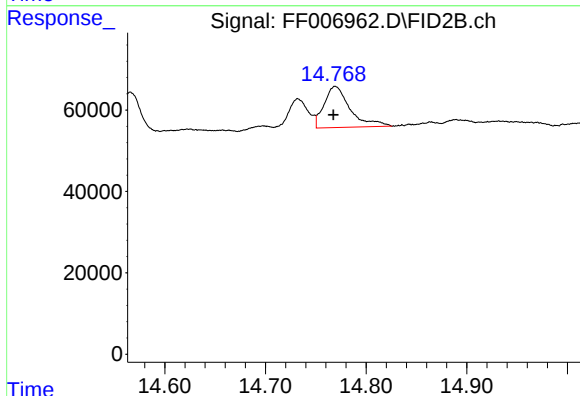


#10 N-TETRACOSANE

R.T.: 14.769 min
Delta R.T.: 0.002 min
Response: 180890
Conc: 1.16 ug/ml

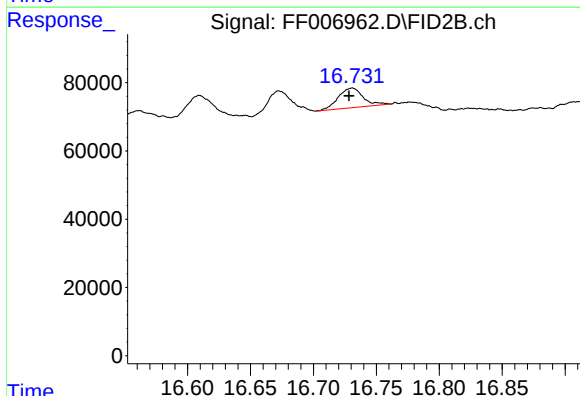


#12 N-OCTACOSANE

R.T.: 16.731 min
Delta R.T.: 0.002 min
Response: 79260
Conc: 0.51 ug/ml

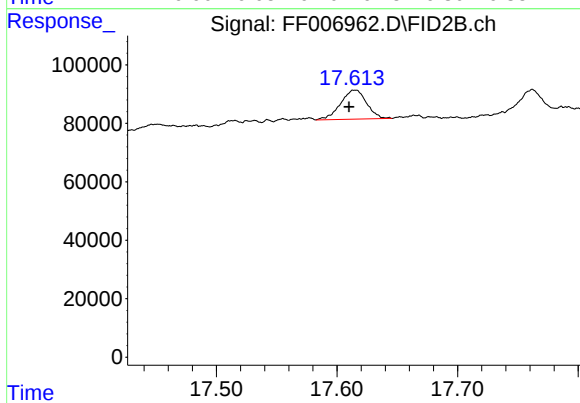

#13 N-TRIACONTANE


R.T.: 17.615 min
Delta R.T.: 0.005 min
Response: 148887
Conc: 0.96 ug/ml

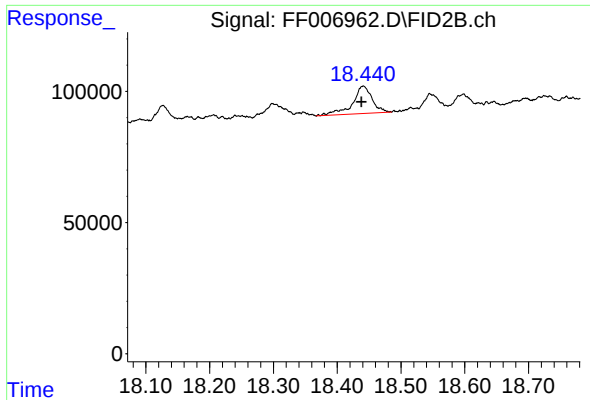

#14 N-DOTRIACONTANE


R.T.: 18.441 min
Delta R.T.: 0.003 min
Response: 222717
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :

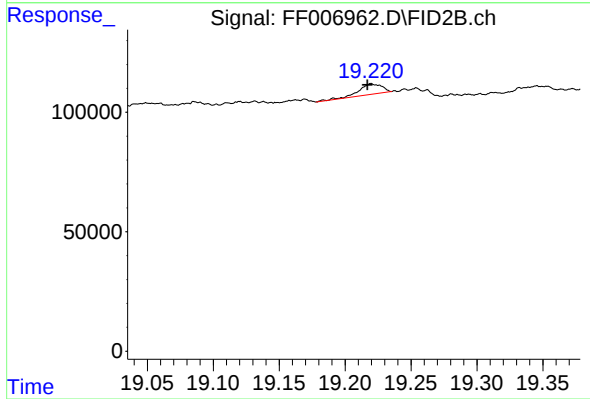

#15 N-TETRATRIACONTANE

R.T.: 19.220 min
Delta R.T.: 0.003 min
Response: 53898
Conc: 0.41 ug/ml

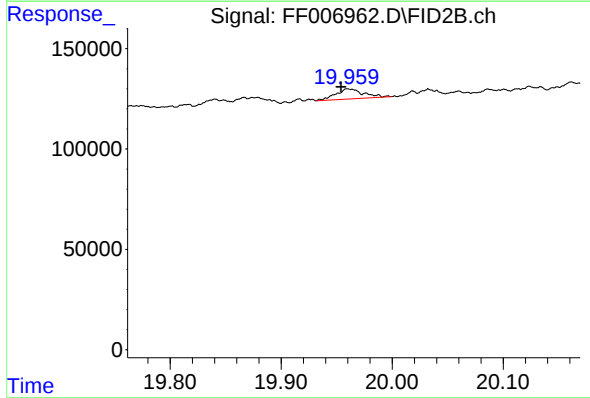

#16 N-HEXATRIACONTANE

R.T.: 19.960 min
Delta R.T.: 0.006 min
Response: 87682
Conc: 0.73 ug/ml