

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
 Data File : FF006967.D
 Signal(s) : FID2B.ch
 Acq On : 13 May 2020 17:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 14 05:14:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.566	2106411	15.506 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.443	70149	0.477 ug/ml
15) N-TETRATRIACONTANE	19.218	133469	1.009 ug/ml
16) N-HEXATRIACONTANE	19.984	193075	1.604 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006967.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 17:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:14:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

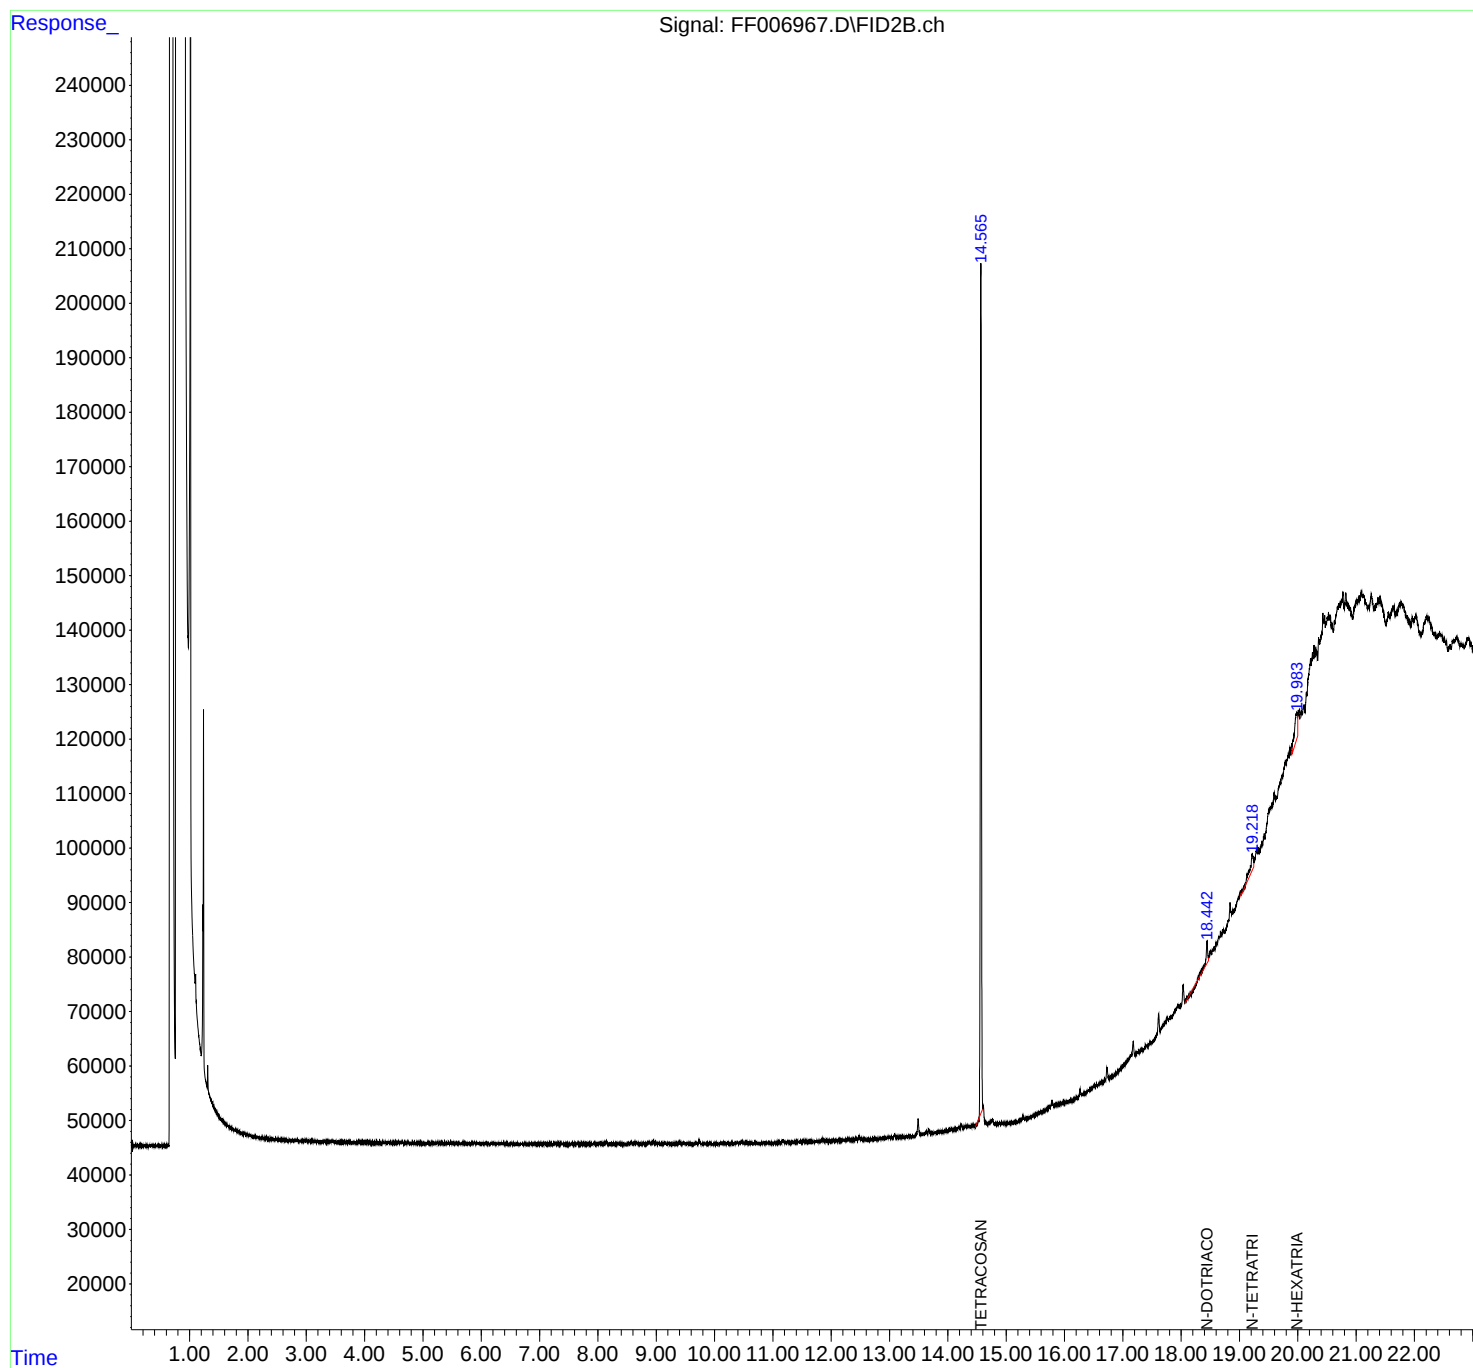


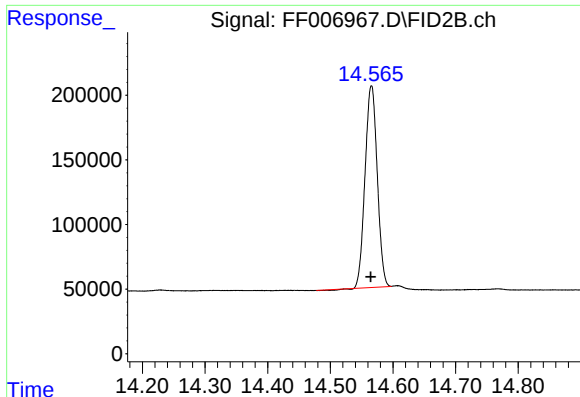

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.566 min
Delta R.T.: 0.000 min
Response: 2106411
Conc: 15.51 ug/ml

Instrument :
FID_F
ClientSampleId :

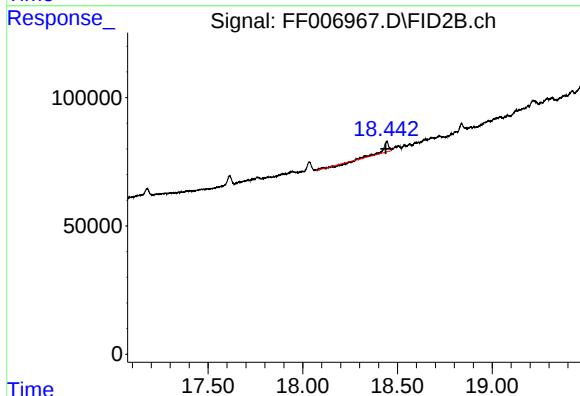


#14 N-DOTRIACONTANE

R.T.: 18.443 min
Delta R.T.: 0.005 min
Response: 70149
Conc: 0.48 ug/ml

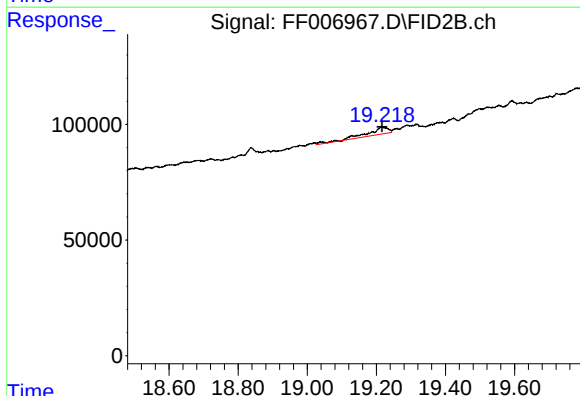

#15 N-TETRATRIACONTANE

R.T.: 19.218 min
Delta R.T.: 0.001 min
Response: 133469
Conc: 1.01 ug/ml

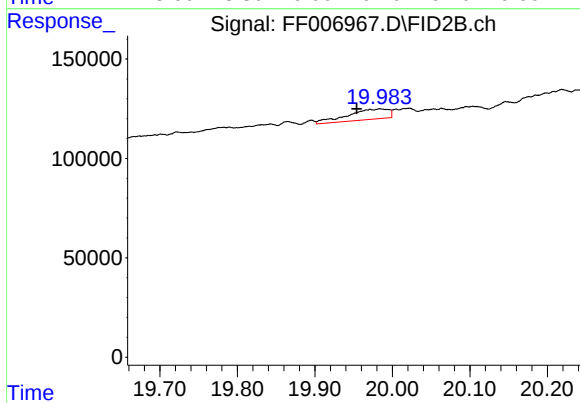

#16 N-HEXATRIACONTANE

R.T.: 19.984 min
Delta R.T.: 0.030 min
Response: 193075
Conc: 1.60 ug/ml