

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
 Data File : FF006960.D
 Signal(s) : FID2B.ch
 Acq On : 13 May 2020 14:22
 Operator : DD\AJ
 Sample : PB128848BS
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB128848BS

Integration File: autoint1.e
 Quant Time: May 14 05:13:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
 Quant Title :
 QLast Update : Wed Apr 29 02:00:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.565	2035996	14.988 ug/ml
Target Compounds			
2) N-DECANE	4.337	2424346	17.603 ug/ml
3) N-DODECANE	6.351	2479814	17.392 ug/ml
4) N-TETRADECANE	8.140	2461014	16.945 ug/ml
5) N-HEXADECANE	9.735	2469463	16.763 ug/ml
6) N-OCTADECANE	11.172	2540358	16.310 ug/ml
7) N-EICOSANE	12.476	2451951	15.864 ug/ml
8) N-DOCOSANE	13.671	2430799	15.519 ug/ml
10) N-TETRACOSANE	14.769	2376859	15.250 ug/ml
11) N-HEXACOSANE	15.785	2332072	15.092 ug/ml
12) N-OCTACOSANE	16.732	2315468	15.023 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051320\
Data File : FF006960.D
Signal(s) : FID2B.ch
Acq On : 13 May 2020 14:22
Operator : DD\AJ
Sample : PB128848BS
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB128848BS

Integration File: autoint1.e
Quant Time: May 14 05:13:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042820.M
Quant Title :
QLast Update : Wed Apr 29 02:00:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

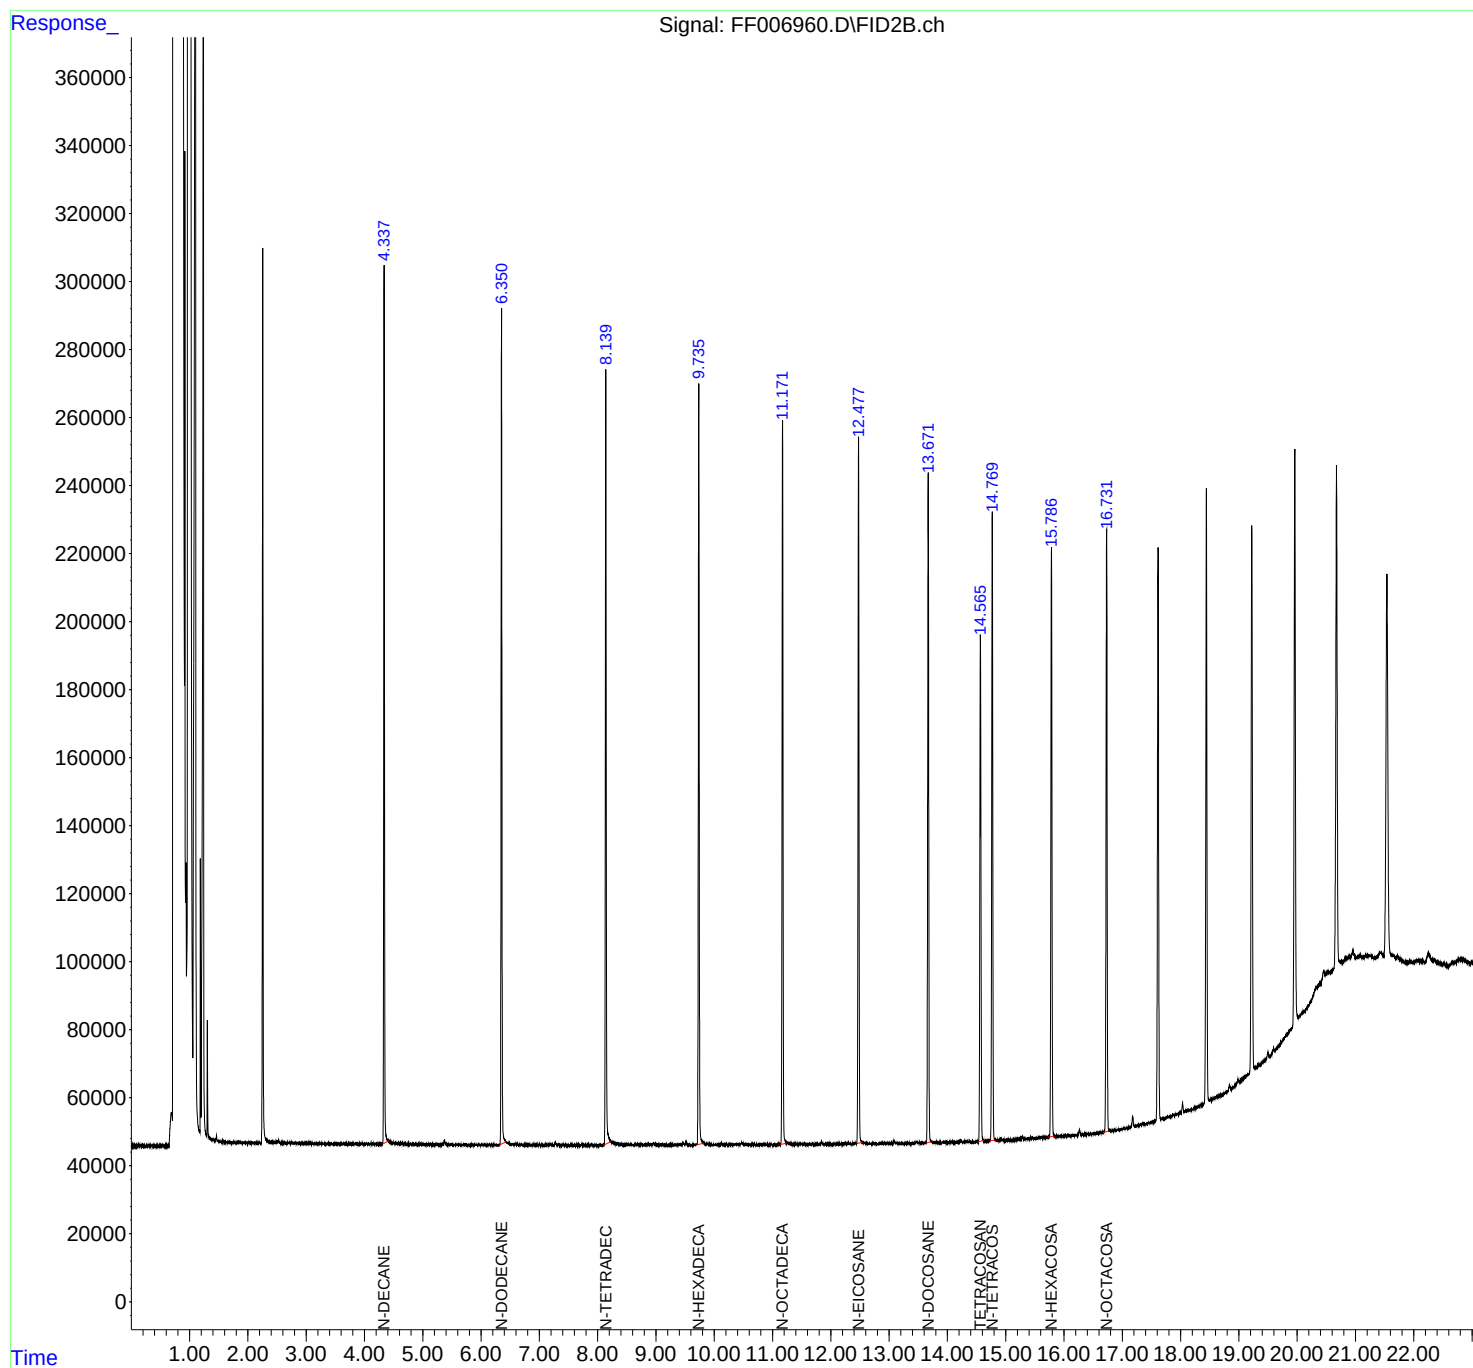


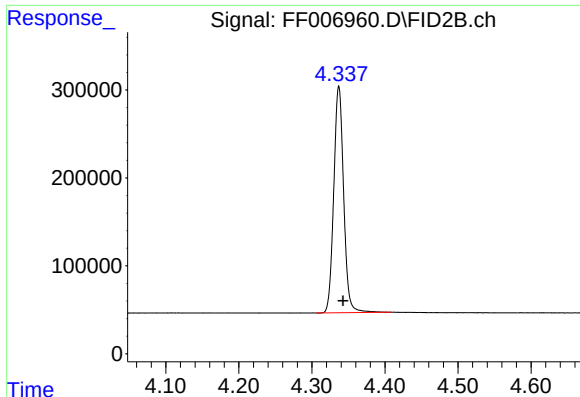

#2 N-DECANE


R.T.: 4.337 min
Delta R.T.: -0.006 min
Response: 2424346
Conc: 17.60 ug/ml

Instrument :
FID_F
ClientSampleId :
PB128848BS

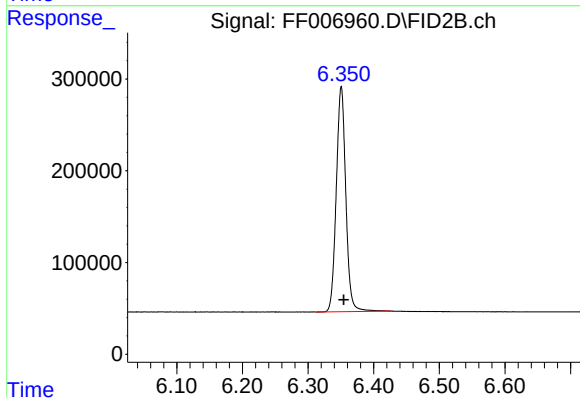


#3 N-DODECANE

R.T.: 6.351 min
Delta R.T.: -0.004 min
Response: 2479814
Conc: 17.39 ug/ml

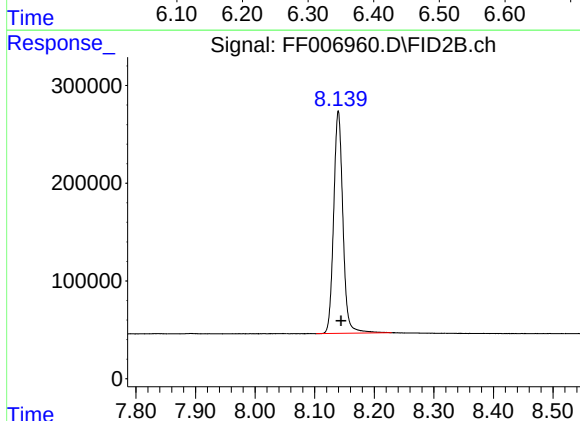


#4 N-TETRADECANE

R.T.: 8.140 min
Delta R.T.: -0.005 min
Response: 2461014
Conc: 16.95 ug/ml

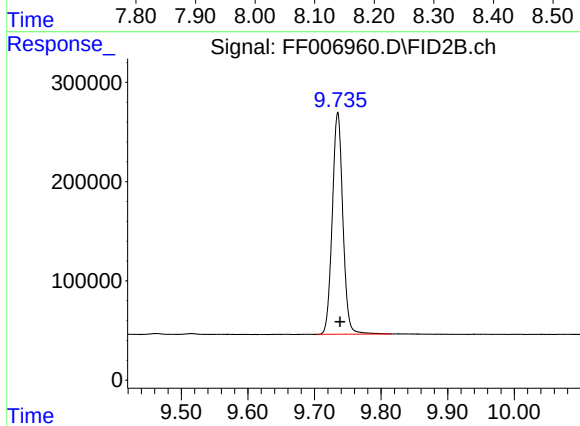

#5 N-HEXADECANE


R.T.: 9.735 min
Delta R.T.: -0.003 min
Response: 2469463
Conc: 16.76 ug/ml

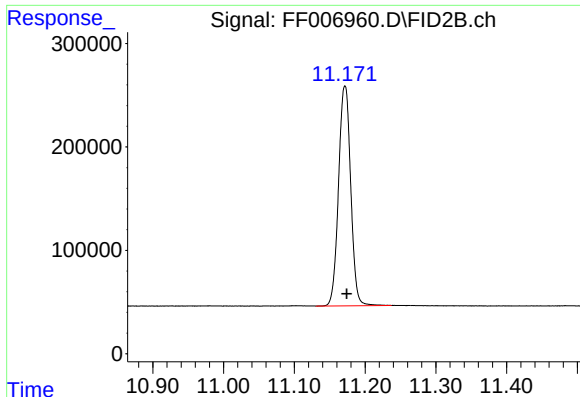

#6 N-OCTADECANE


R.T.: 11.172 min
Delta R.T.: -0.003 min
Response: 2540358
Conc: 16.31 ug/ml

Instrument :
FID_F
ClientSampleId :
PB128848BS

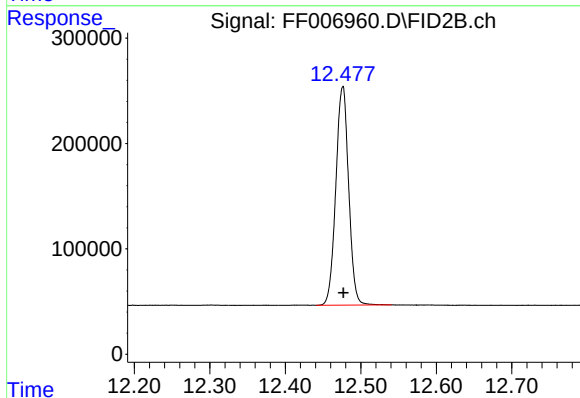


#7 N-EICOSANE

R.T.: 12.476 min
Delta R.T.: 0.000 min
Response: 2451951
Conc: 15.86 ug/ml

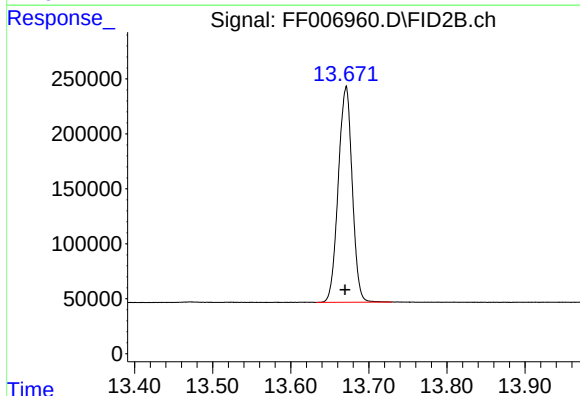


#8 N-DOCOSANE

R.T.: 13.671 min
Delta R.T.: 0.002 min
Response: 2430799
Conc: 15.52 ug/ml

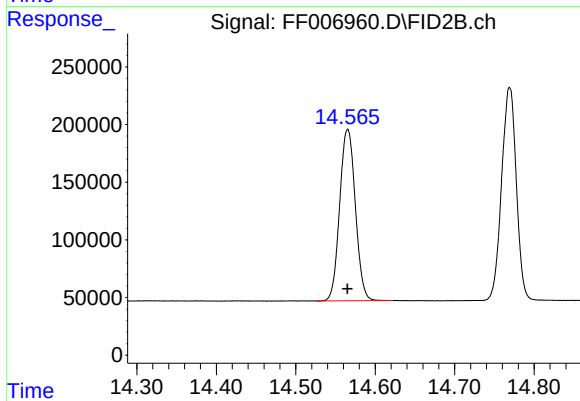

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.565 min
Delta R.T.: 0.000 min
Response: 2035996
Conc: 14.99 ug/ml

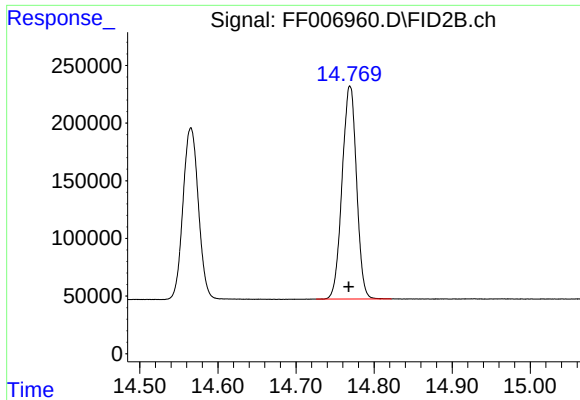

#10 N-TETRACOSANE


R.T.: 14.769 min
Delta R.T.: 0.002 min
Response: 2376859
Conc: 15.25 ug/ml

Instrument :
FID_F
ClientSampleId :
PB128848BS

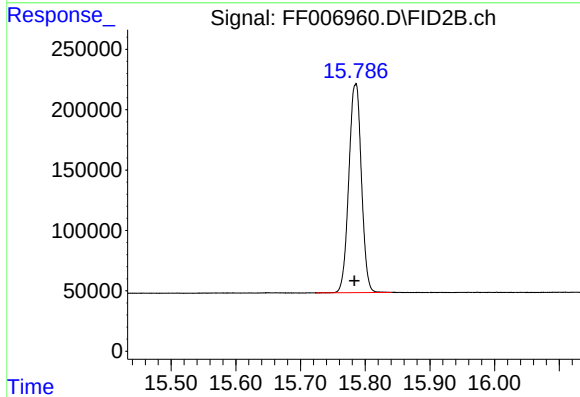

#11 N-HEXACOSANE

R.T.: 15.785 min
Delta R.T.: 0.002 min
Response: 2332072
Conc: 15.09 ug/ml

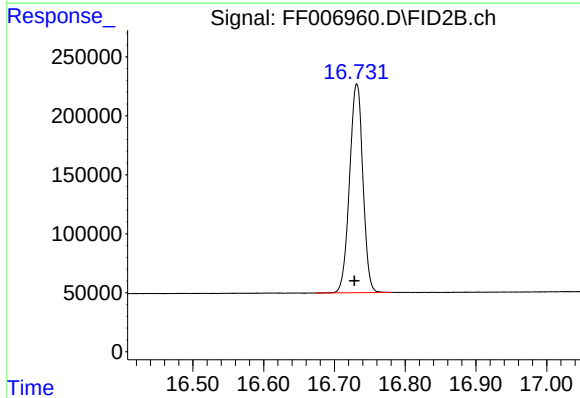

#12 N-OCTACOSANE

R.T.: 16.732 min
Delta R.T.: 0.003 min
Response: 2315468
Conc: 15.02 ug/ml