

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051325\
Data File : FF015833.D
Signal(s) : FID2B.ch
Acq On : 13 May 2025 15:54
Operator : YP\AJ
Sample : Q2008-01
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:51:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042225.M
Quant Title :
QLast Update : Tue Apr 22 11:27:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.016	1930224	17.105 ug/ml
Target Compounds			
18) N-TETRACONTANE	22.207f	132274	3.253 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051325\
Data File : FF015833.D
Signal(s) : FID2B.ch
Acq On : 13 May 2025 15:54
Operator : YP\AJ
Sample : Q2008-01
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 14 05:51:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042225.M
Quant Title :
QLast Update : Tue Apr 22 11:27:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

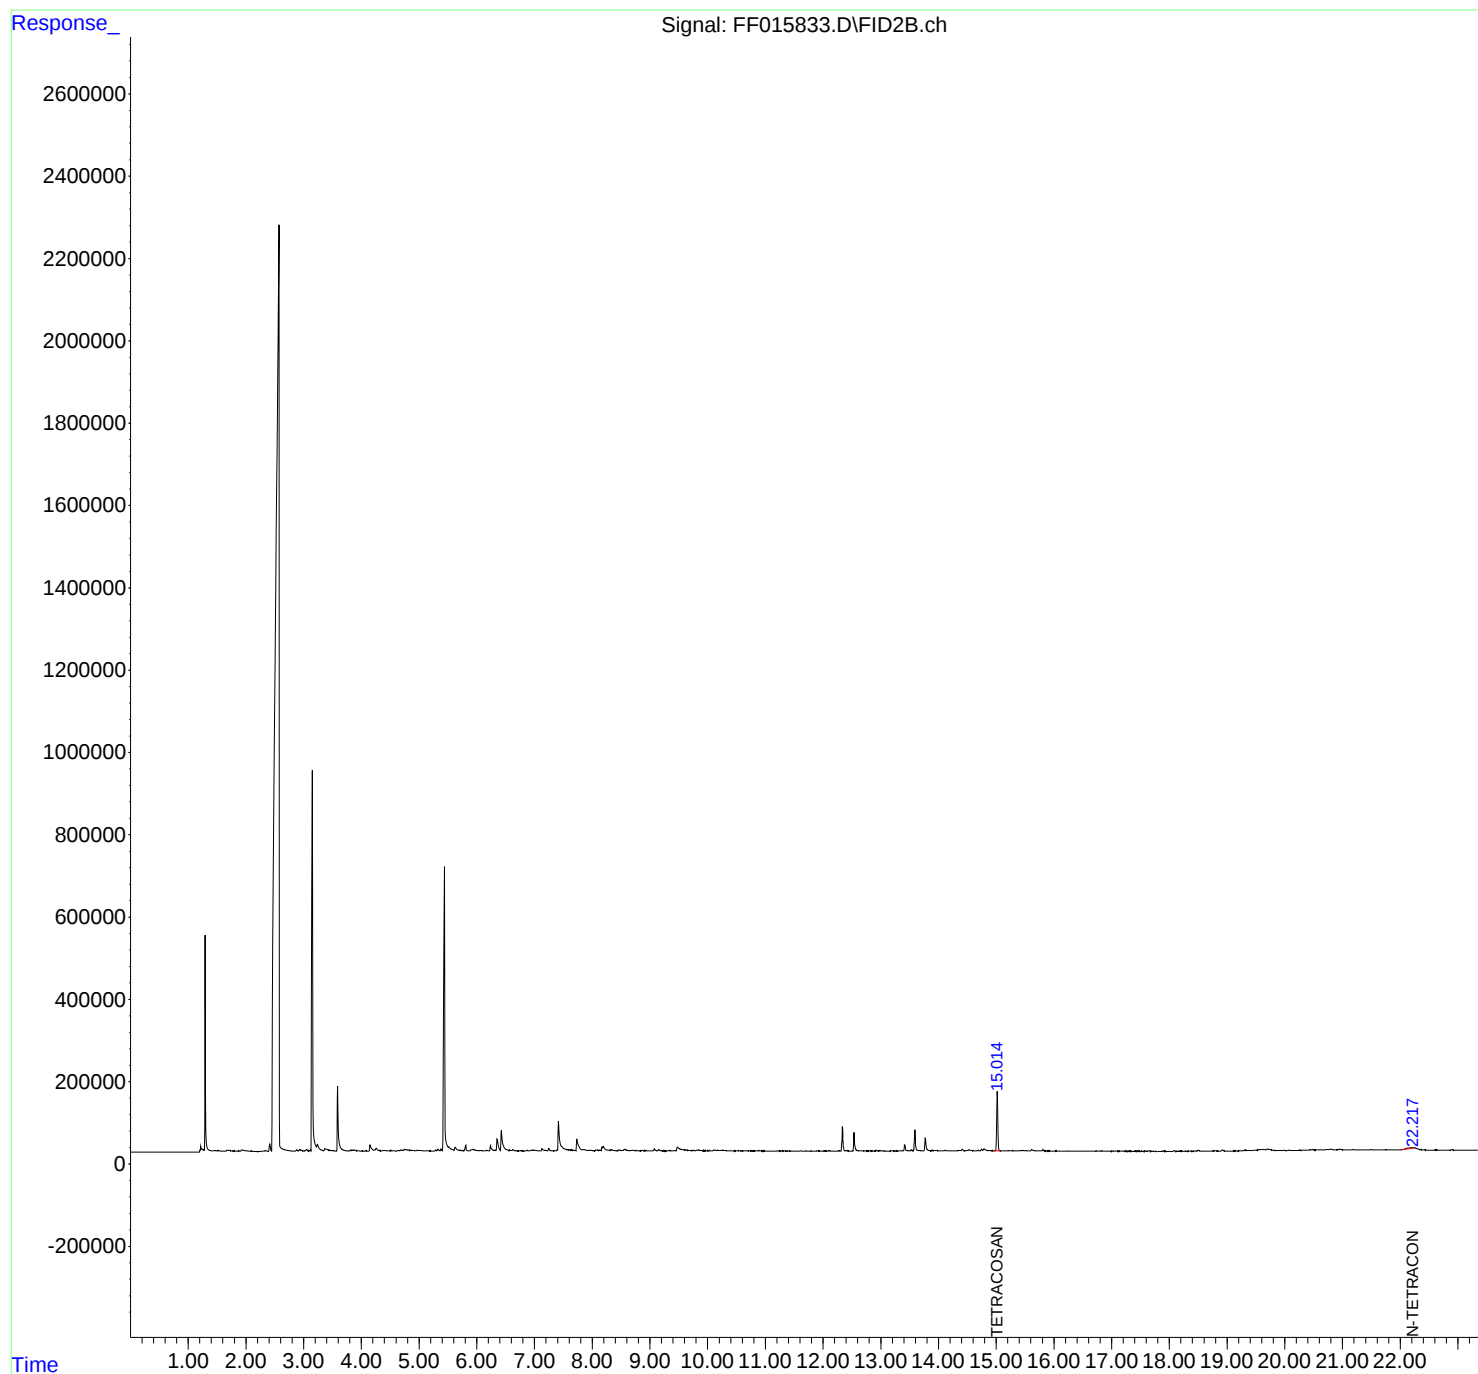


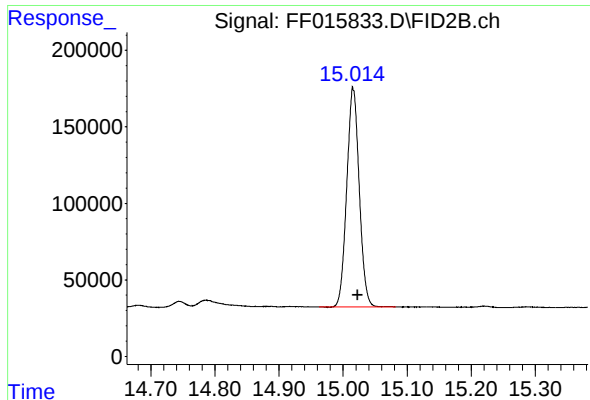

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.016 min
Delta R.T.: -0.007 min
Response: 1930224
Conc: 17.10 ug/ml

Instrument :
FID_F
ClientSampleId :

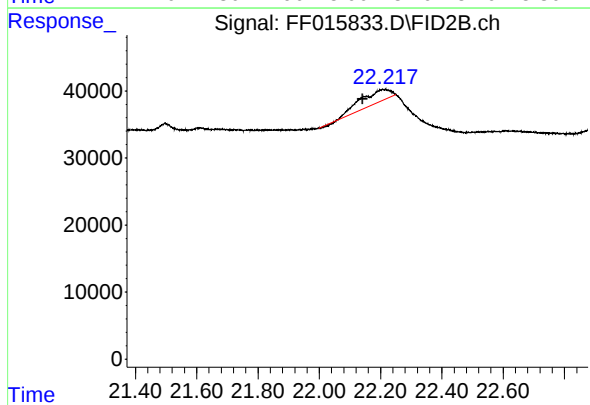

#18 N-TETRACONTANE

R.T.: 22.207 min
Delta R.T.: 0.065 min
Response: 132274
Conc: 3.25 ug/ml