

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051719\
 Data File : FF004567.D
 Signal(s) : FID2B.ch
 Acq On : 17 May 2019 14:11
 Operator : AJ\SJ
 Sample : IDOC-02 FOR RC
 Misc : IDOC-02 FOR RC
 ALS Vial : 57 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: May 18 05:02:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
 Quant Title :
 QLast Update : Thu May 09 09:32:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.702	2027446	20.231 ug/ml
Target Compounds			
2) N-DECANE	4.422	2883878	19.977 ug/ml
3) N-DODECANE	6.444	2813802	19.893 ug/ml
4) N-TETRADECANE	8.239	2704444	19.902 ug/ml
5) N-HEXADECANE	9.841	2631971	20.106 ug/ml
6) N-OCTADECANE	11.285	2553251	20.597 ug/ml
7) N-EICOSANE	12.598	2503688	20.805 ug/ml
8) N-DOCOSANE	13.800	2480550	21.376 ug/ml
10) N-TETRACOSANE	14.905	2535266	22.143 ug/ml
11) N-HEXACOSANE	15.930	2561797	22.438 ug/ml
12) N-OCTACOSANE	16.884	2632406	23.035 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051719\
Data File : FF004567.D
Signal(s) : FID2B.ch
Acq On : 17 May 2019 14:11
Operator : AJ\SJ
Sample : IDOC-02 FOR RC
Misc : IDOC-02 FOR RC
ALS Vial : 57 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: May 18 05:02:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
Quant Title :
QLast Update : Thu May 09 09:32:48 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

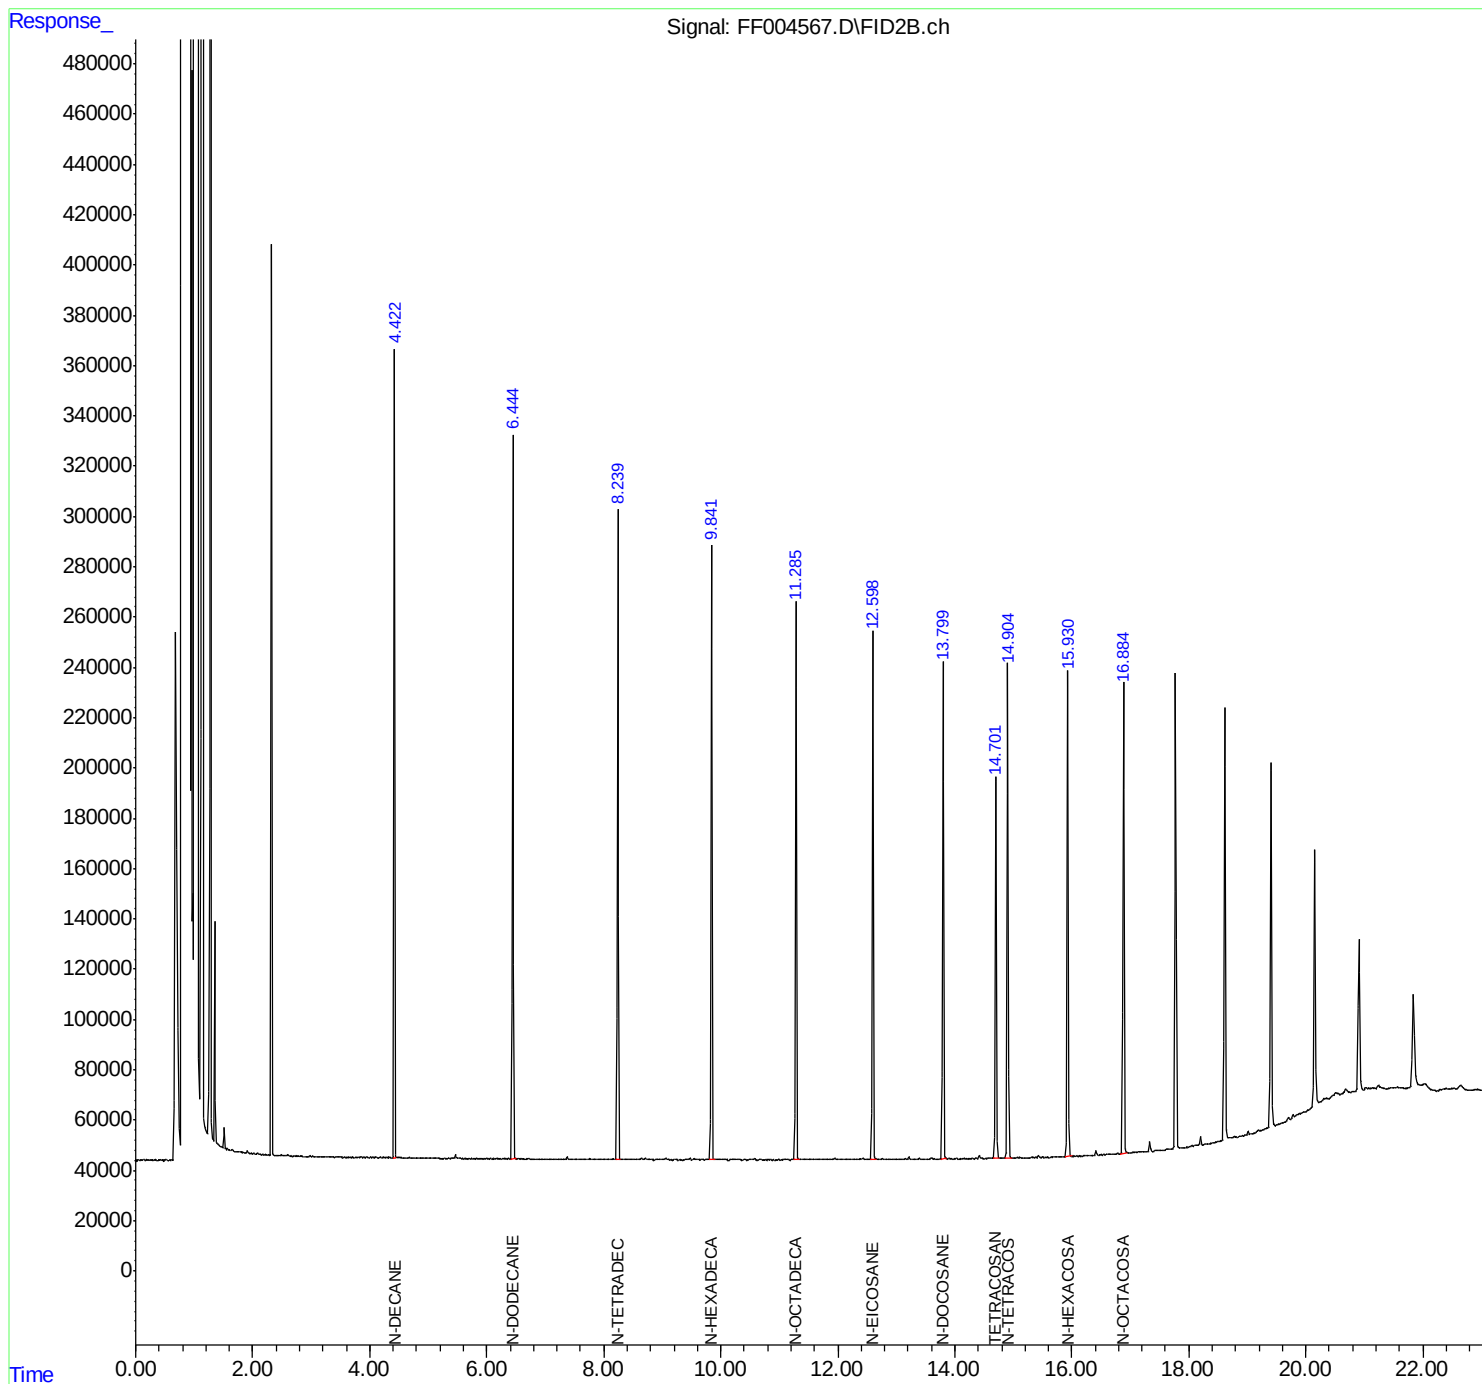

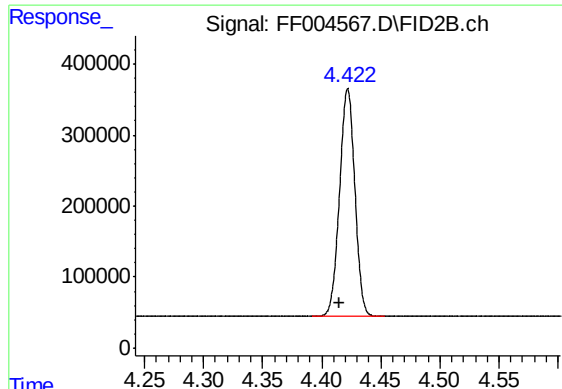


#2 N-DECANE

R.T.: 4.422 min
Delta R.T.: 0.007 min
Response: 2883878
Conc: 19.98 ug/ml

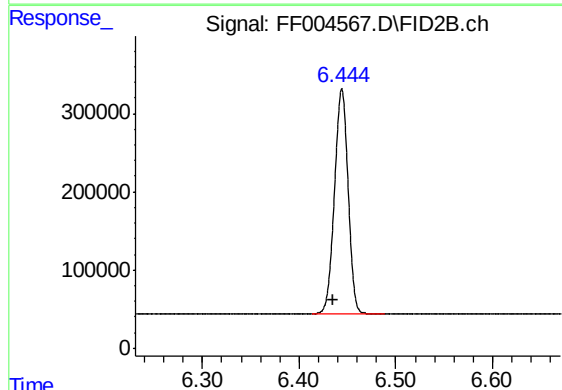


#3 N-DODECANE

R.T.: 6.444 min
Delta R.T.: 0.010 min
Response: 2813802
Conc: 19.89 ug/ml

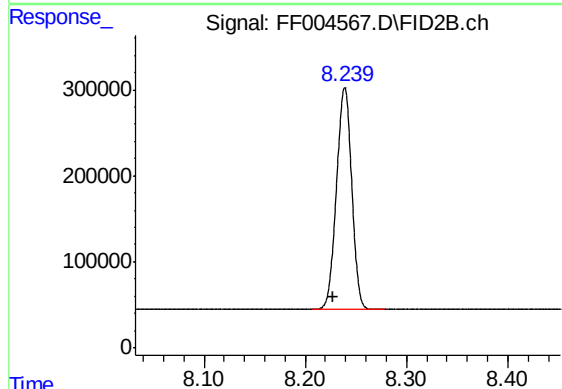


#4 N-TETRADECANE

R.T.: 8.239 min
Delta R.T.: 0.011 min
Response: 2704444
Conc: 19.90 ug/ml

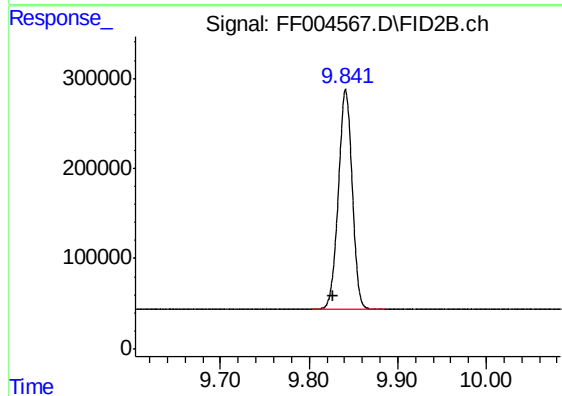


#5 N-HEXADECANE

R.T.: 9.841 min
Delta R.T.: 0.014 min
Response: 2631971
Conc: 20.11 ug/ml

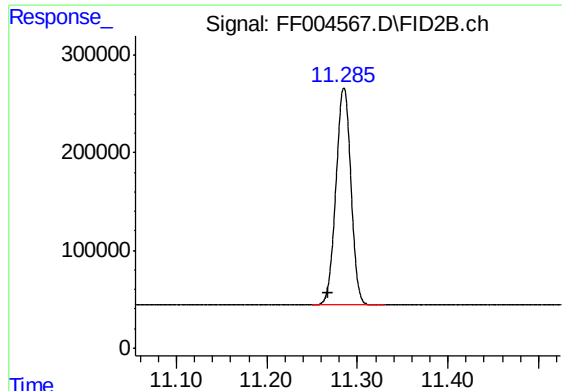


#6 N-OCTADECANE

R.T.: 11.285 min
Delta R.T.: 0.017 min
Response: 2553251
Conc: 20.60 ug/ml

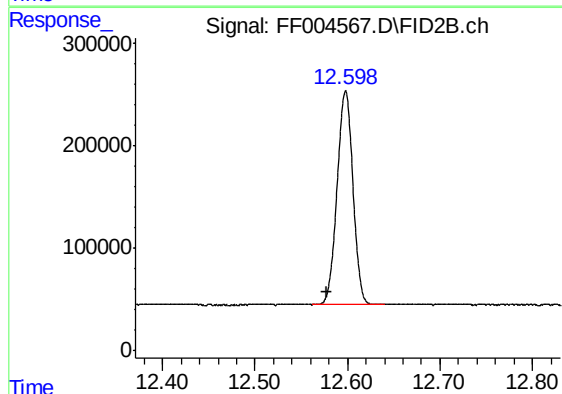


#7 N-EICOSANE

R.T.: 12.598 min
Delta R.T.: 0.020 min
Response: 2503688
Conc: 20.80 ug/ml

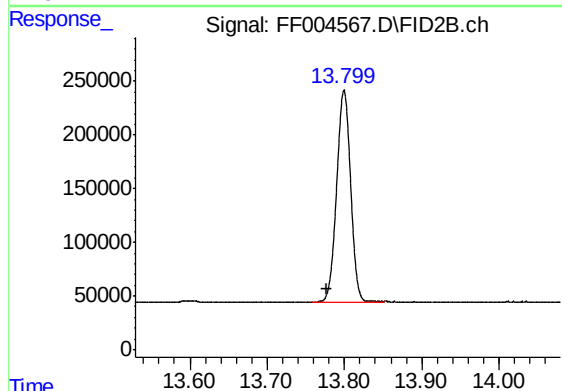


#8 N-DOCOSANE

R.T.: 13.800 min
Delta R.T.: 0.022 min
Response: 2480550
Conc: 21.38 ug/ml

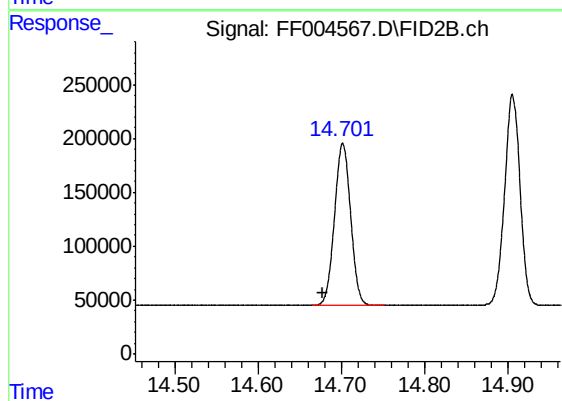


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.702 min
Delta R.T.: 0.024 min
Response: 2027446
Conc: 20.23 ug/ml

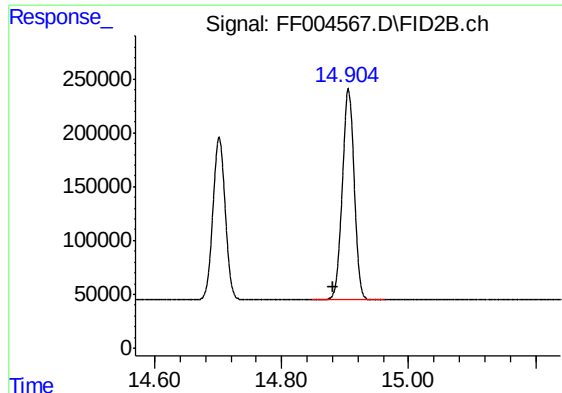


#10 N-TETRACOSANE

R.T.: 14.905 min
Delta R.T.: 0.023 min
Response: 2535266
Conc: 22.14 ug/ml

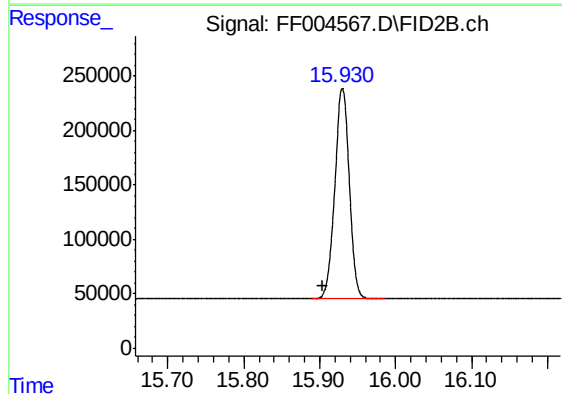

#11 N-HEXACOSANE

R.T.: 15.930 min
Delta R.T.: 0.026 min
Response: 2561797
Conc: 22.44 ug/ml

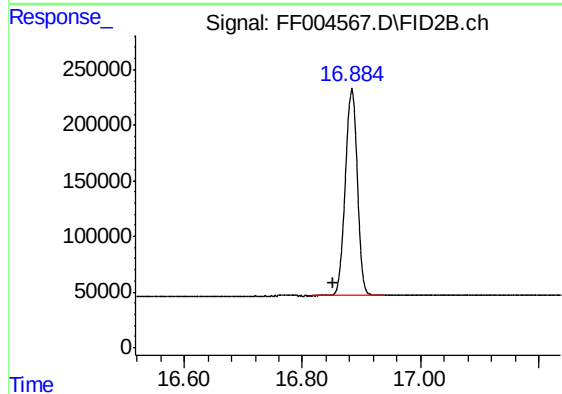

#12 N-OCTACOSANE

R.T.: 16.884 min
Delta R.T.: 0.031 min
Response: 2632406
Conc: 23.03 ug/ml