

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051721\
Data File : FF008431.D
Signal(s) : FID2B.ch
Acq On : 17 May 2021 12:23
Operator : DD\AJ
Sample : PB136186BL
Misc : MDL-WATER-BL
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB136186BL

Integration File: autoint1.e
Quant Time: May 17 15:01:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.777	2672376	21.404 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051721\
Data File : FF008431.D
Signal(s) : FID2B.ch
Acq On : 17 May 2021 12:23
Operator : DD\AJ
Sample : PB136186BL
Misc : MDL-WATER-BL
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB136186BL

Integration File: autoint1.e
Quant Time: May 17 15:01:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

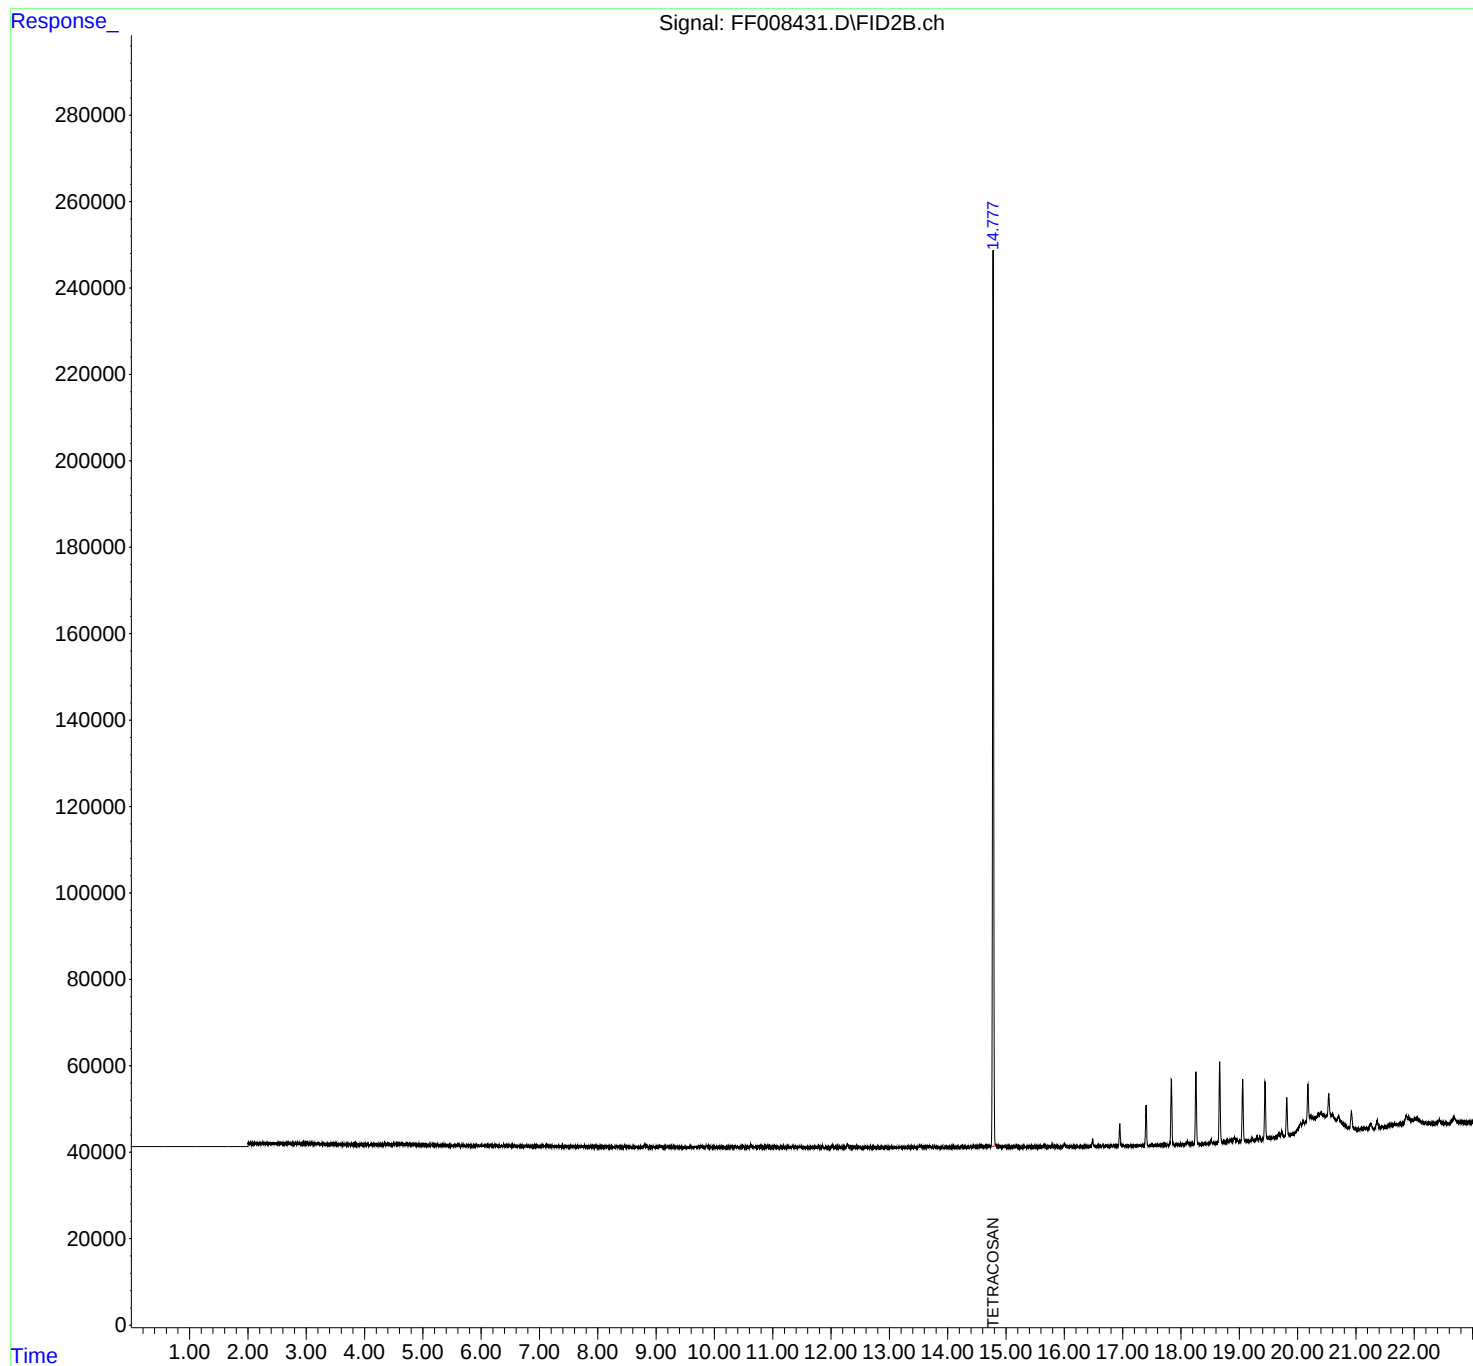

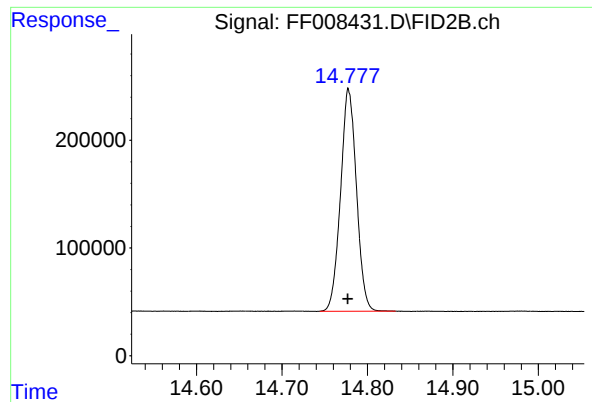

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.777 min
Delta R.T.: 0.000 min
Response: 2672376
Conc: 21.40 ug/ml

Instrument :
FID_F
ClientSampleId :
PB136186BL