

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051721\
 Data File : FF008436.D
 Signal(s) : FID2B.ch
 Acq On : 17 May 2021 14:58
 Operator : DD\AJ
 Sample : M2392-11MS
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-04-COMPMS

Integration File: autoint1.e
 Quant Time: May 17 15:12:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	1014127	8.122 ug/ml
Target Compounds			
2) N-DECANE	4.534	1738774	12.880 ug/ml
3) N-DODECANE	6.547	1791139	13.101 ug/ml
4) N-TETRADECANE	8.337	1832799	13.114 ug/ml
5) N-HEXADECANE	9.933	1812902	13.001 ug/ml
6) N-OCTADECANE	11.370	1796474	12.601 ug/ml
7) N-EICOSANE	12.678	1782174	12.545 ug/ml
8) N-DOCOSANE	13.878	1718901	12.077 ug/ml
10) N-TETRACOSANE	14.984	1678555	11.769 ug/ml
11) N-HEXACOSANE	16.006	1584724	11.239 ug/ml
12) N-OCTACOSANE	16.954	1534326	10.935 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051721\
Data File : FF008436.D
Signal(s) : FID2B.ch
Acq On : 17 May 2021 14:58
Operator : DD\AJ
Sample : M2392-11MS
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-04-COMPMS

Integration File: autoint1.e
Quant Time: May 17 15:12:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

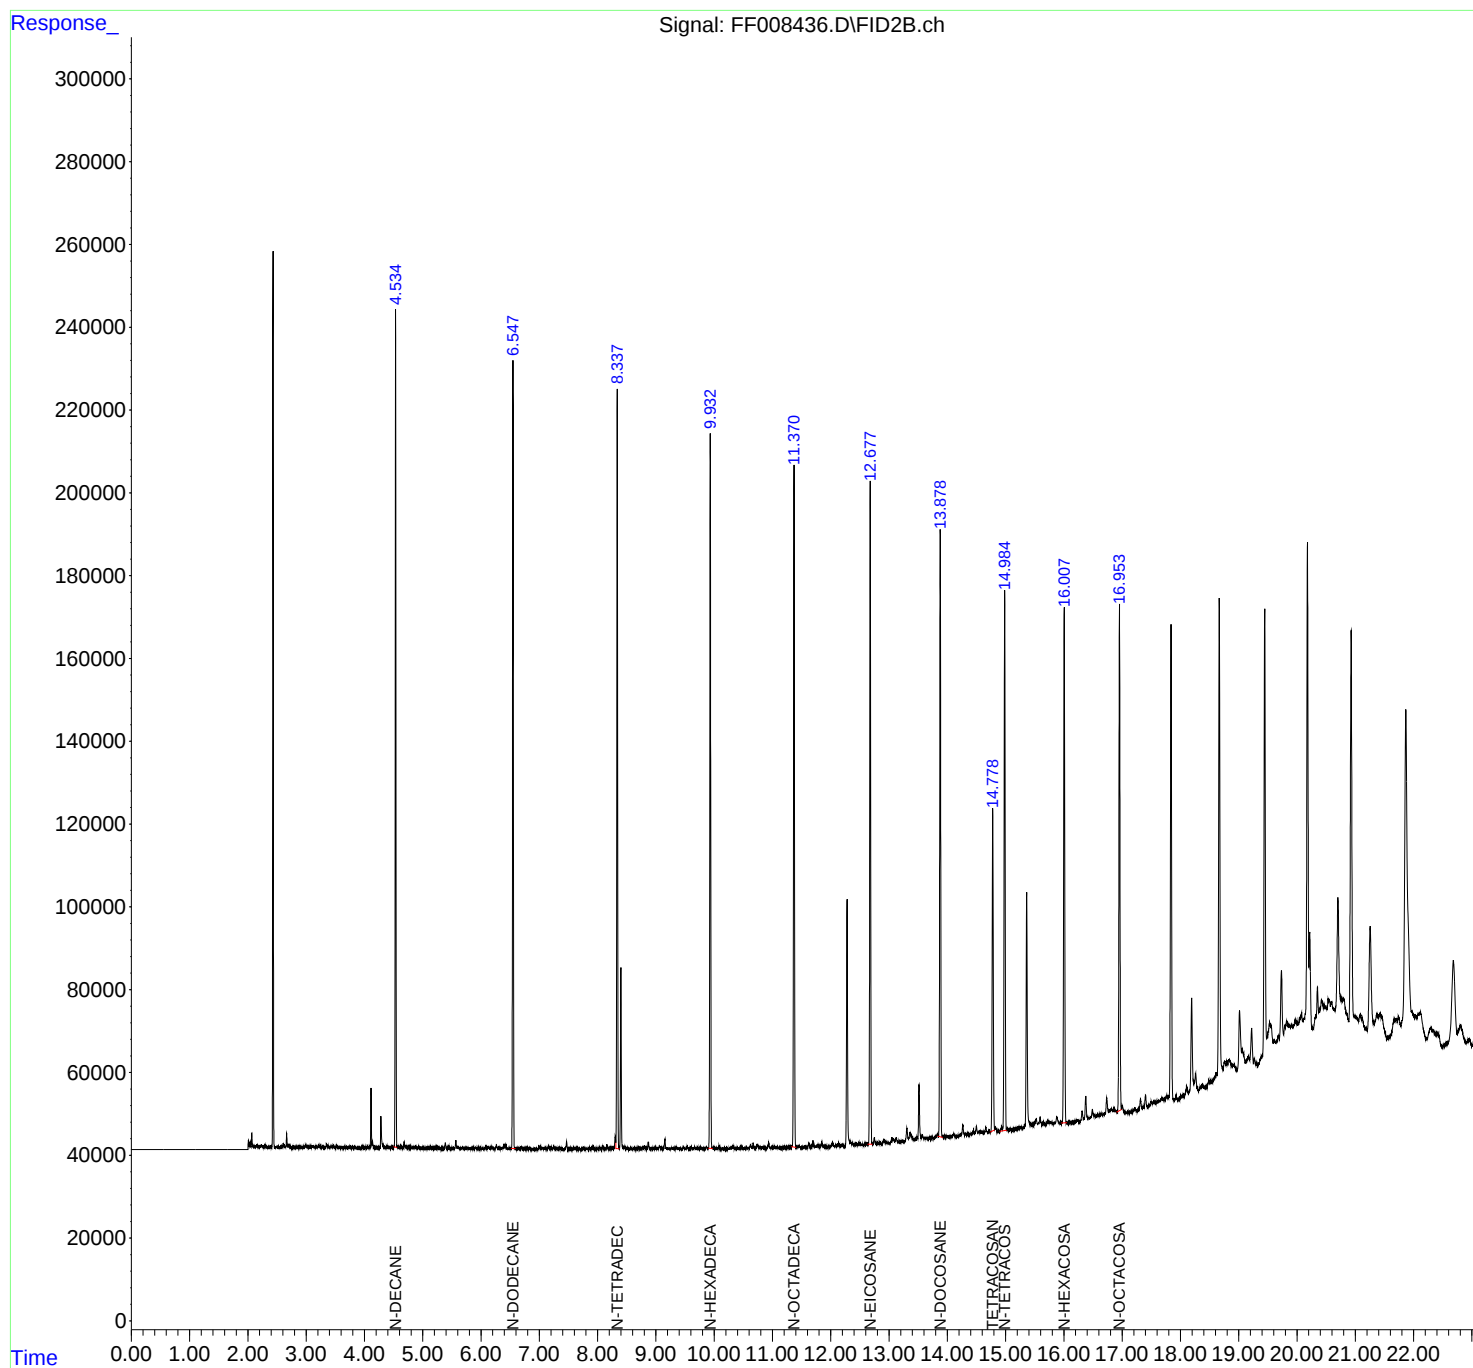


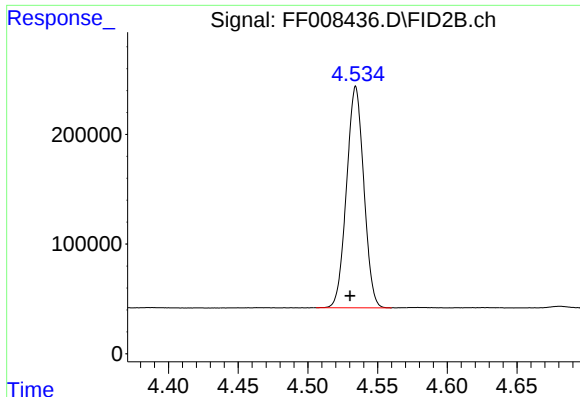

#2 N-DECANE


R.T.: 4.534 min
Delta R.T.: 0.004 min
Response: 1738774
Conc: 12.88 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-04-COMPMS

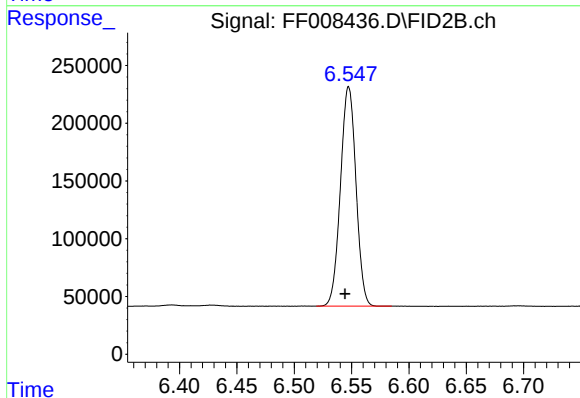


#3 N-DODECANE

R.T.: 6.547 min
Delta R.T.: 0.003 min
Response: 1791139
Conc: 13.10 ug/ml

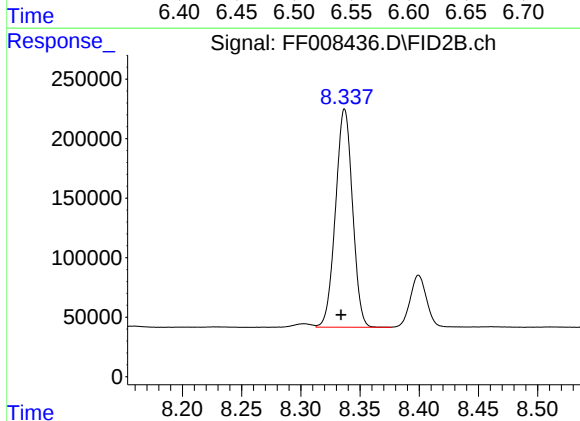


#4 N-TETRADECANE

R.T.: 8.337 min
Delta R.T.: 0.003 min
Response: 1832799
Conc: 13.11 ug/ml

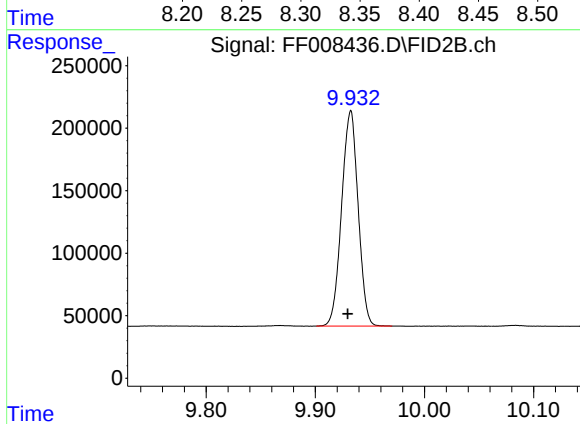

#5 N-HEXADECANE


R.T.: 9.933 min
Delta R.T.: 0.003 min
Response: 1812902
Conc: 13.00 ug/ml

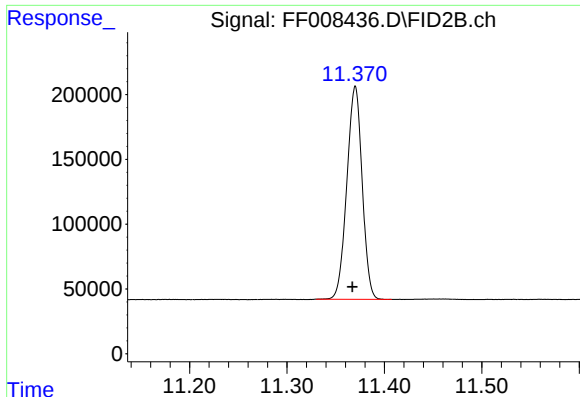

#6 N-OCTADECANE


R.T.: 11.370 min
Delta R.T.: 0.003 min
Response: 1796474
Conc: 12.60 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-04-COMPMS

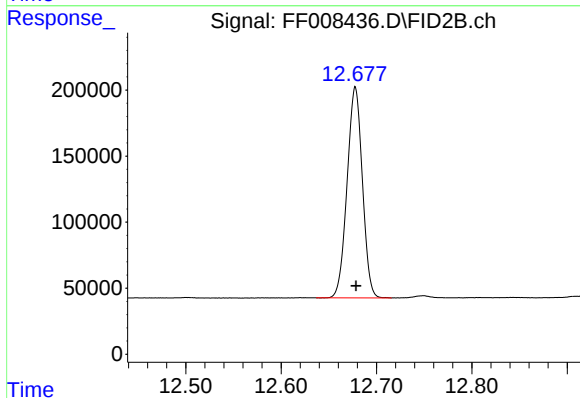


#7 N-EICOSANE

R.T.: 12.678 min
Delta R.T.: 0.000 min
Response: 1782174
Conc: 12.55 ug/ml

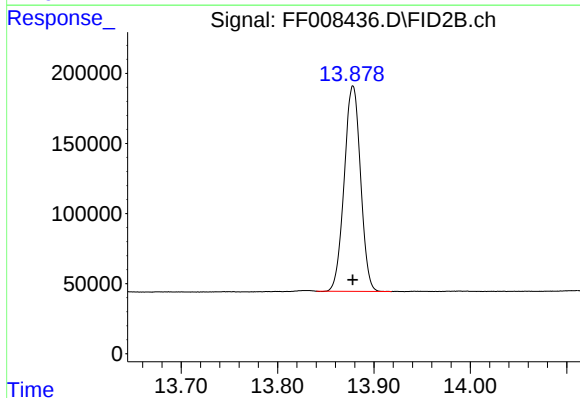


#8 N-DOCOSANE

R.T.: 13.878 min
Delta R.T.: 0.000 min
Response: 1718901
Conc: 12.08 ug/ml

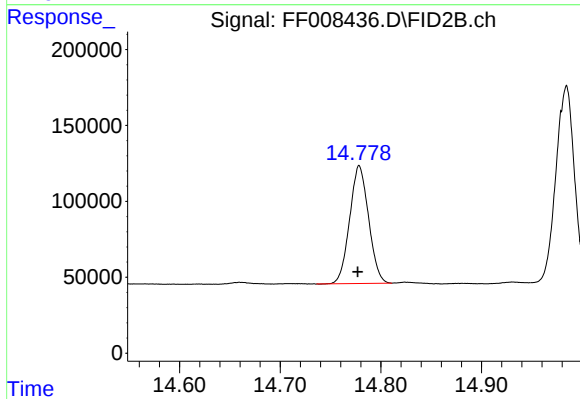

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.778 min
Delta R.T.: 0.001 min
Response: 1014127
Conc: 8.12 ug/ml

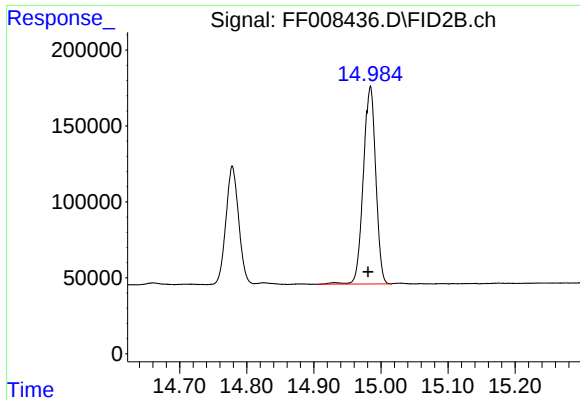

#10 N-TETRACOSANE


R.T.: 14.984 min
Delta R.T.: 0.004 min
Response: 1678555
Conc: 11.77 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-04-COMPMS

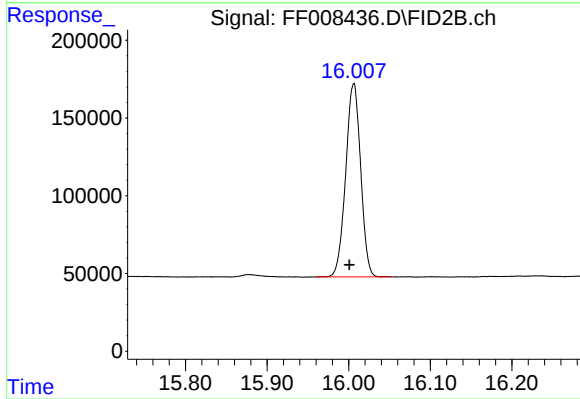

#11 N-HEXACOSANE

R.T.: 16.006 min
Delta R.T.: 0.005 min
Response: 1584724
Conc: 11.24 ug/ml

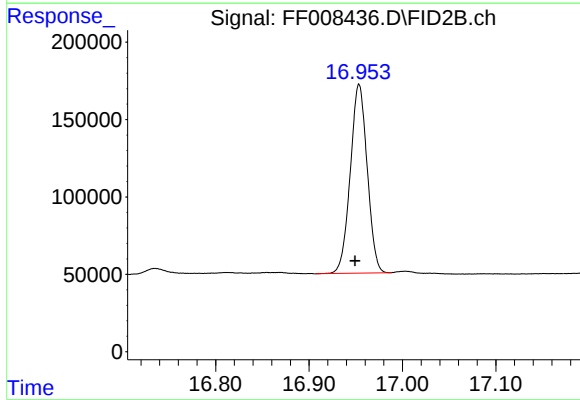

#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.004 min
Response: 1534326
Conc: 10.93 ug/ml