

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051823\
Data File : FF012613.D
Signal(s) : FID2B.ch
Acq On : 18 May 2023 10:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 19 01:43:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.000	2197875	18.207 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051823\
Data File : FF012613.D
Signal(s) : FID2B.ch
Acq On : 18 May 2023 10:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: May 19 01:43:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

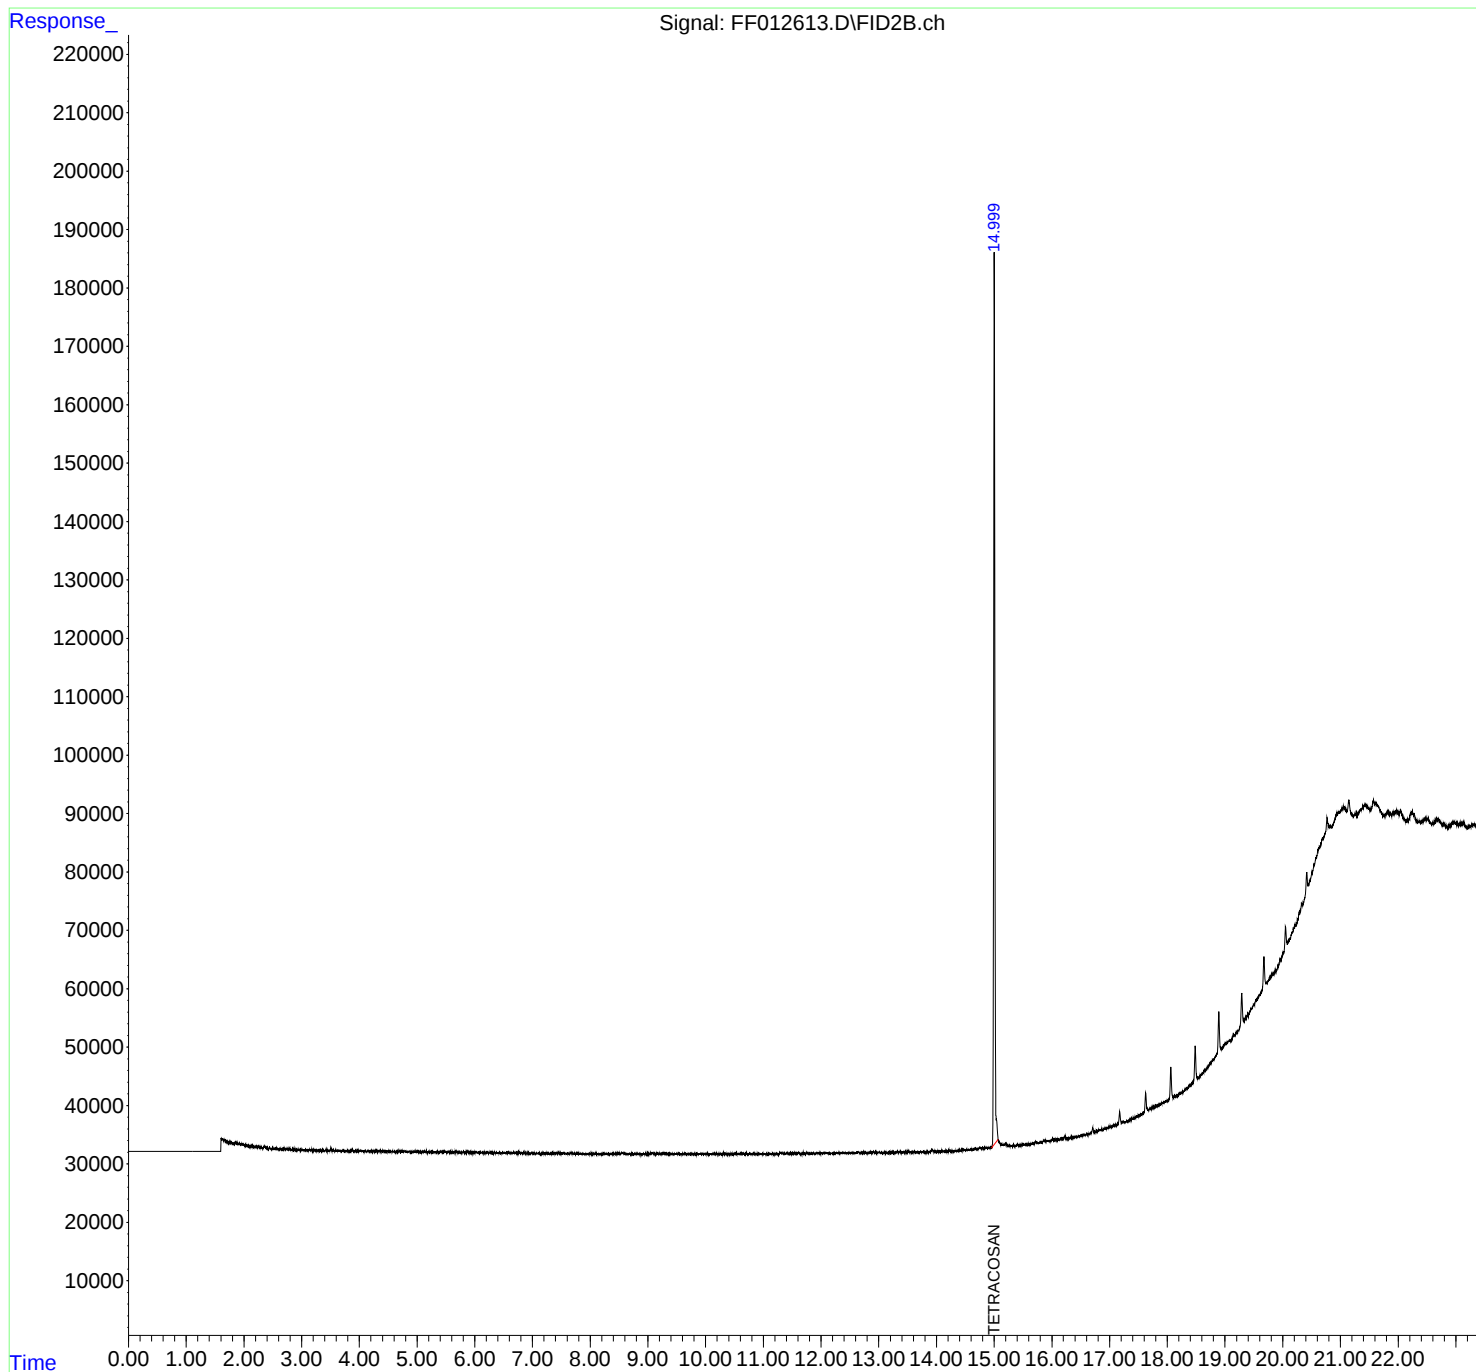

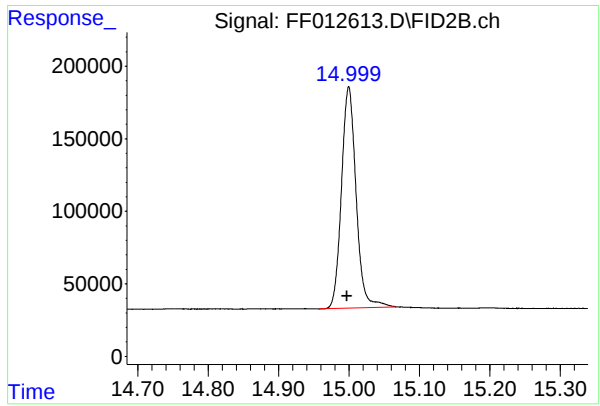

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.000 min
Delta R.T.: 0.003 min
Response: 2197875
Conc: 18.21 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK