

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051823\
Data File : FF012616.D
Signal(s) : FID2B.ch
Acq On : 18 May 2023 14:45
Operator : YP\AJ
Sample : PB152871BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB152871BL

Integration File: autoint1.e
Quant Time: May 19 01:43:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.995	2035869	16.865 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051823\
Data File : FF012616.D
Signal(s) : FID2B.ch
Acq On : 18 May 2023 14:45
Operator : YP\AJ
Sample : PB152871BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB152871BL

Integration File: autoint1.e
Quant Time: May 19 01:43:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

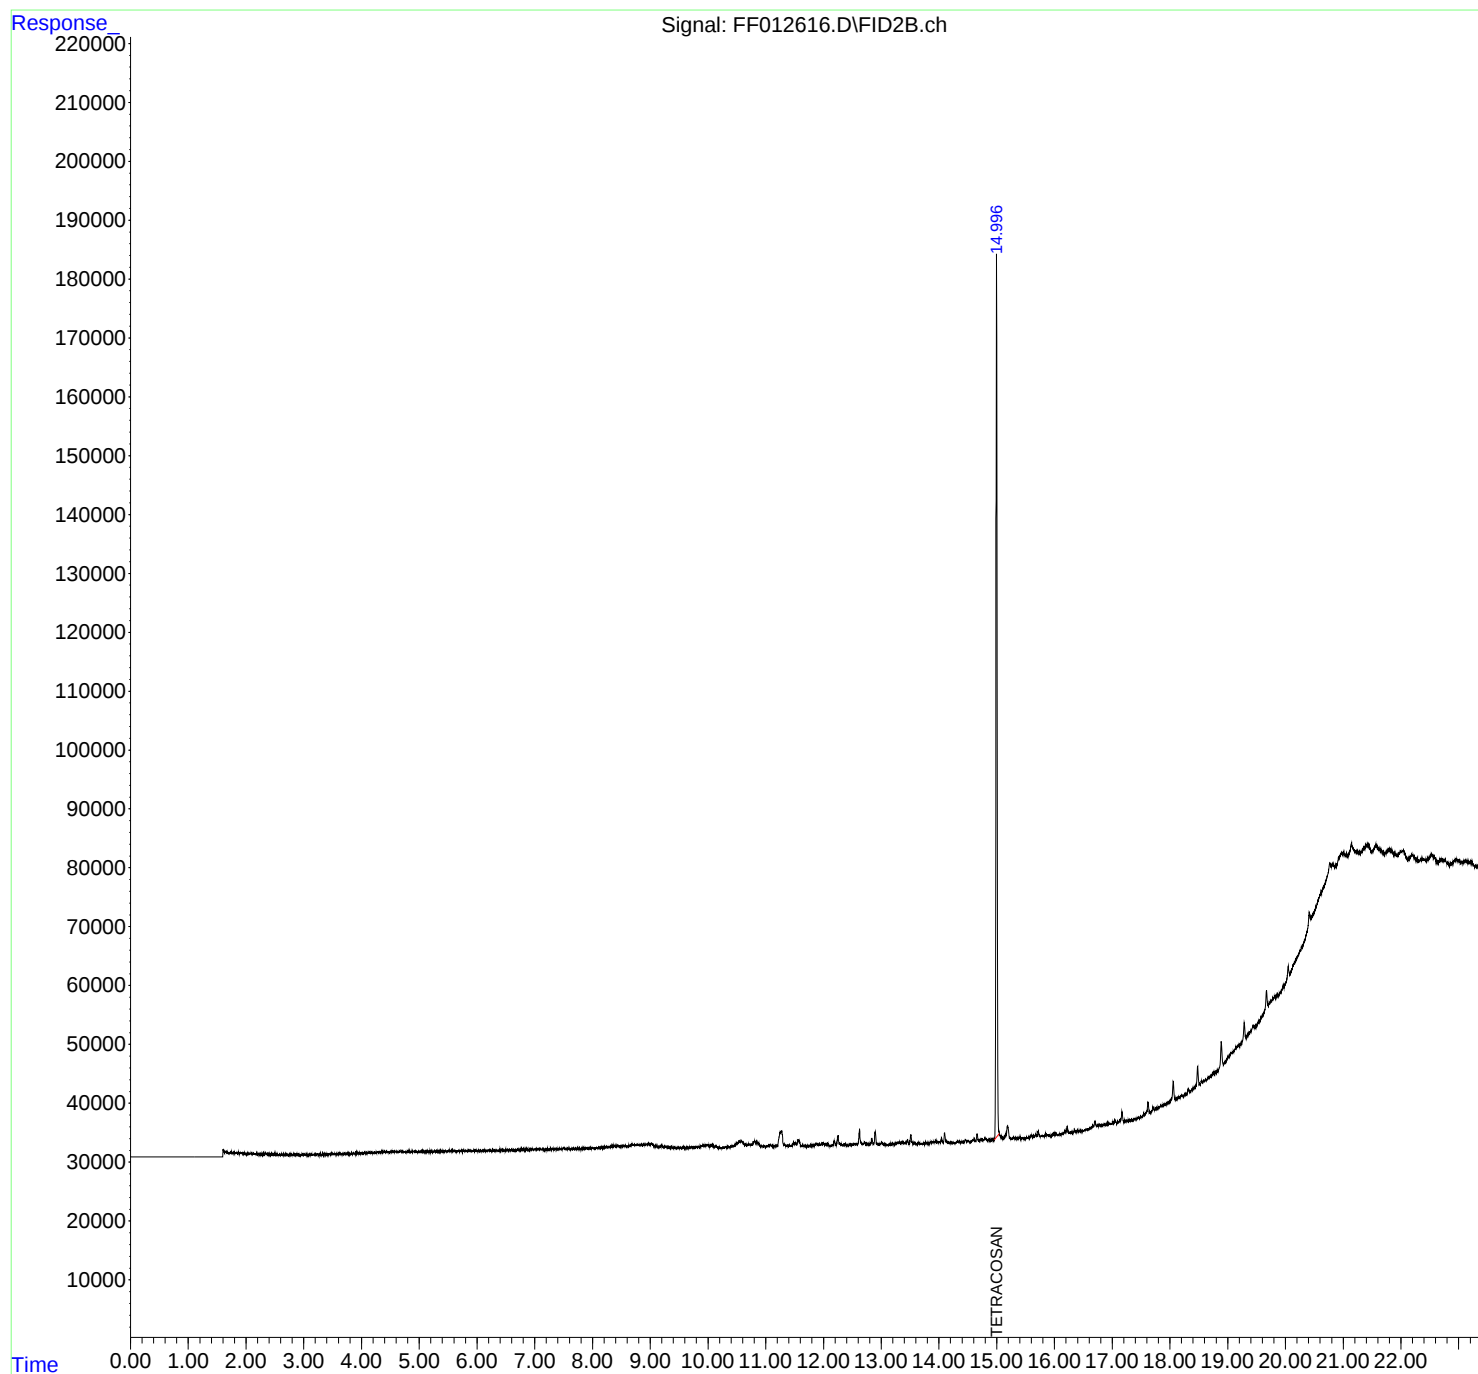

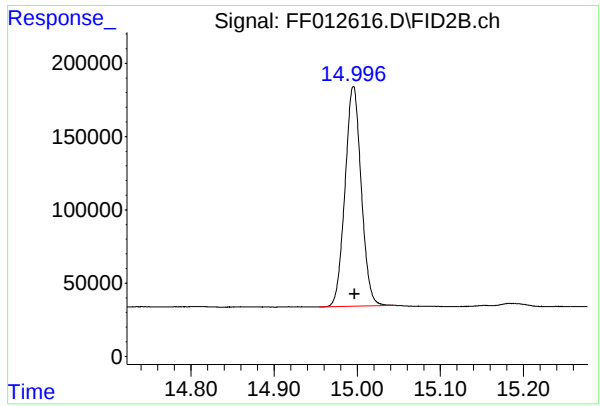

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.995 min
Delta R.T.: -0.001 min
Response: 2035869
Conc: 16.86 ug/ml

Instrument :
FID_F
ClientSampleId :
PB152871BL