

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051925\
 Data File : FF015870.D
 Signal(s) : FID2B.ch
 Acq On : 19 May 2025 18:08
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: May 20 03:55:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042225.M
 Quant Title :
 QLast Update : Tue Apr 22 11:27:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.021	5948329	52.711 ug/ml
Target Compounds			
2) N-DECANE	4.563	6051106	59.298 ug/ml
3) N-DODECANE	6.733	6272737	57.287 ug/ml
4) N-TETRADECANE	8.560	6301846	54.599 ug/ml
5) N-HEXADECANE	10.168	6414492	54.351 ug/ml
6) N-OCTADECANE	11.611	6638617	52.773 ug/ml
7) N-EICOSANE	12.922	6649486	50.971 ug/ml
8) N-DOCOSANE	14.121	6565472	51.543 ug/ml
10) N-TETRACOSANE	15.225	6573948	52.262 ug/ml
11) N-HEXACOSANE	16.247	6464054	53.028 ug/ml
12) N-OCTACOSANE	17.198	6509624	55.012 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF051925\
Data File : FF015870.D
Signal(s) : FID2B.ch
Acq On : 19 May 2025 18:08
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: May 20 03:55:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF042225.M
Quant Title :
QLast Update : Tue Apr 22 11:27:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

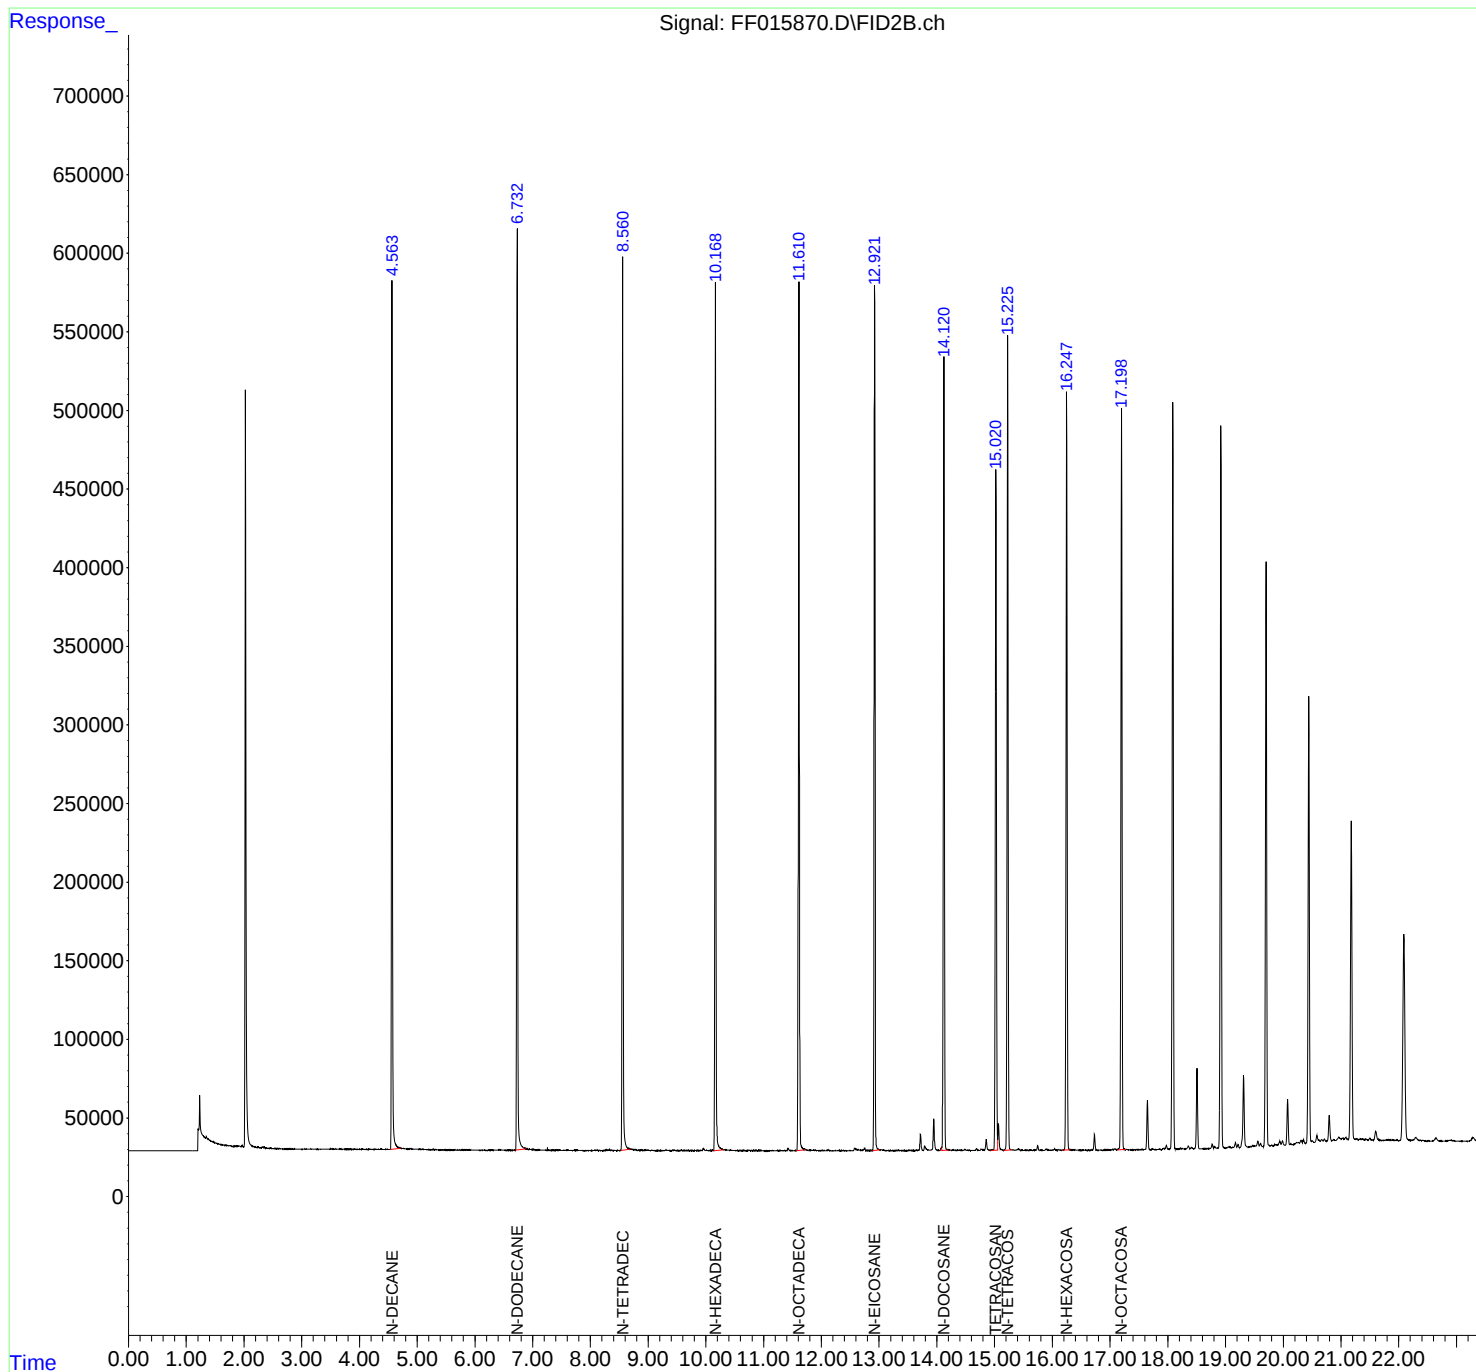


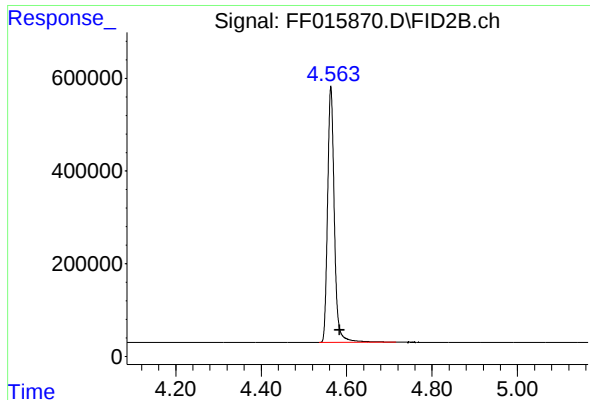

#2 N-DECANE


R.T.: 4.563 min
Delta R.T.: -0.021 min
Response: 6051106
Conc: 59.30 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

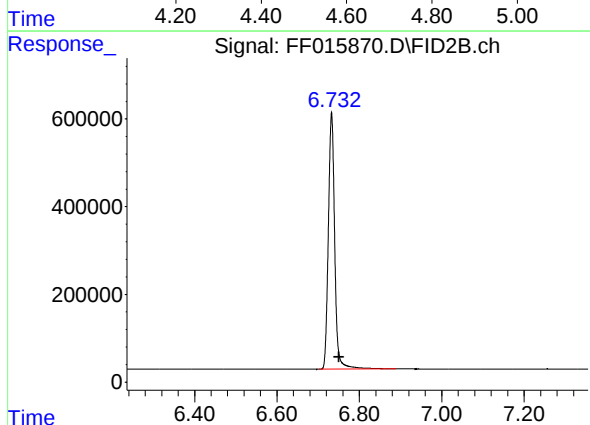


#3 N-DODECANE

R.T.: 6.733 min
Delta R.T.: -0.017 min
Response: 6272737
Conc: 57.29 ug/ml

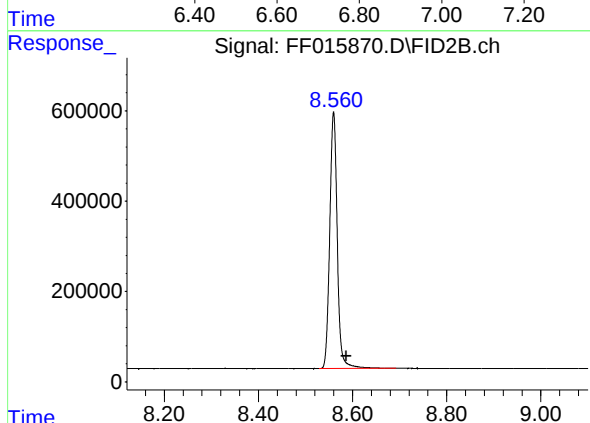


#4 N-TETRADECANE

R.T.: 8.560 min
Delta R.T.: -0.027 min
Response: 6301846
Conc: 54.60 ug/ml

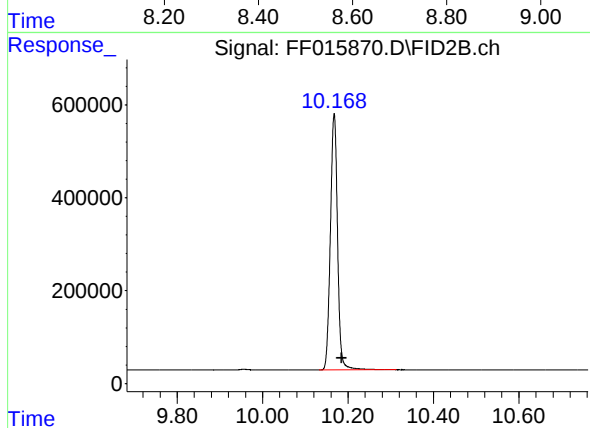

#5 N-HEXADECANE


R.T.: 10.168 min
Delta R.T.: -0.017 min
Response: 6414492
Conc: 54.35 ug/ml

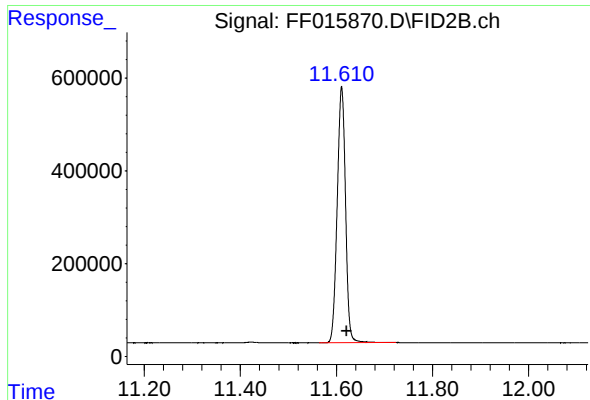

#6 N-OCTADECANE


R.T.: 11.611 min
Delta R.T.: -0.010 min
Response: 6638617
Conc: 52.77 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

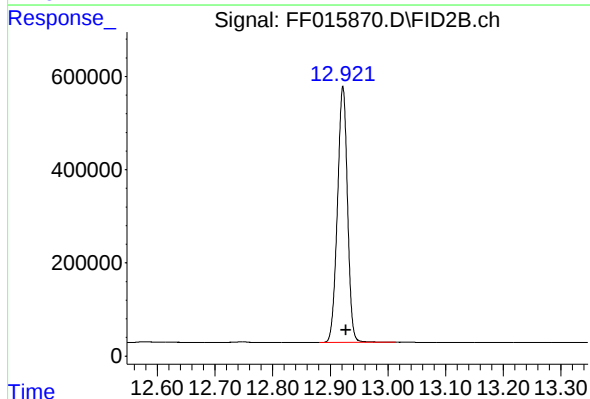


#7 N-EICOSANE

R.T.: 12.922 min
Delta R.T.: -0.005 min
Response: 6649486
Conc: 50.97 ug/ml

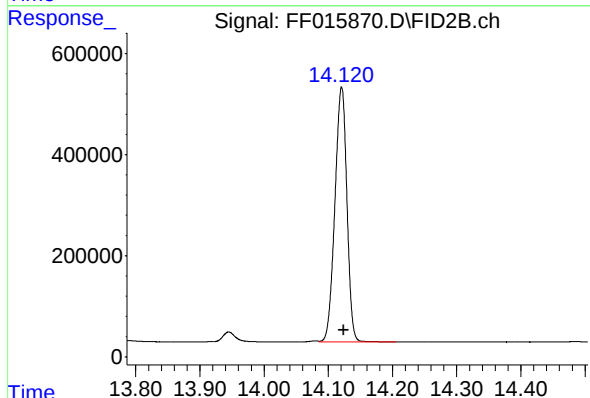


#8 N-DOCOSANE

R.T.: 14.121 min
Delta R.T.: -0.003 min
Response: 6565472
Conc: 51.54 ug/ml

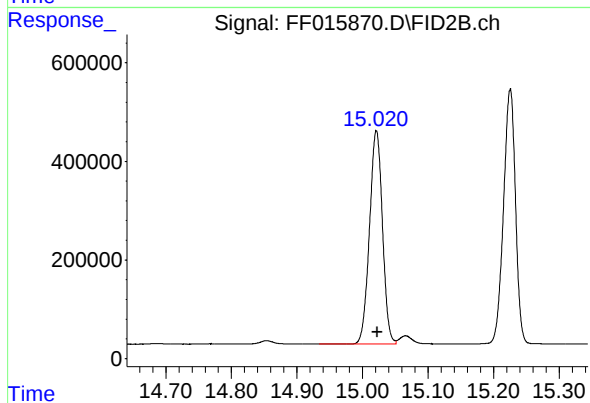

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.021 min
Delta R.T.: -0.001 min
Response: 5948329
Conc: 52.71 ug/ml

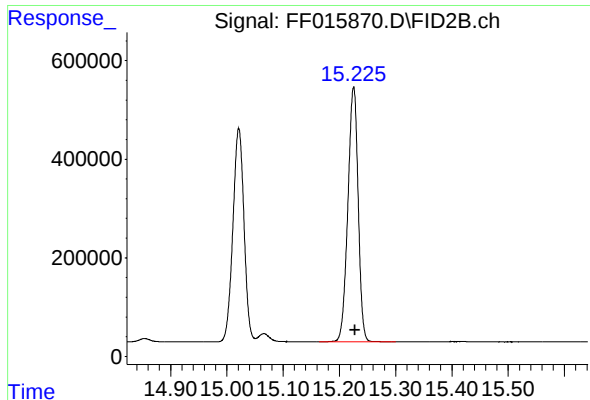

#10 N-TETRACOSANE


R.T.: 15.225 min
Delta R.T.: -0.002 min
Response: 6573948
Conc: 52.26 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

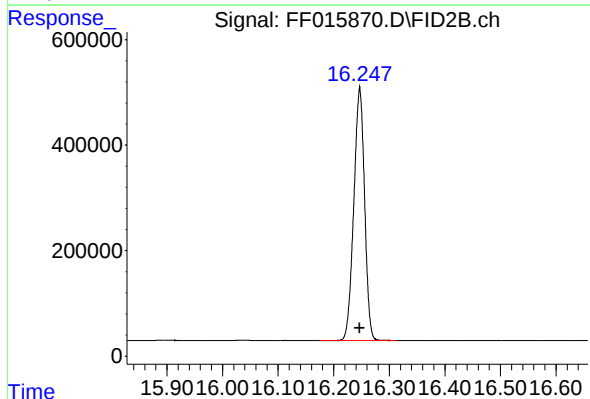

#11 N-HEXACOSANE

R.T.: 16.247 min
Delta R.T.: 0.000 min
Response: 6464054
Conc: 53.03 ug/ml

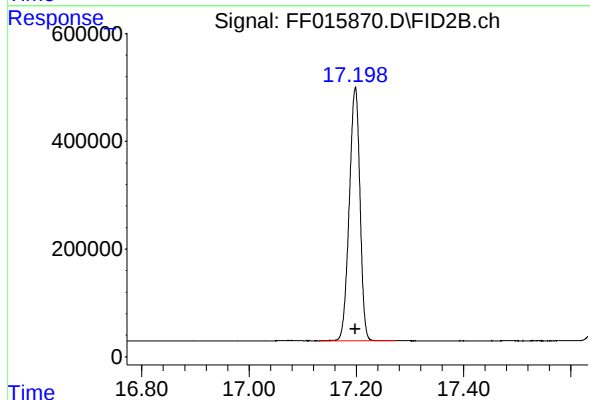

#12 N-OCTACOSANE

R.T.: 17.198 min
Delta R.T.: 0.000 min
Response: 6509624
Conc: 55.01 ug/ml