

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052019\
 Data File : FF004578.D
 Signal(s) : FID2B.ch
 Acq On : 20 May 2019 12:02
 Operator : AJ\SJ
 Sample : K2880-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 21 00:46:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
 Quant Title :
 QLast Update : Thu May 09 09:32:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.703	1486753	14.836 ug/ml
Target Compounds			
4) N-TETRADECANE	8.293f	520849	3.833 ug/ml
10) N-TETRACOSANE	14.877	126744	1.107 ug/ml
11) N-HEXACOSANE	15.938	54089	0.474 ug/ml
12) N-OCTACOSANE	16.853	301704	2.640 ug/ml
13) N-TRIACONTANE	17.761	202747	1.751 ug/ml
14) N-DOTRIACONTANE	18.601	36302	0.296 ug/ml
15) N-TETRATRIACONTANE	19.416	90992	0.791 ug/ml
16) N-HEXATRIACONTANE	20.095	496764	4.609 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052019\
Data File : FF004578.D
Signal(s) : FID2B.ch
Acq On : 20 May 2019 12:02
Operator : AJ\SJ
Sample : K2880-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 21 00:46:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050819.M
Quant Title :
QLast Update : Thu May 09 09:32:48 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

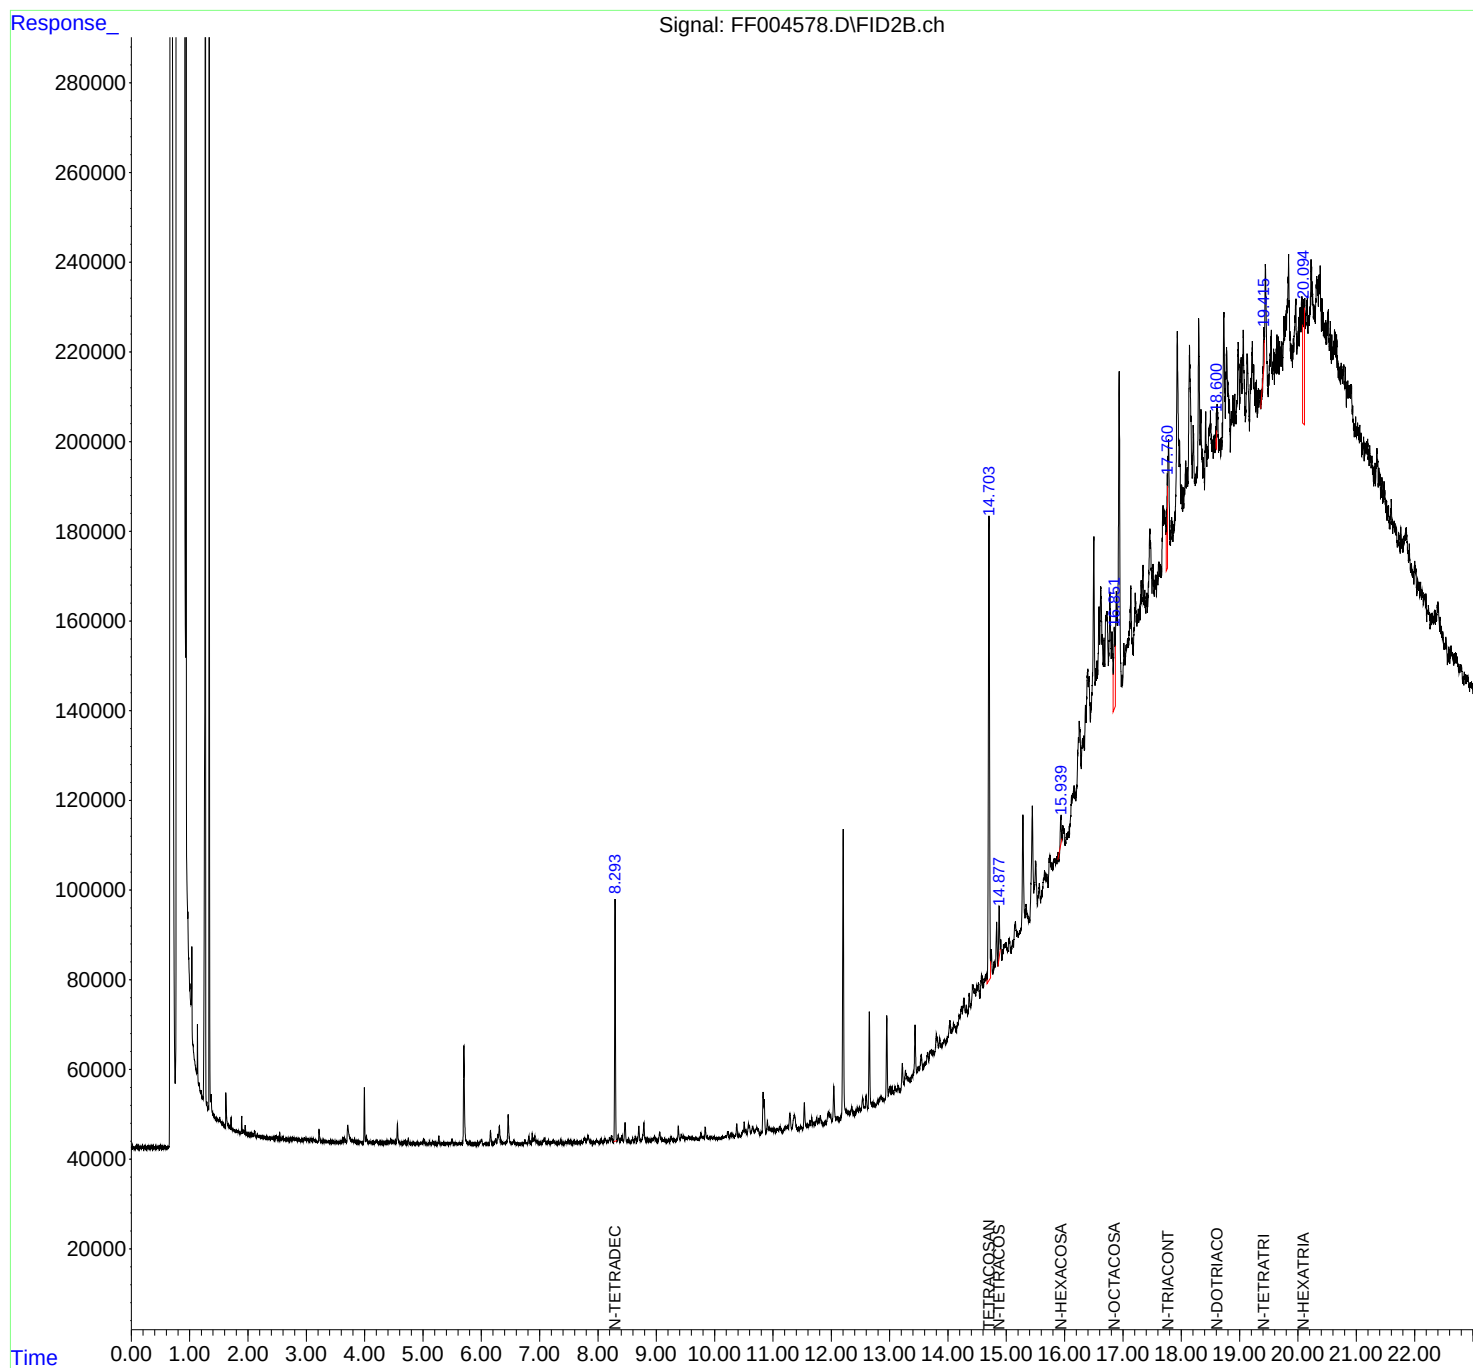

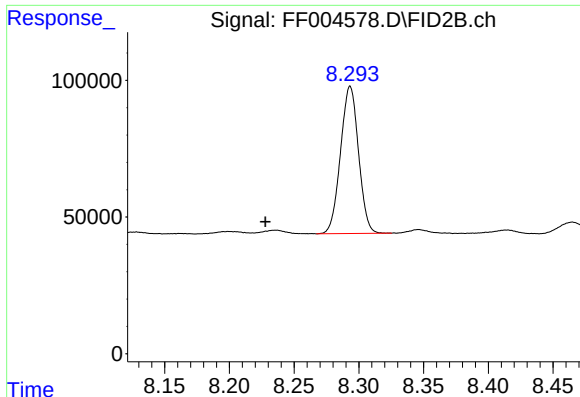


#4 N-TETRADECANE

R.T.: 8.293 min
Delta R.T.: 0.066 min
Response: 520849
Conc: 3.83 ug/ml

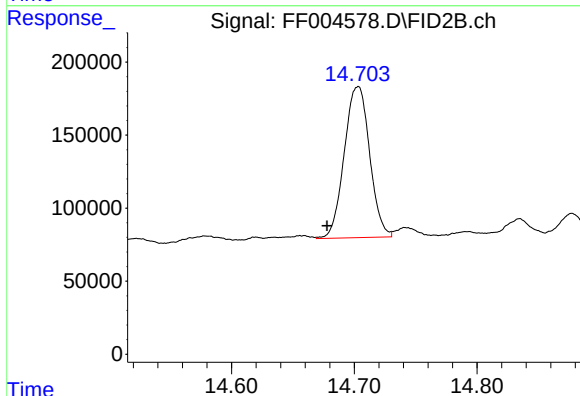


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.703 min
Delta R.T.: 0.025 min
Response: 1486753
Conc: 14.84 ug/ml

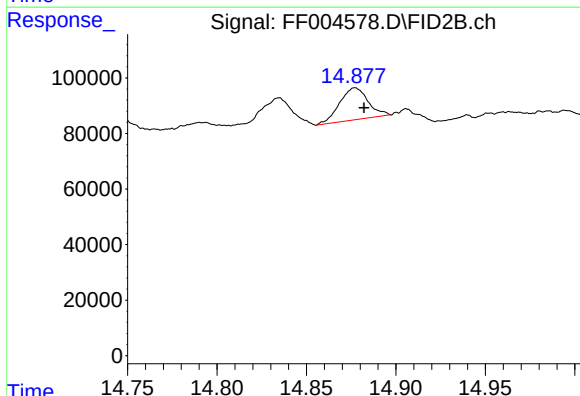


#10 N-TETRACOSANE

R.T.: 14.877 min
Delta R.T.: -0.005 min
Response: 126744
Conc: 1.11 ug/ml

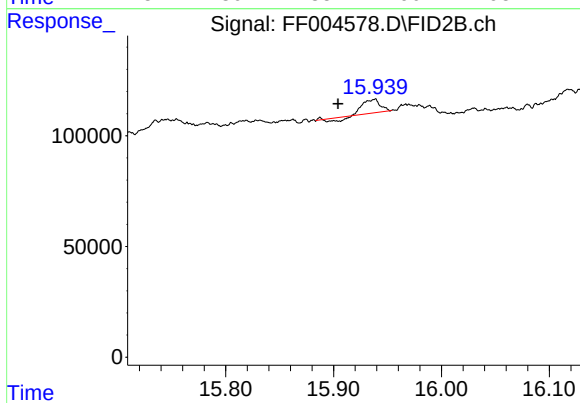


#11 N-HEXACOSANE

R.T.: 15.938 min
Delta R.T.: 0.034 min
Response: 54089
Conc: 0.47 ug/ml

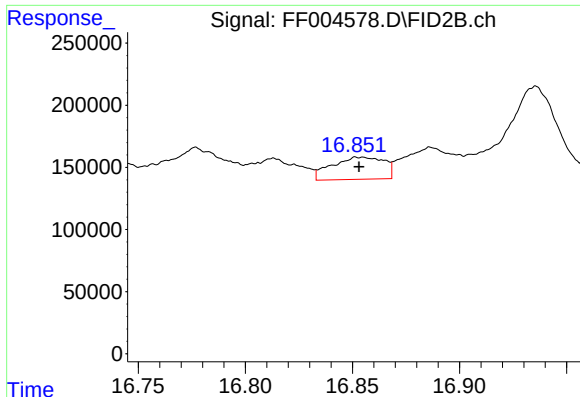


#12 N-OCTACOSANE

R.T.: 16.853 min
Delta R.T.: 0.000 min
Response: 301704
Conc: 2.64 ug/ml

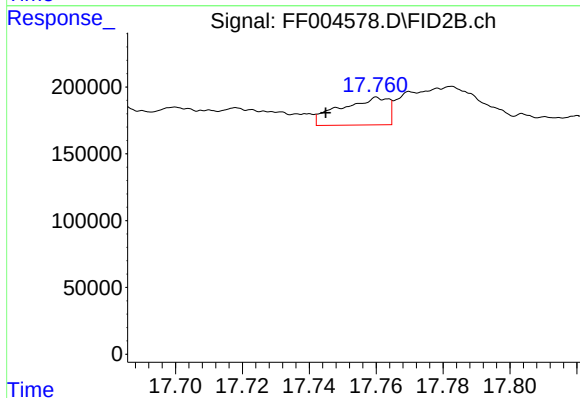


#13 N-TRIACONTANE

R.T.: 17.761 min
Delta R.T.: 0.016 min
Response: 202747
Conc: 1.75 ug/ml

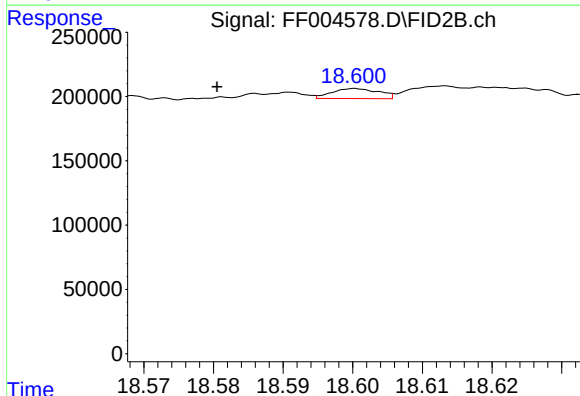


#14 N-DOTRIACONTANE

R.T.: 18.601 min
Delta R.T.: 0.020 min
Response: 36302
Conc: 0.30 ug/ml

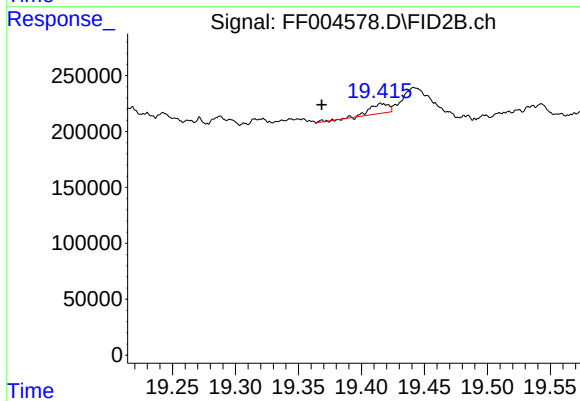

#15 N-TETRATRIACONTANE

R.T.: 19.416 min
Delta R.T.: 0.047 min
Response: 90992
Conc: 0.79 ug/ml

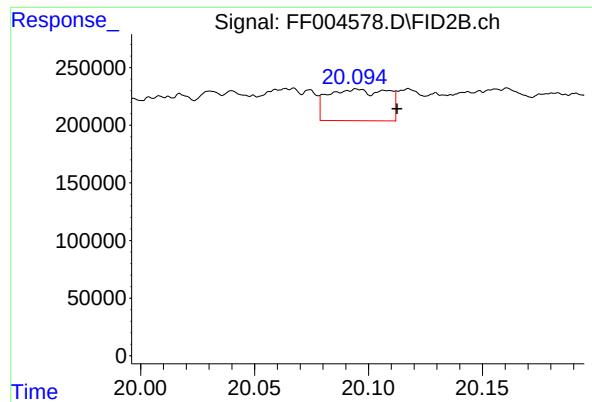

#16 N-HEXATRIACONTANE

R.T.: 20.095 min
Delta R.T.: -0.017 min
Response: 496764
Conc: 4.61 ug/ml