

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052021\
 Data File : FF008458.D
 Signal(s) : FID2B.ch
 Acq On : 20 May 2021 16:53
 Operator : DD\AJ
 Sample : M2432-01 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 21 01:19:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1474020	11.806 ug/ml
Target Compounds			
4) N-TETRADECANE	8.402f	407506	2.916 ug/ml
6) N-OCTADECANE	11.384	123789	0.868 ug/ml
10) N-TETRACOSANE	14.976	226438	1.588 ug/ml
13) N-TRIACONTANE	17.840	195997	1.415 ug/ml
14) N-DOTRIACONTANE	18.664	428900	3.165 ug/ml
15) N-TETRATRIACONTANE	19.374f	97472	0.764 ug/ml
18) N-TETRACONTANE	21.887	284980	2.507 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052021\
Data File : FF008458.D
Signal(s) : FID2B.ch
Acq On : 20 May 2021 16:53
Operator : DD\AJ
Sample : M2432-01 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 21 01:19:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

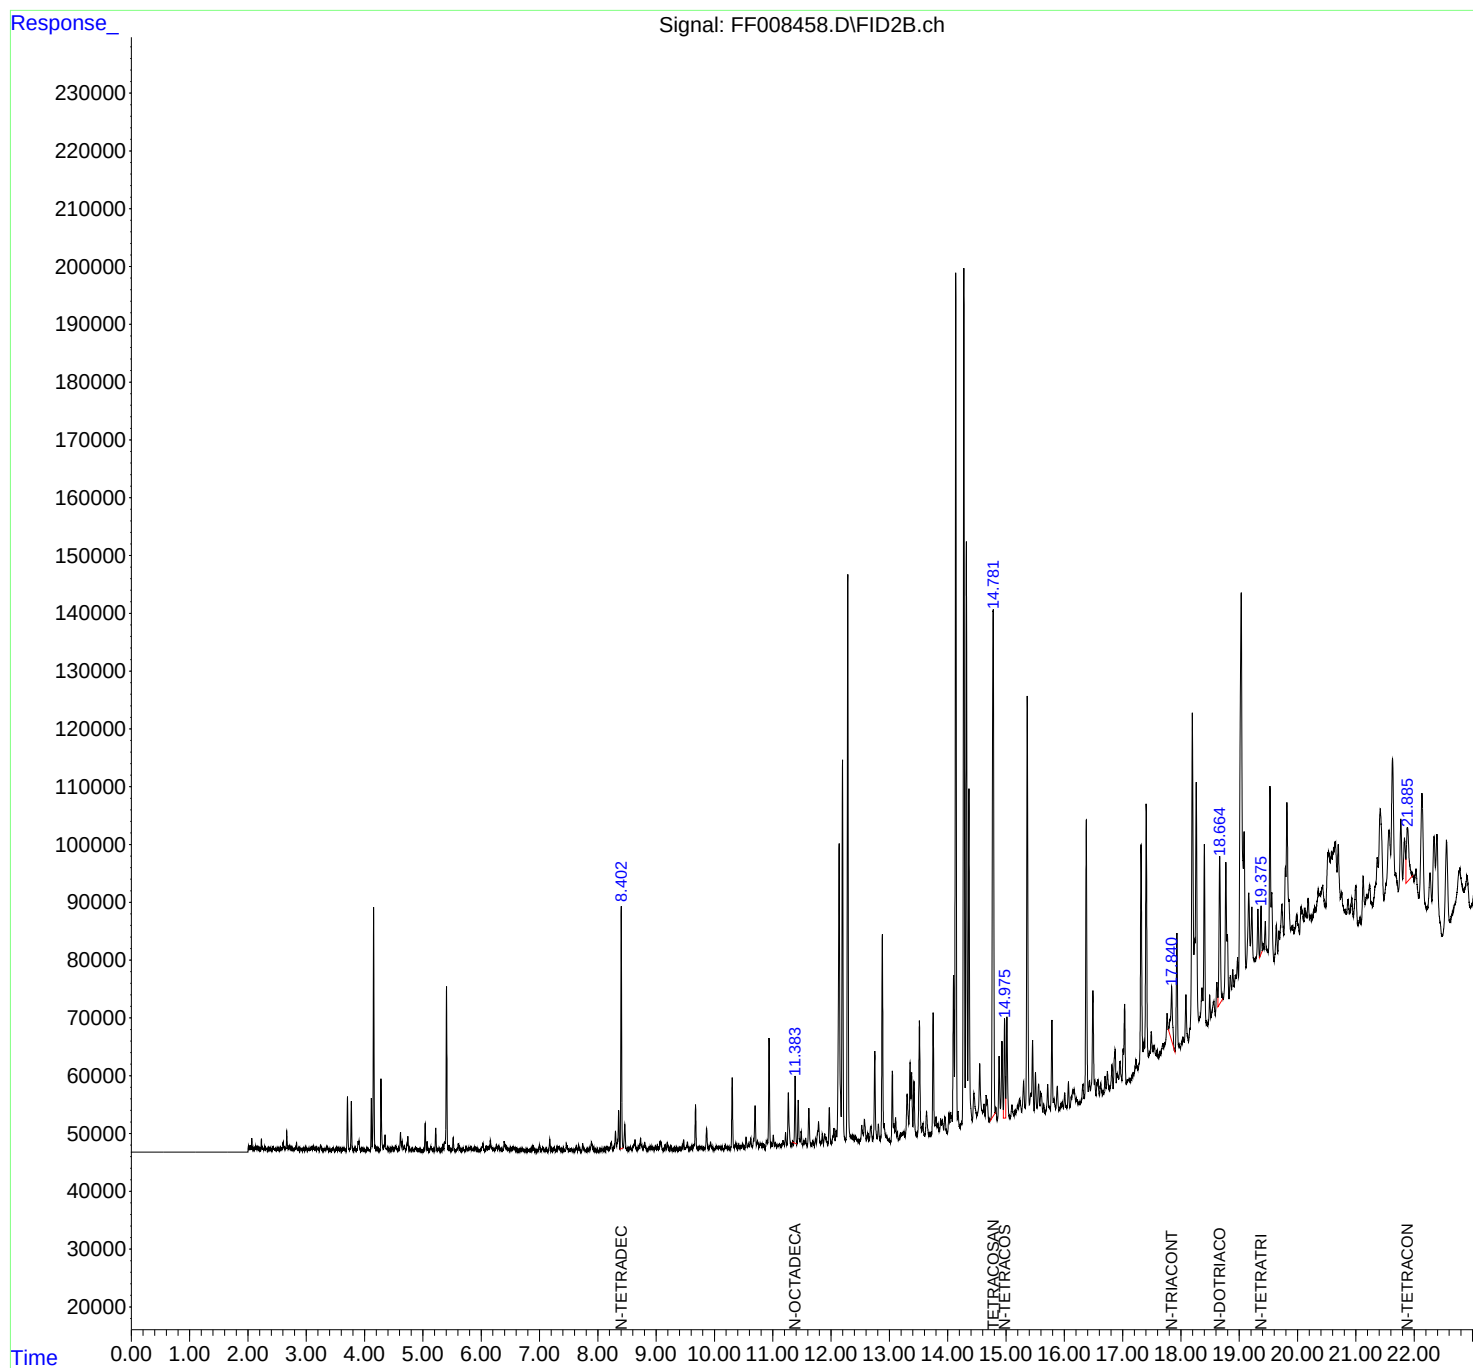


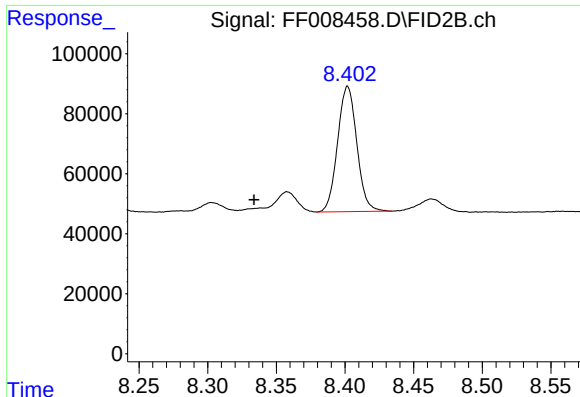

#4 N-TETRADECANE


R.T.: 8.402 min
Delta R.T.: 0.068 min
Response: 407506
Conc: 2.92 ug/ml

Instrument :
FID_F
ClientSampleId :

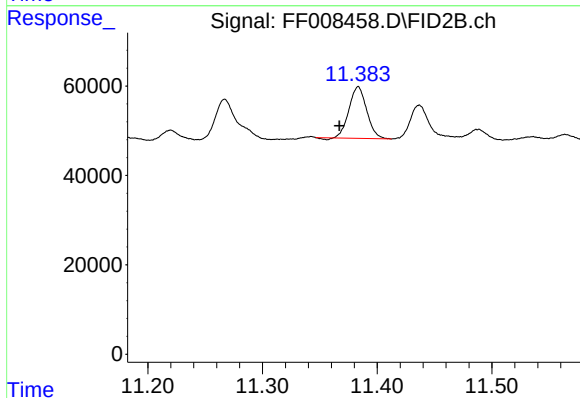


#6 N-OCTADECANE

R.T.: 11.384 min
Delta R.T.: 0.016 min
Response: 123789
Conc: 0.87 ug/ml

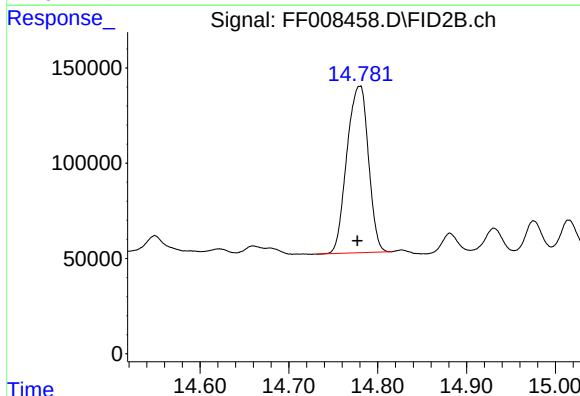


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: 0.003 min
Response: 1474020
Conc: 11.81 ug/ml

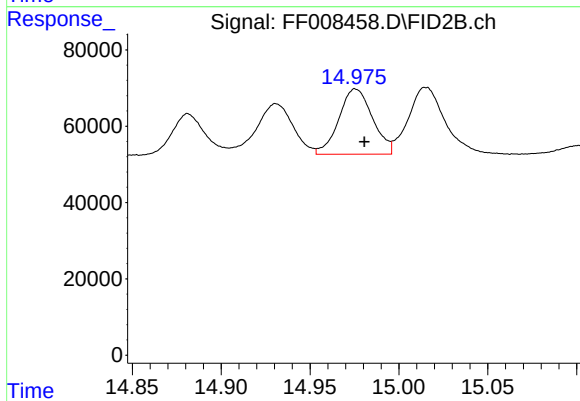

#10 N-TETRACOSANE


R.T.: 14.976 min
Delta R.T.: -0.005 min
Response: 226438
Conc: 1.59 ug/ml

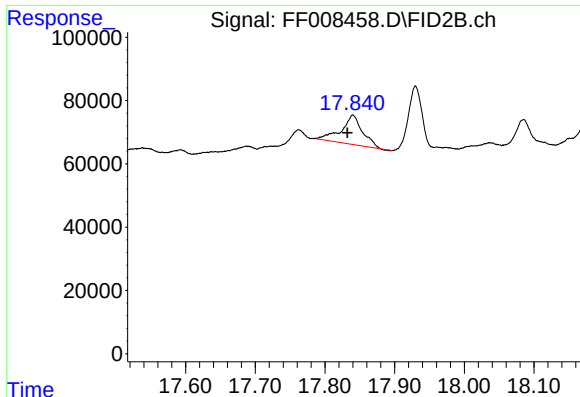

#13 N-TRIACONTANE


R.T.: 17.840 min
Delta R.T.: 0.008 min
Response: 195997
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

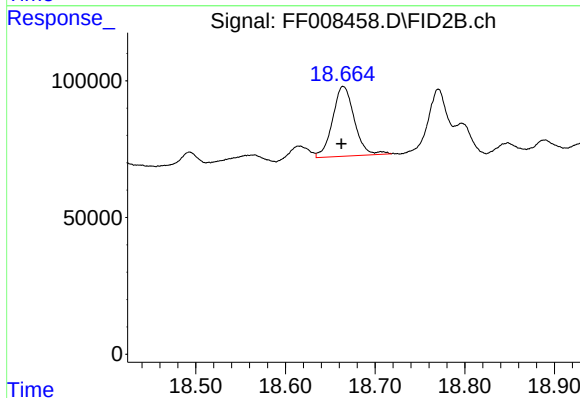


#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: 0.002 min
Response: 428900
Conc: 3.17 ug/ml

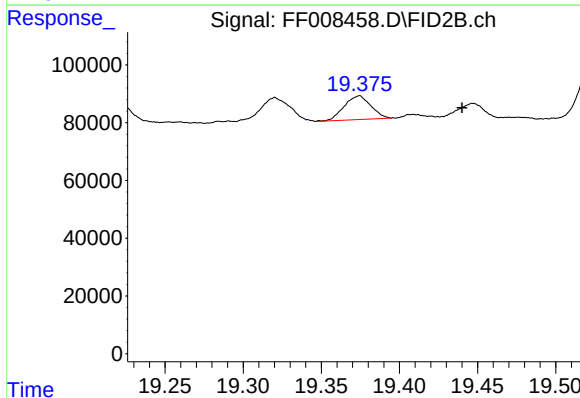

#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: -0.066 min
Response: 97472
Conc: 0.76 ug/ml

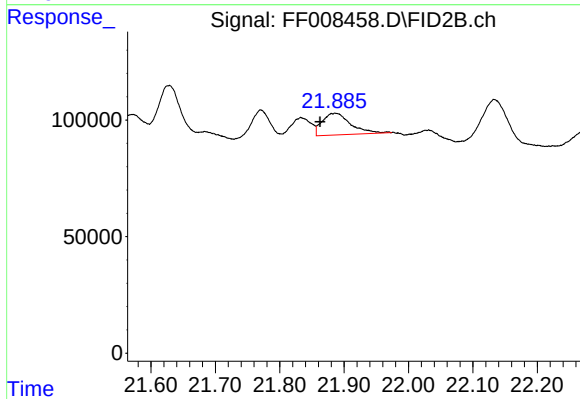

#18 N-TETRACONTANE

R.T.: 21.887 min
Delta R.T.: 0.024 min
Response: 284980
Conc: 2.51 ug/ml