

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052319\
 Data File : FF004608.D
 Signal(s) : FID2B.ch
 Acq On : 23 May 2019 12:34
 Operator : AJ\SJ
 Sample : PB119990BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 24 01:05:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.697	2391290	19.583 ug/ml
Target Compounds			
2) N-DECANE	4.408	3010729	20.561 ug/ml
3) N-DODECANE	6.433	3044391	20.573 ug/ml
4) N-TETRADECANE	8.230	3023504	20.584 ug/ml
5) N-HEXADECANE	9.834	3002163	20.334 ug/ml
6) N-OCTADECANE	11.279	2962508	20.405 ug/ml
7) N-EICOSANE	12.593	2915958	20.134 ug/ml
8) N-DOCOSANE	13.795	2830159	20.029 ug/ml
10) N-TETRACOSANE	14.902	2777483	20.041 ug/ml
11) N-HEXACOSANE	15.927	2716787	19.939 ug/ml
12) N-OCTACOSANE	16.880	2719099	19.999 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052319\
Data File : FF004608.D
Signal(s) : FID2B.ch
Acq On : 23 May 2019 12:34
Operator : AJ\SJ
Sample : PB119990BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 24 01:05:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

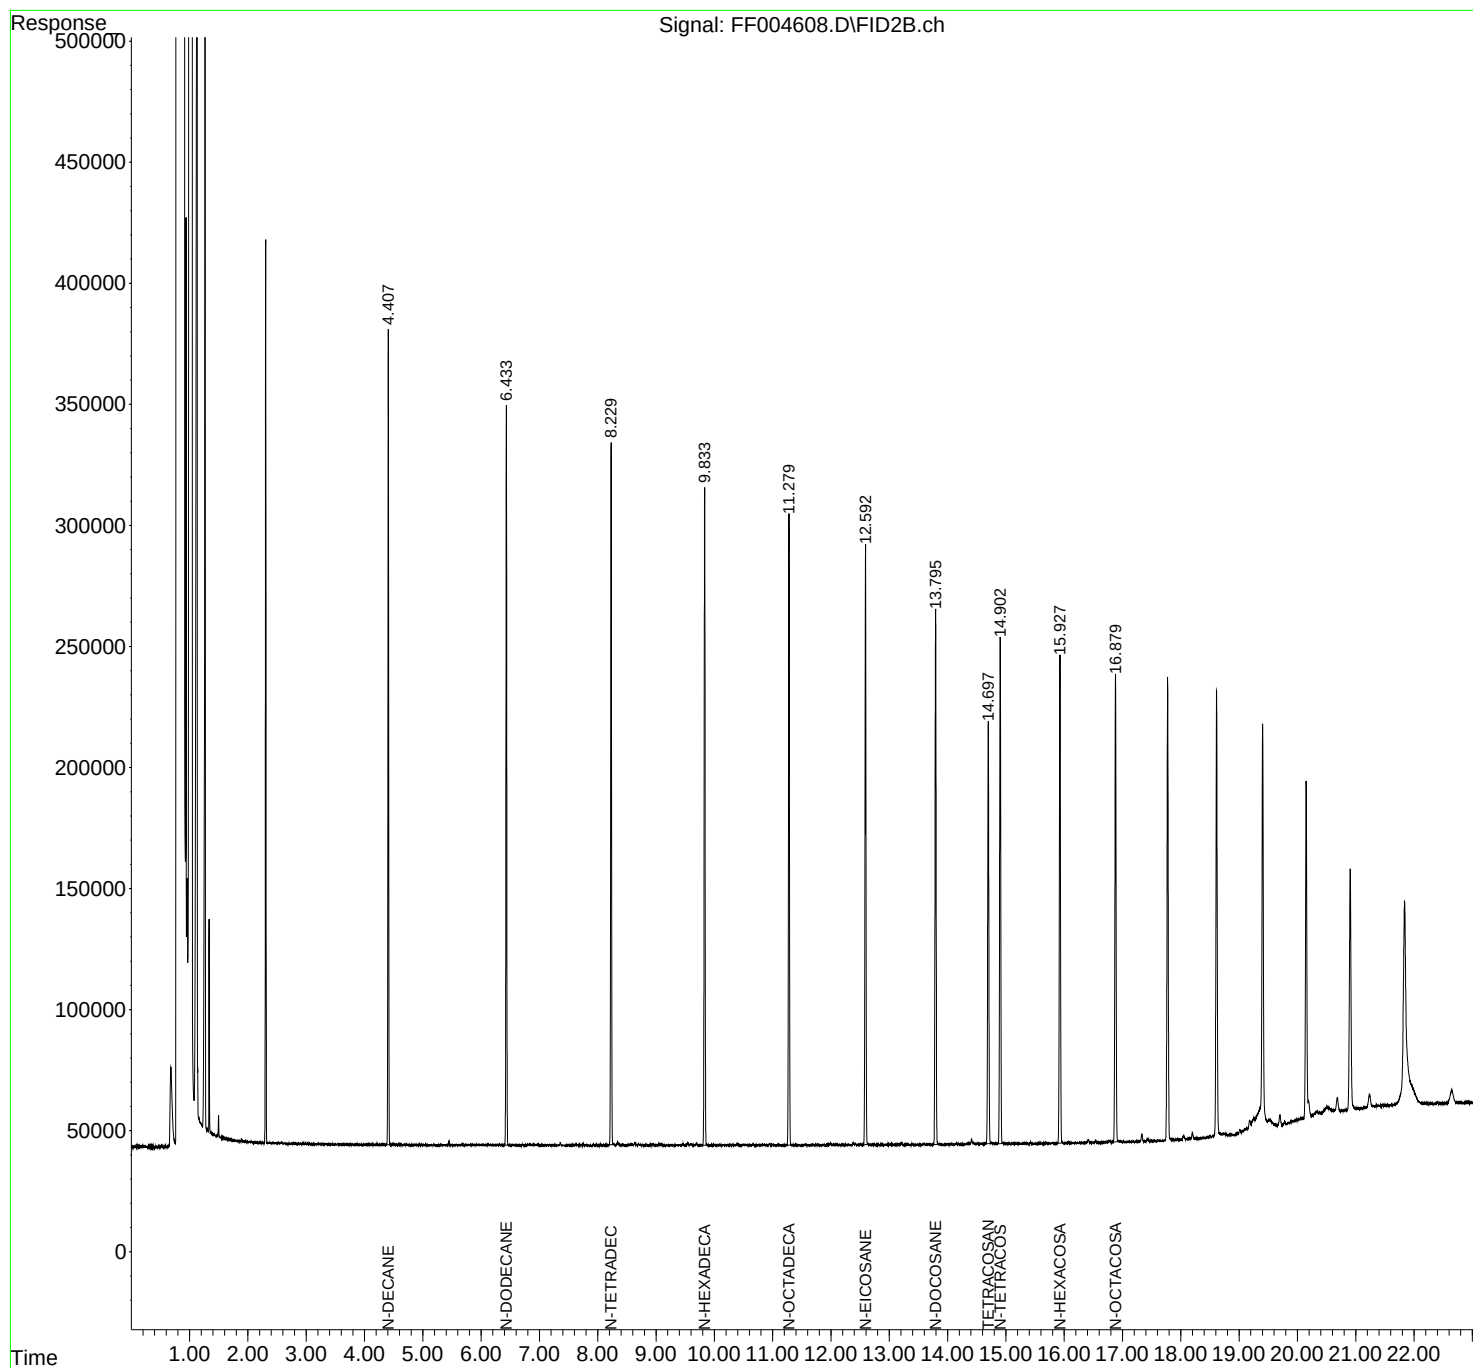

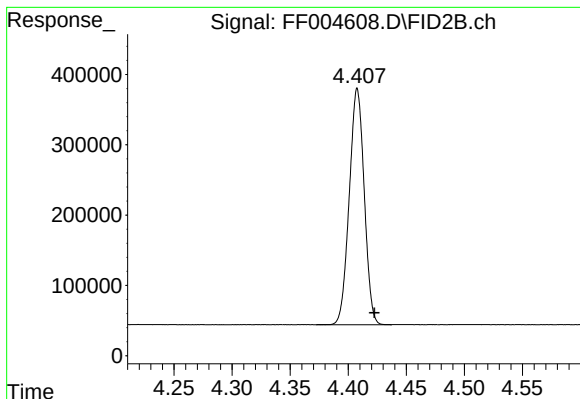


#2 N-DECANE

R.T.: 4.408 min
Delta R.T.: -0.015 min
Response: 3010729
Conc: 20.56 ug/ml

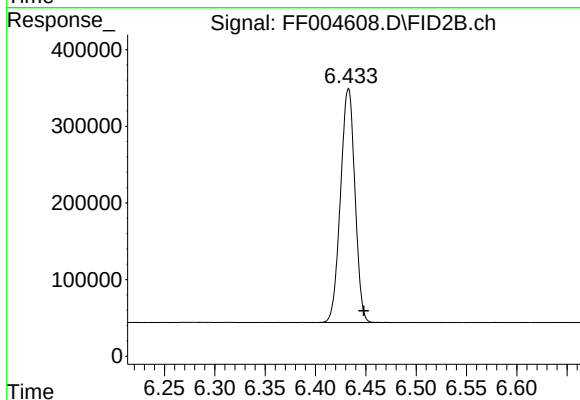


#3 N-DODECANE

R.T.: 6.433 min
Delta R.T.: -0.015 min
Response: 3044391
Conc: 20.57 ug/ml

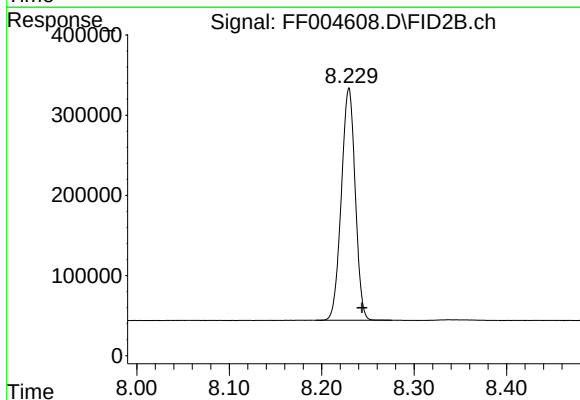


#4 N-TETRADECANE

R.T.: 8.230 min
Delta R.T.: -0.014 min
Response: 3023504
Conc: 20.58 ug/ml

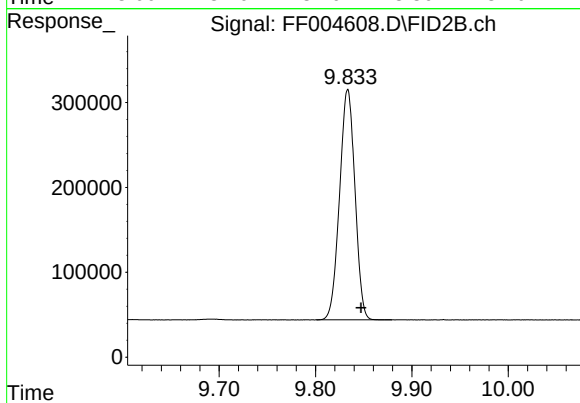


#5 N-HEXADECANE

R.T.: 9.834 min
Delta R.T.: -0.014 min
Response: 3002163
Conc: 20.33 ug/ml

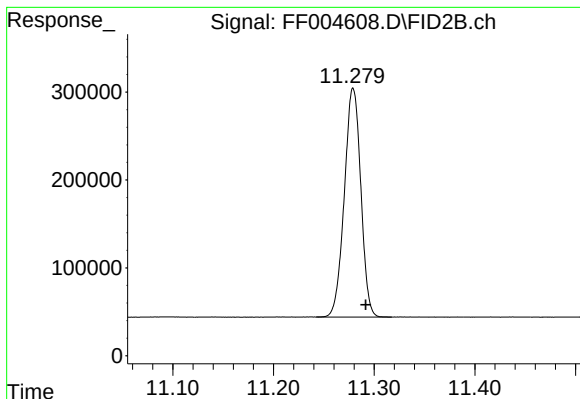


#6 N-OCTADECANE

R.T.: 11.279 min
Delta R.T.: -0.013 min
Response: 2962508
Conc: 20.41 ug/ml

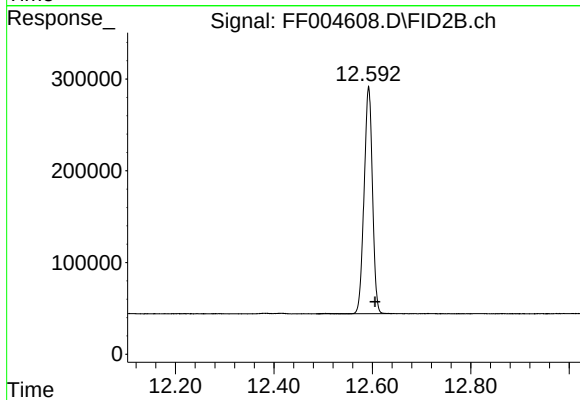


#7 N-EICOSANE

R.T.: 12.593 min
Delta R.T.: -0.013 min
Response: 2915958
Conc: 20.13 ug/ml

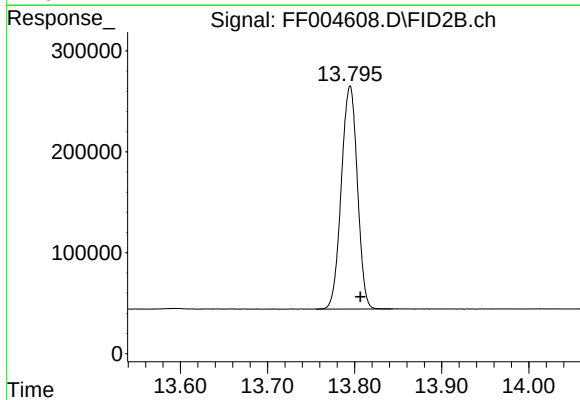


#8 N-DOCOSANE

R.T.: 13.795 min
Delta R.T.: -0.012 min
Response: 2830159
Conc: 20.03 ug/ml

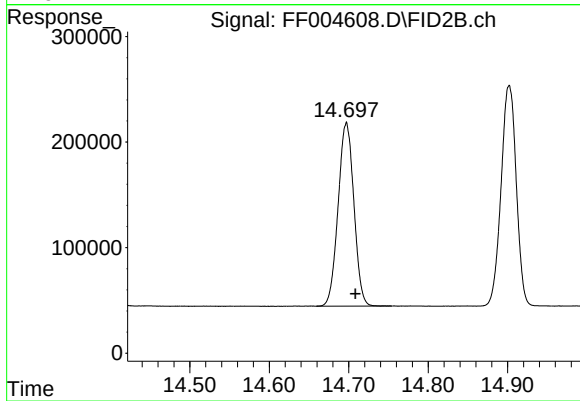


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.697 min
Delta R.T.: -0.011 min
Response: 2391290
Conc: 19.58 ug/ml

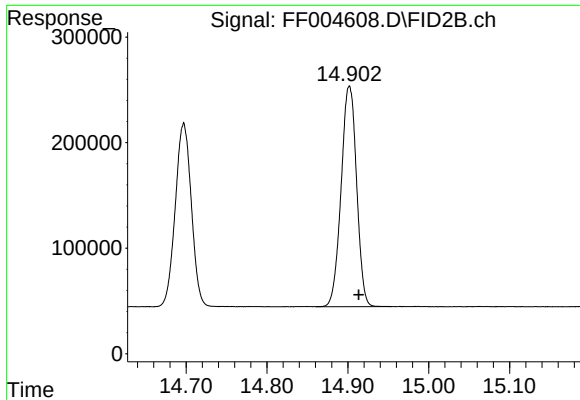


#10 N-TETRACOSANE

R.T.: 14.902 min
Delta R.T.: -0.012 min
Response: 2777483
Conc: 20.04 ug/ml

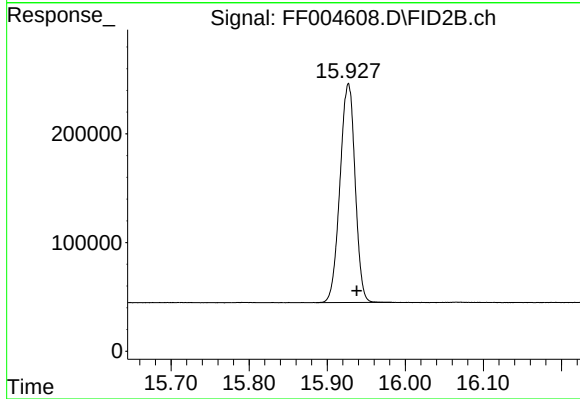

#11 N-HEXACOSANE

R.T.: 15.927 min
Delta R.T.: -0.010 min
Response: 2716787
Conc: 19.94 ug/ml

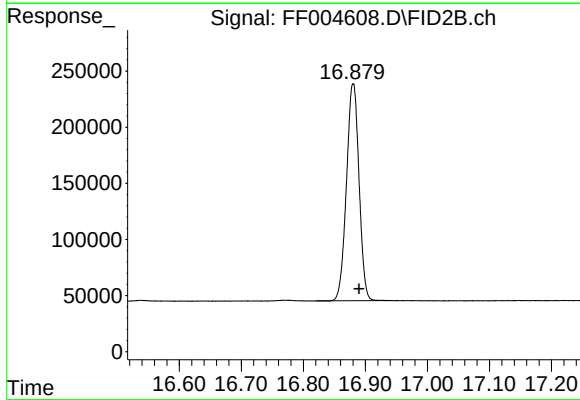

#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: -0.009 min
Response: 2719099
Conc: 20.00 ug/ml