

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052419\
 Data File : FF004624.D
 Signal(s) : FID2B.ch
 Acq On : 24 May 2019 17:07
 Operator : AJ\SJ
 Sample : K3008-01 20X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: May 24 22:49:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.702	193444	1.584 ug/ml
Target Compounds			
7) N-EICOSANE	12.653	2194949	15.156 ug/ml
8) N-DOCOSANE	13.818	202394	1.432 ug/ml
10) N-TETRACOSANE	14.877	1195284	8.625 ug/ml
12) N-OCTACOSANE	16.880	357467	2.629 ug/ml
13) N-TRIACONTANE	17.777	340646	2.463 ug/ml
14) N-DOTRIACONTANE	18.616	174701	1.263 ug/ml
15) N-TETRATRIACONTANE	19.403	79271	0.580 ug/ml
16) N-HEXATRIACONTANE	20.196	81385	0.618 ug/ml
18) N-TETRACONTANE	21.881	545987	4.434 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052419\
Data File : FF004624.D
Signal(s) : FID2B.ch
Acq On : 24 May 2019 17:07
Operator : AJ\SJ
Sample : K3008-01 20X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: May 24 22:49:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

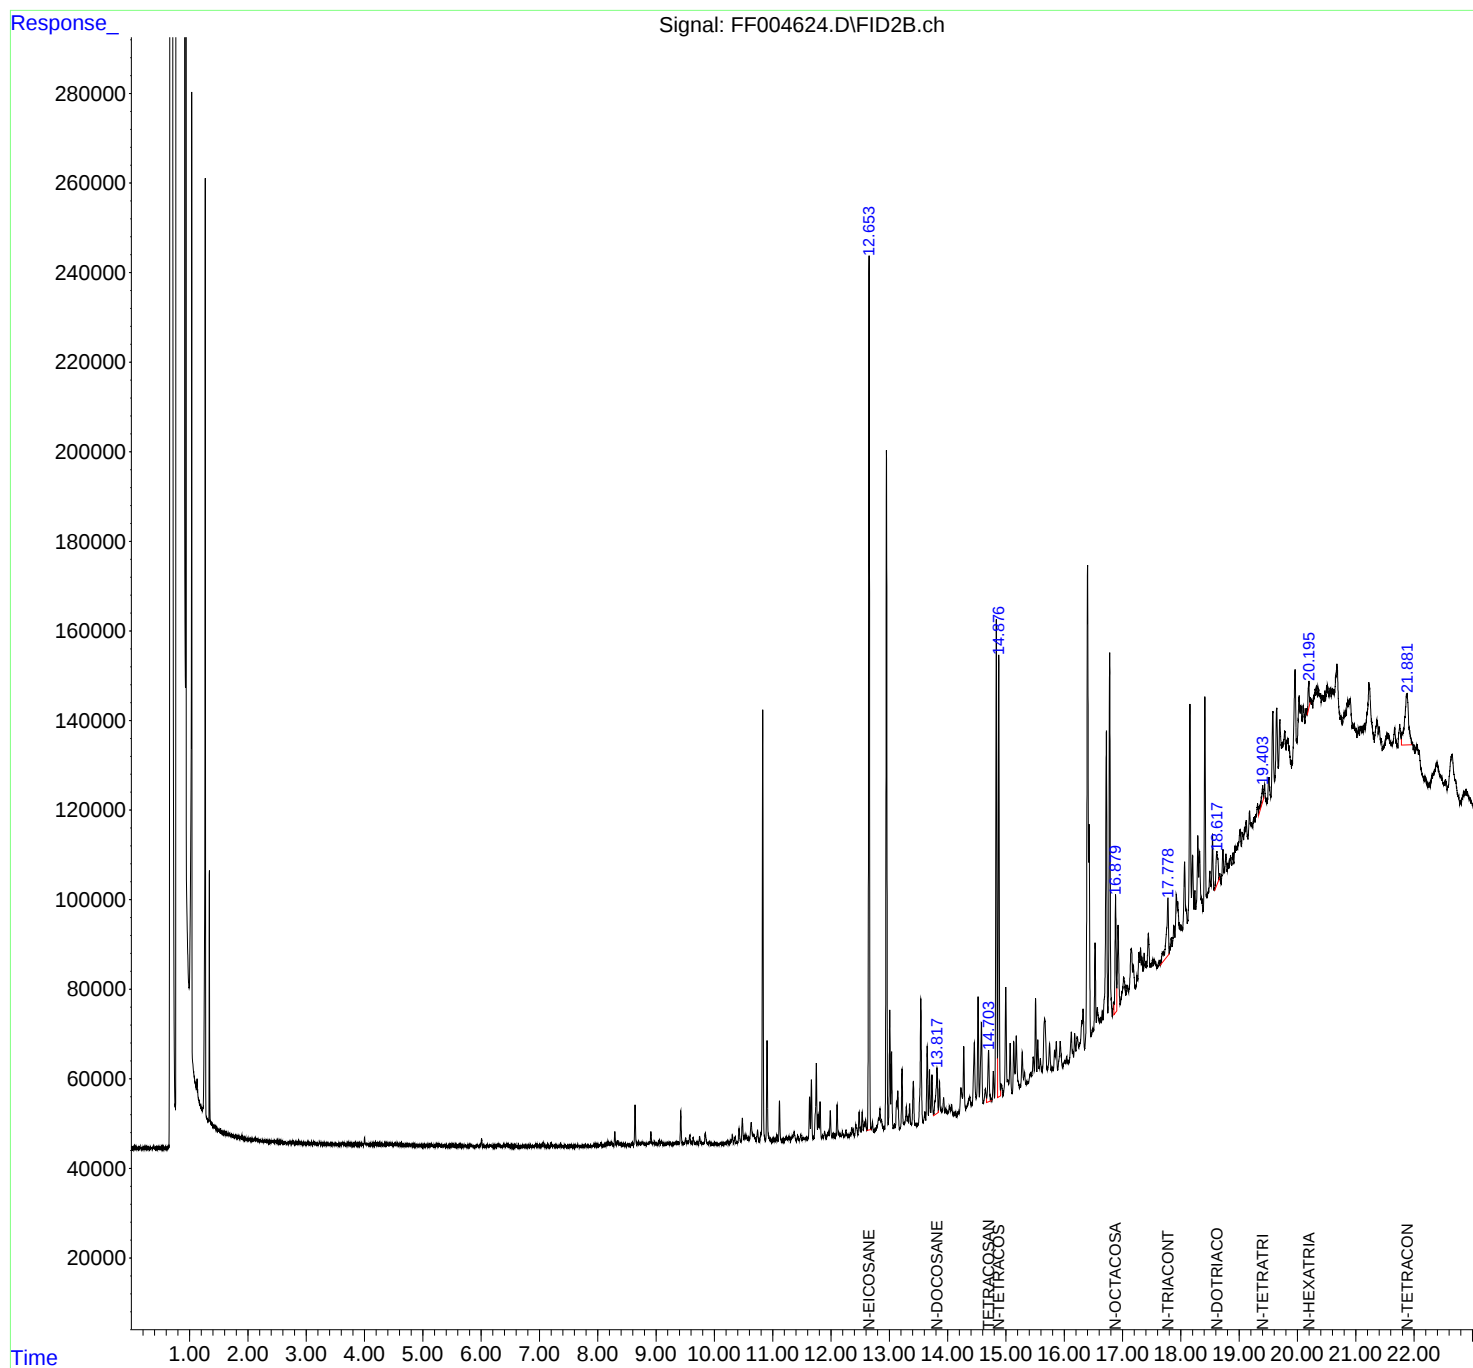

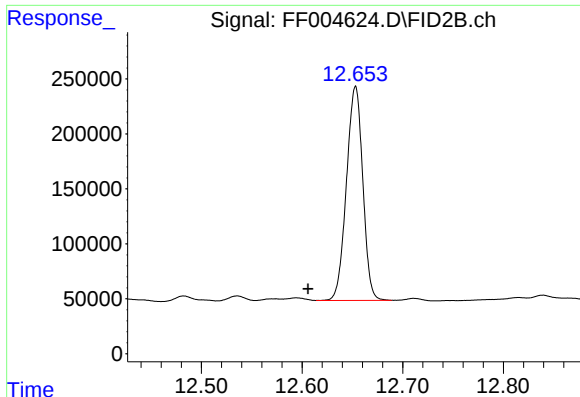


#7 N-EICOSANE

R.T.: 12.653 min
Delta R.T.: 0.047 min
Response: 2194949
Conc: 15.16 ug/ml

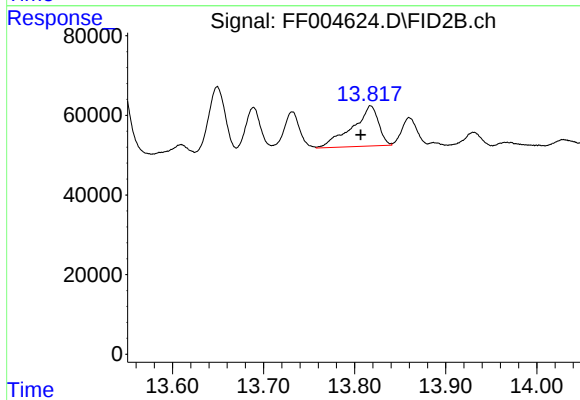


#8 N-DOCOSANE

R.T.: 13.818 min
Delta R.T.: 0.011 min
Response: 202394
Conc: 1.43 ug/ml

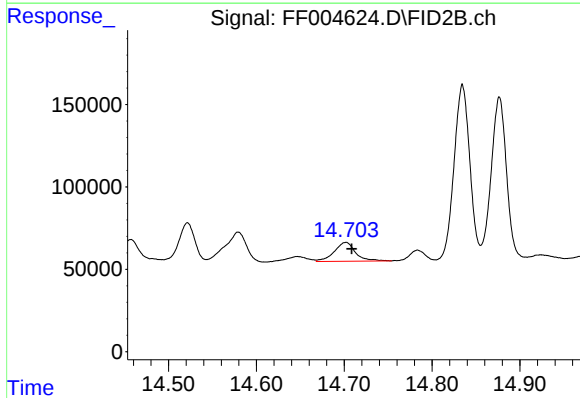


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.702 min
Delta R.T.: -0.006 min
Response: 193444
Conc: 1.58 ug/ml

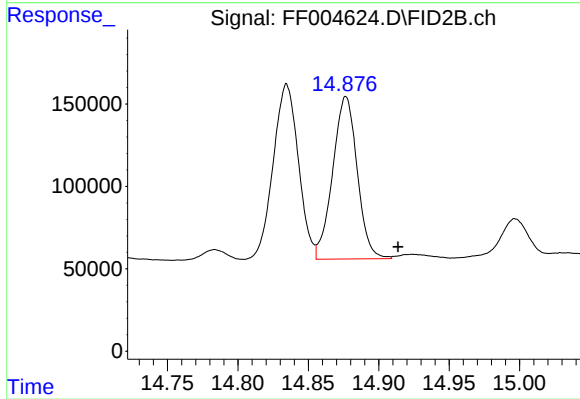


#10 N-TETRACOSANE

R.T.: 14.877 min
Delta R.T.: -0.037 min
Response: 1195284
Conc: 8.62 ug/ml

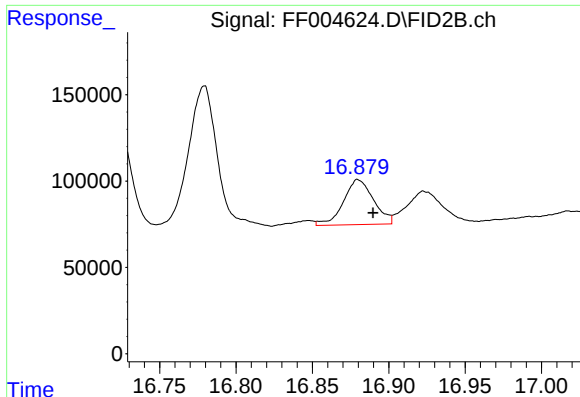


#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: -0.010 min
Response: 357467
Conc: 2.63 ug/ml

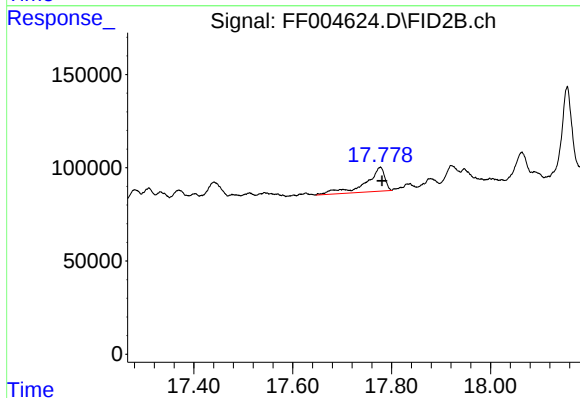


#13 N-TRIACONTANE

R.T.: 17.777 min
Delta R.T.: -0.004 min
Response: 340646
Conc: 2.46 ug/ml

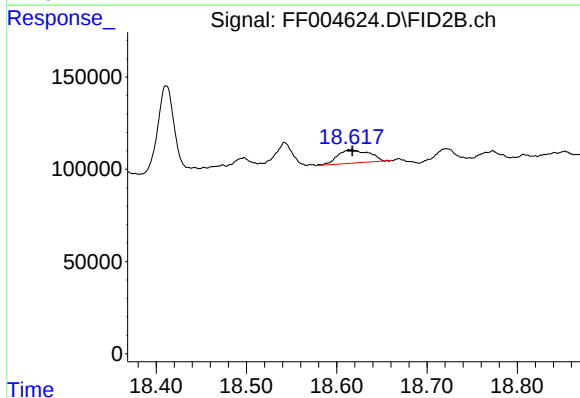


#14 N-DOTRIACONTANE

R.T.: 18.616 min
Delta R.T.: -0.001 min
Response: 174701
Conc: 1.26 ug/ml

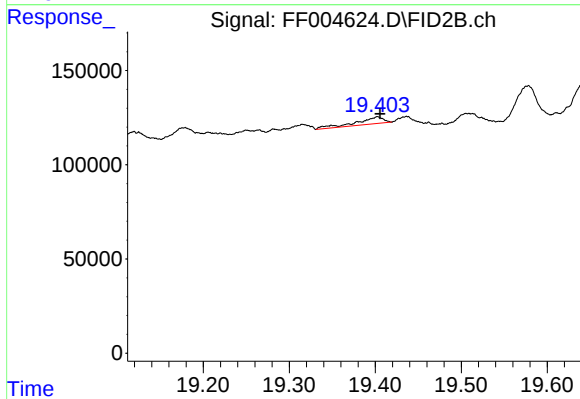


#15 N-TETRATRIACONTANE

R.T.: 19.403 min
Delta R.T.: -0.003 min
Response: 79271
Conc: 0.58 ug/ml

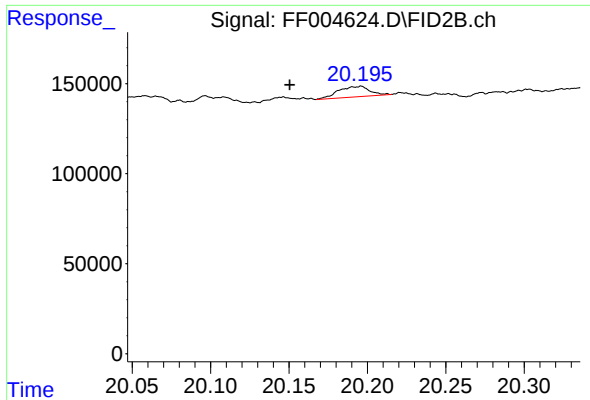

#16 N-HEXATRIACONTANE

R.T.: 20.196 min
Delta R.T.: 0.045 min
Response: 81385
Conc: 0.62 ug/ml

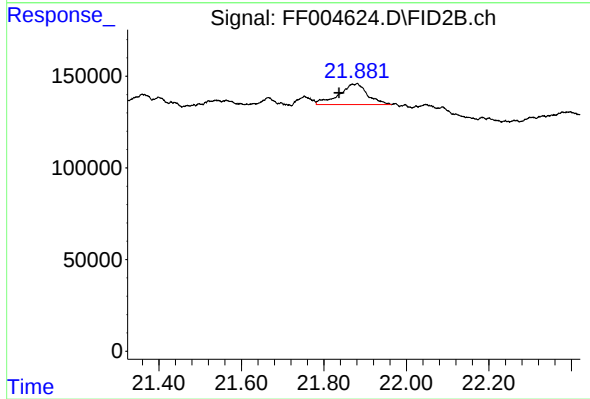

#18 N-TETRACONTANE

R.T.: 21.881 min
Delta R.T.: 0.044 min
Response: 545987
Conc: 4.43 ug/ml