

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052423\
 Data File : FF012749.D
 Signal(s) : FID2B.ch
 Acq On : 25 May 2023 03:22
 Operator : YP\AJ
 Sample : 02899-09
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 25 05:43:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
 Quant Title :
 QLast Update : Fri May 05 16:23:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.980	749813	6.211 ug/ml
Target Compounds			
7) N-EICOSANE	12.963f	323497	2.337 ug/ml
10) N-TETRACOSANE	15.183	205306	1.539 ug/ml
11) N-HEXACOSANE	16.273f	436546	3.367 ug/ml
12) N-OCTACOSANE	17.183	386002	3.046 ug/ml
13) N-TRIACONTANE	18.047	1369934	10.953 ug/ml
14) N-DOTRIACONTANE	18.879	1176827	9.851 ug/ml
15) N-TETRATRIACONTANE	19.671	228343	2.076 ug/ml
16) N-HEXATRIACONTANE	20.409	534823	5.140 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052423\
Data File : FF012749.D
Signal(s) : FID2B.ch
Acq On : 25 May 2023 03:22
Operator : YP\AJ
Sample : 02899-09
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 25 05:43:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

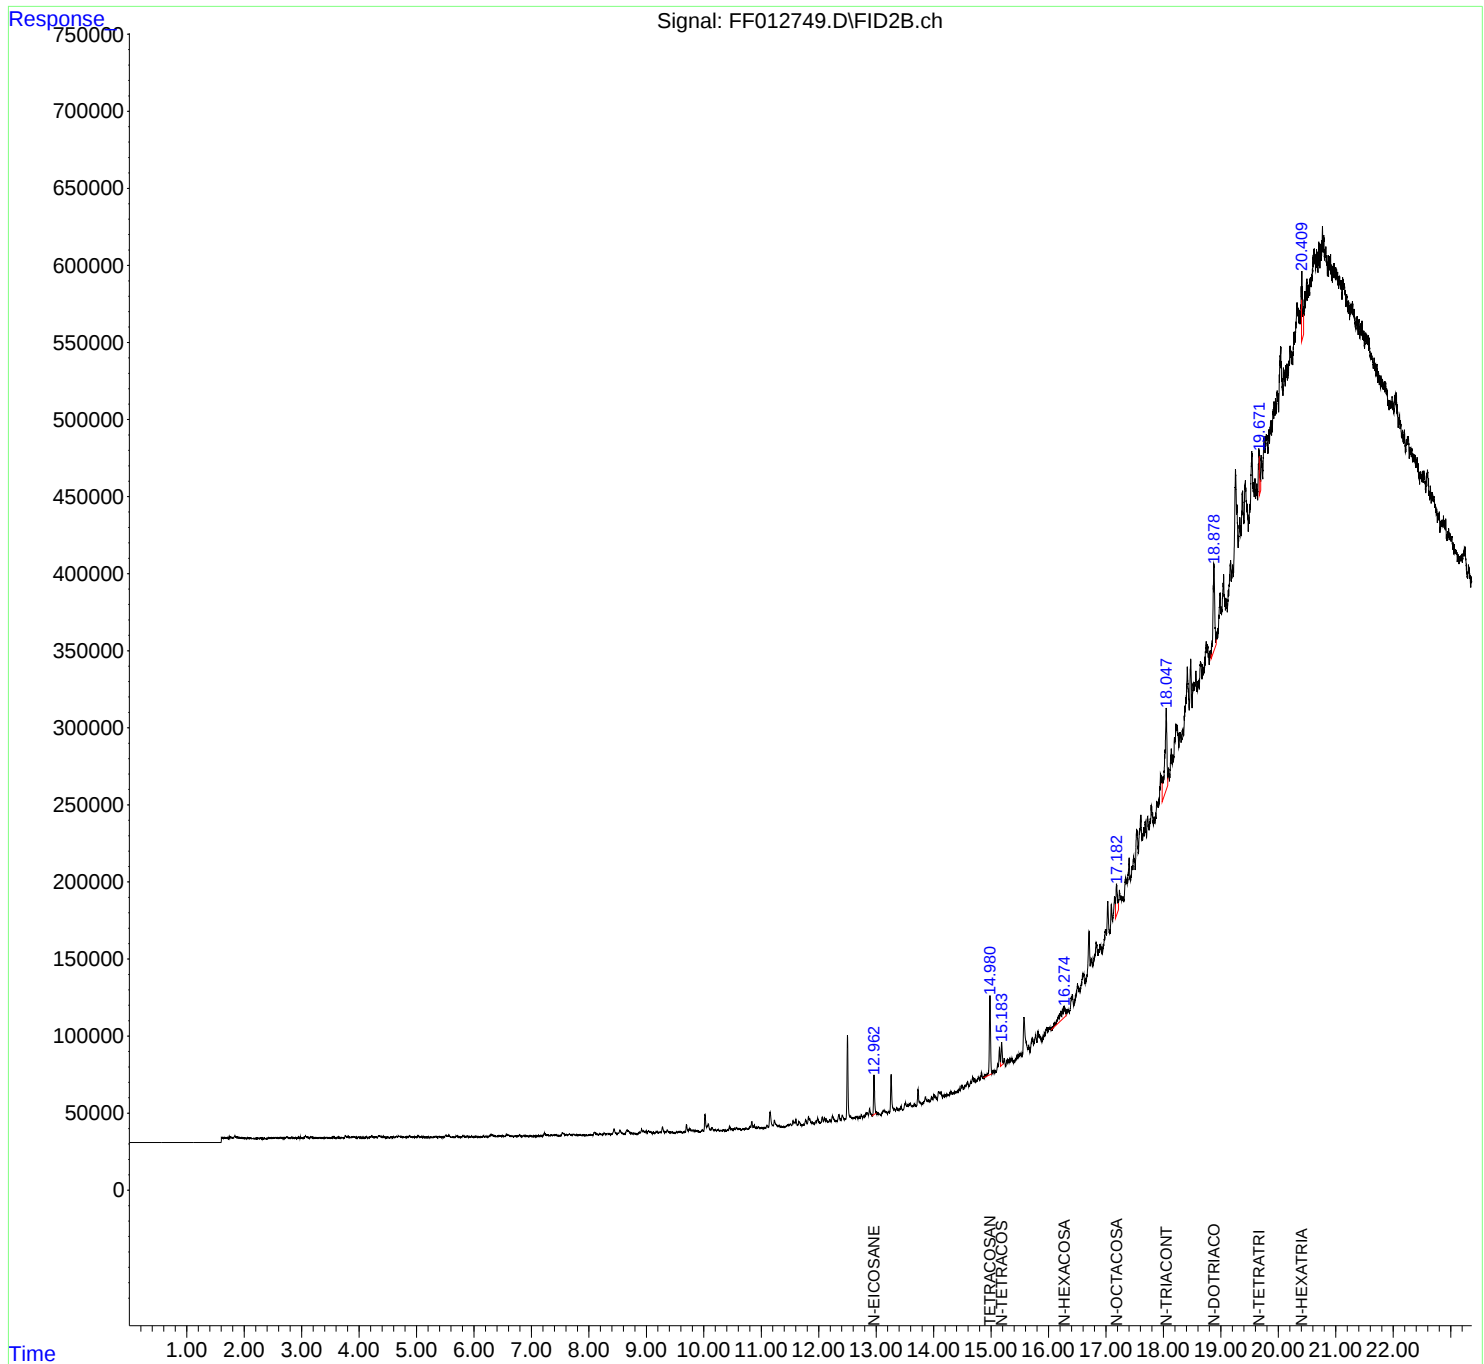


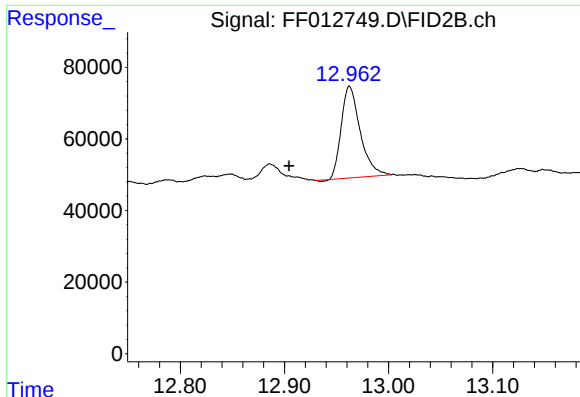

#7 N-EICOSANE


R.T.: 12.963 min
Delta R.T.: 0.058 min
Response: 323497
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :

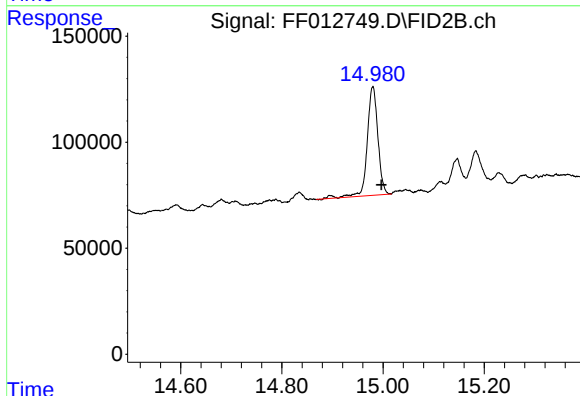


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.980 min
Delta R.T.: -0.017 min
Response: 749813
Conc: 6.21 ug/ml

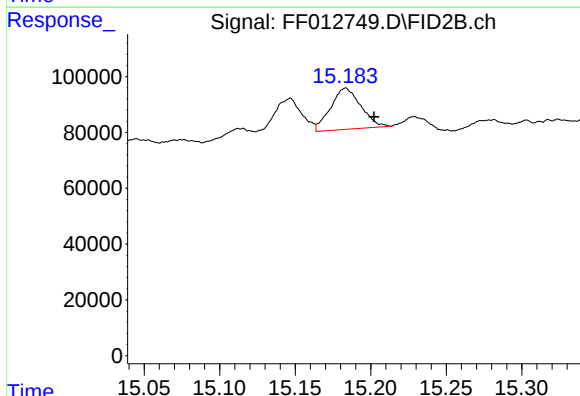


#10 N-TETRACOSANE

R.T.: 15.183 min
Delta R.T.: -0.019 min
Response: 205306
Conc: 1.54 ug/ml

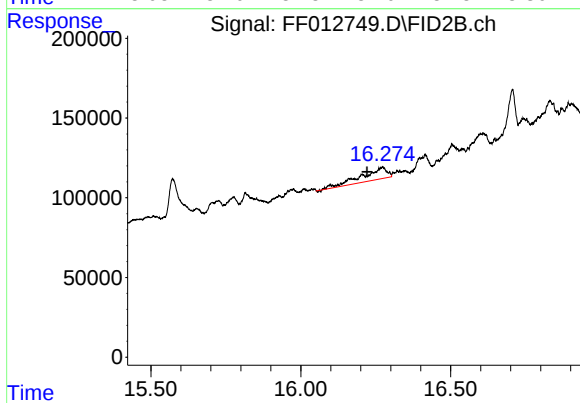

#11 N-HEXACOSANE


R.T.: 16.273 min
Delta R.T.: 0.052 min
Response: 436546
Conc: 3.37 ug/ml

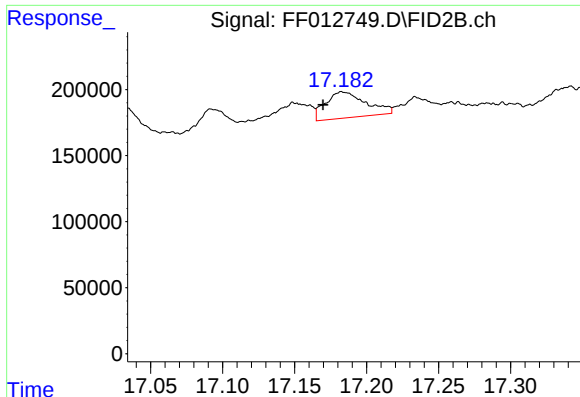

#12 N-OCTACOSANE


R.T.: 17.183 min
Delta R.T.: 0.013 min
Response: 386002
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :

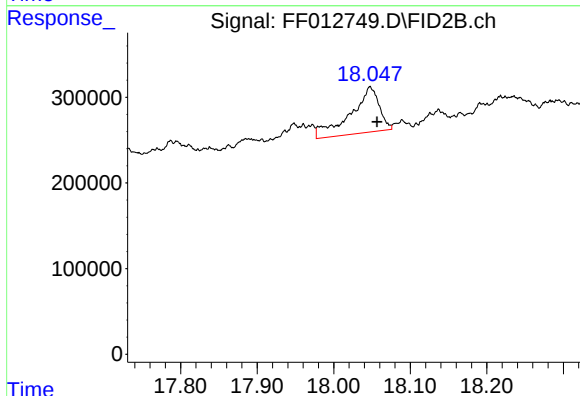


#13 N-TRIACONTANE

R.T.: 18.047 min
Delta R.T.: -0.009 min
Response: 1369934
Conc: 10.95 ug/ml

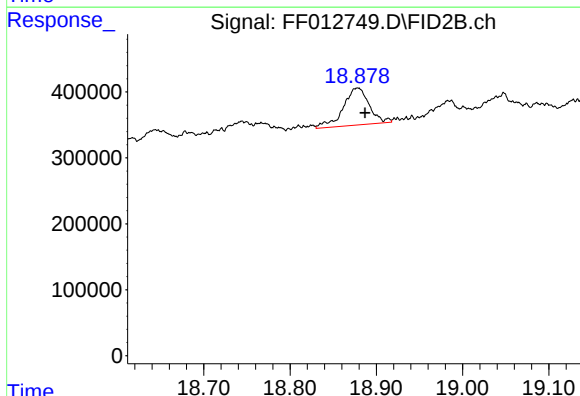


#14 N-DOTRIACONTANE

R.T.: 18.879 min
Delta R.T.: -0.008 min
Response: 1176827
Conc: 9.85 ug/ml

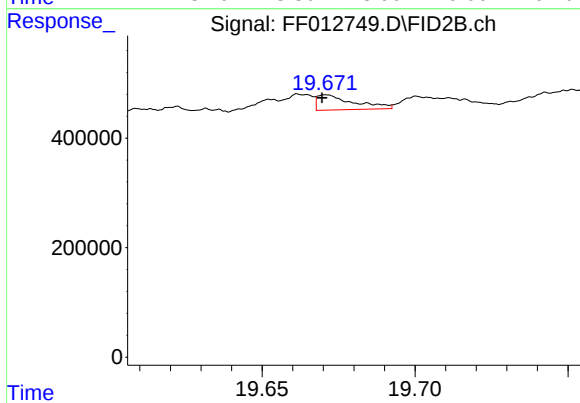

#15 N-TETRATRIACONTANE

R.T.: 19.671 min
Delta R.T.: 0.001 min
Response: 228343
Conc: 2.08 ug/ml

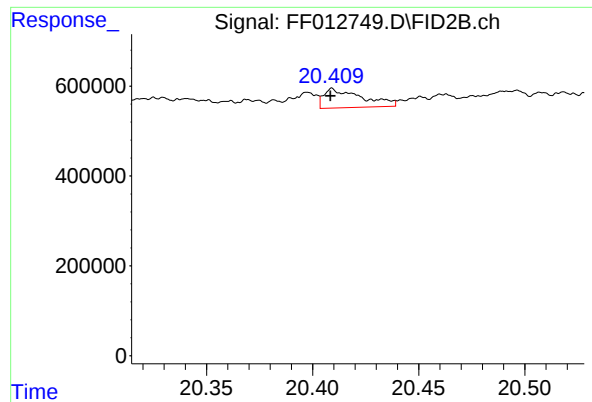

#16 N-HEXATRIACONTANE

R.T.: 20.409 min
Delta R.T.: 0.000 min
Response: 534823
Conc: 5.14 ug/ml

Instrument :

FID_F

ClientSampleId :