

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052423\
Data File : FF012750.D
Signal(s) : FID2B.ch
Acq On : 25 May 2023 04:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 25 05:43:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.985	1763024	14.605 ug/ml
Target Compounds				
15)	N-TETRATRIACONTANE	19.662	200910	1.826 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052423\
Data File : FF012750.D
Signal(s) : FID2B.ch
Acq On : 25 May 2023 04:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 25 05:43:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

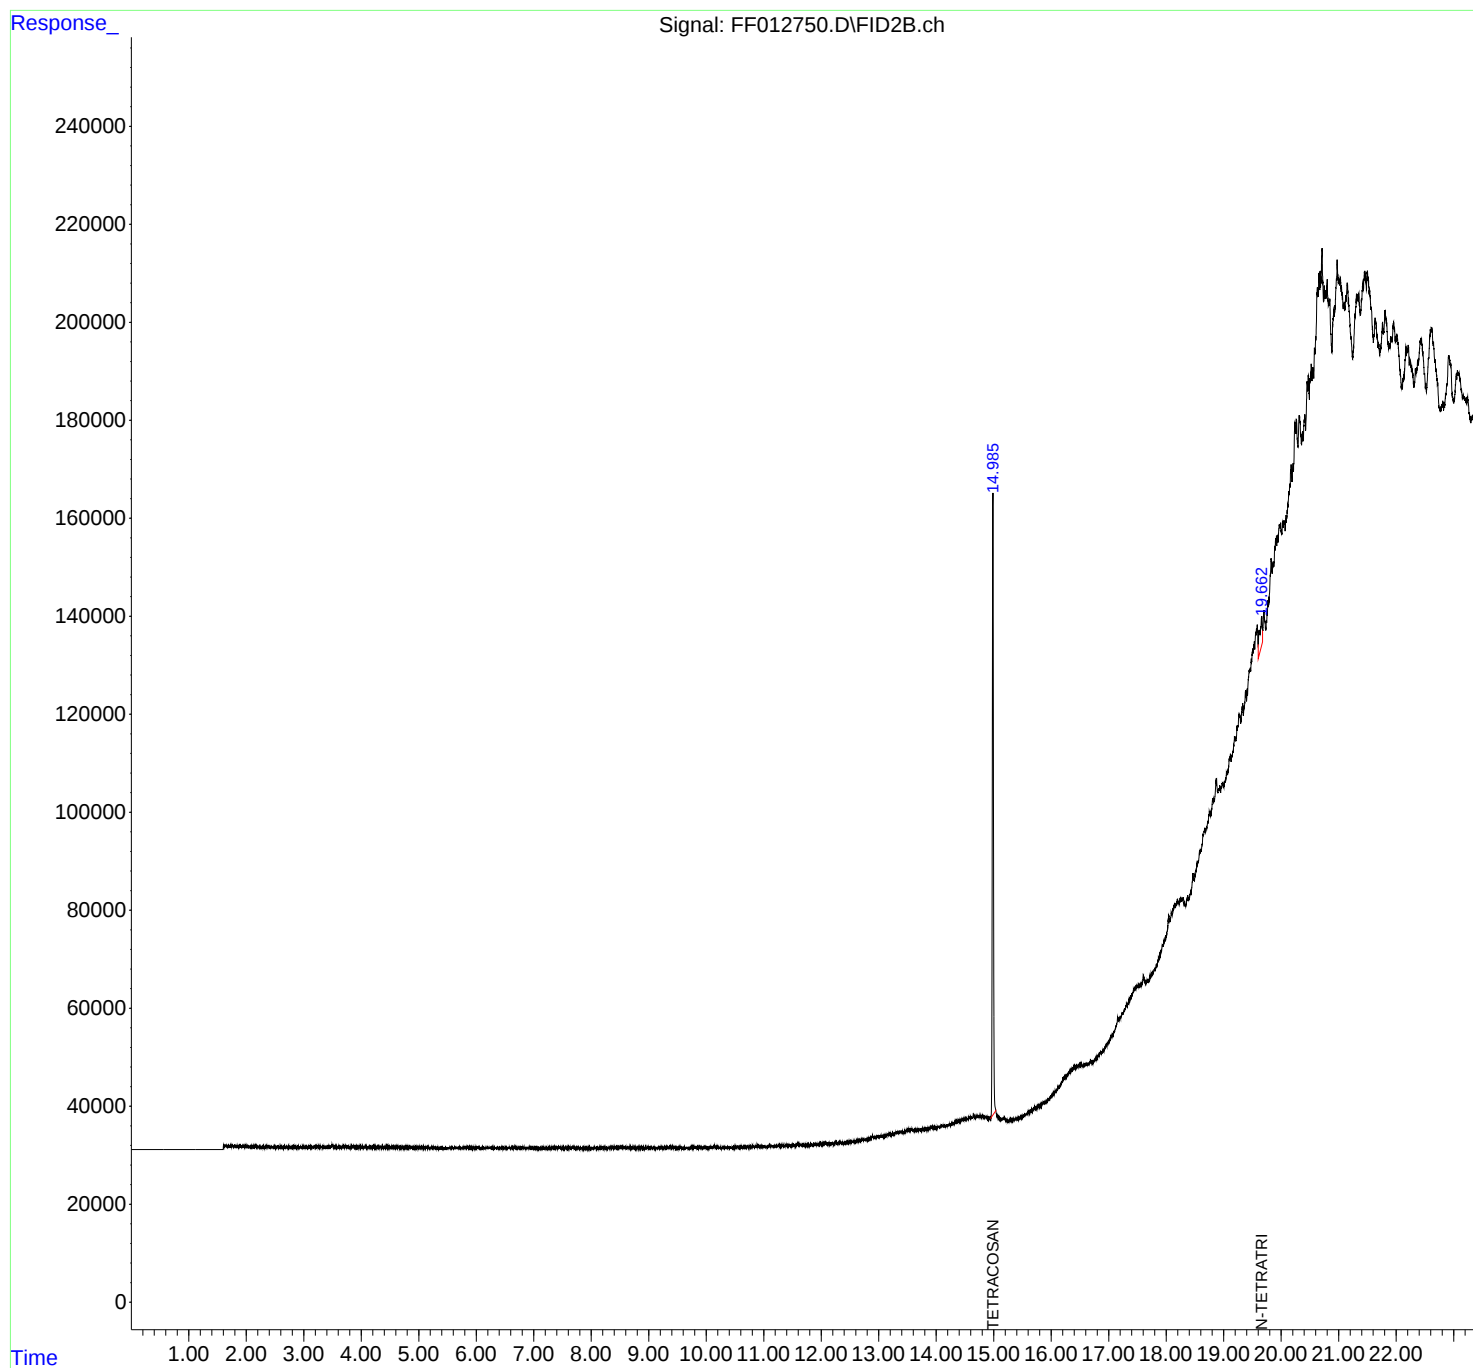


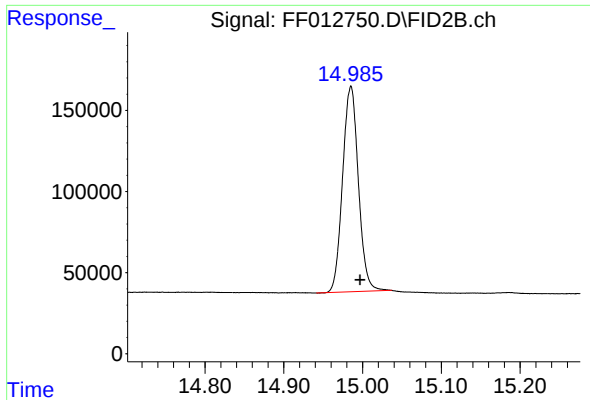

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.985 min
Delta R.T.: -0.012 min
Response: 1763024
Conc: 14.60 ug/ml

Instrument :
FID_F
ClientSampleId :

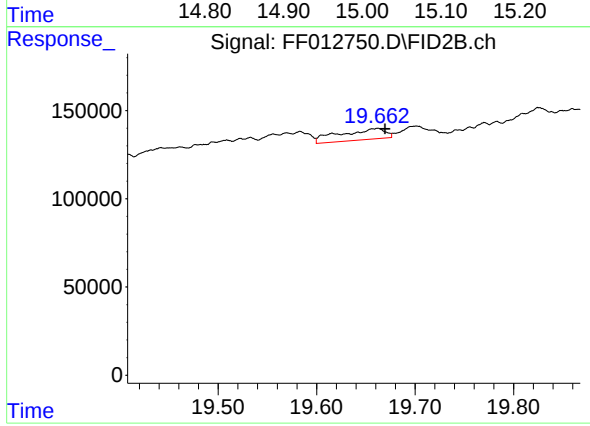

#15 N-TETRATRIACONTANE

R.T.: 19.662 min
Delta R.T.: -0.007 min
Response: 200910
Conc: 1.83 ug/ml