

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
 Data File : FF012769.D
 Signal(s) : FID2B.ch
 Acq On : 26 May 2023 17:56
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 27 02:53:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
 Quant Title :
 QLast Update : Fri May 05 16:23:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.991	1832580	15.181 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.050	1052	0.008 ug/ml
14) N-DOTRIACONTANE	18.887	816217	6.833 ug/ml
15) N-TETRATRIACONTANE	19.663	234541	2.132 ug/ml
16) N-HEXATRIACONTANE	20.428	927621	8.915 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012769.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 17:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 27 02:53:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

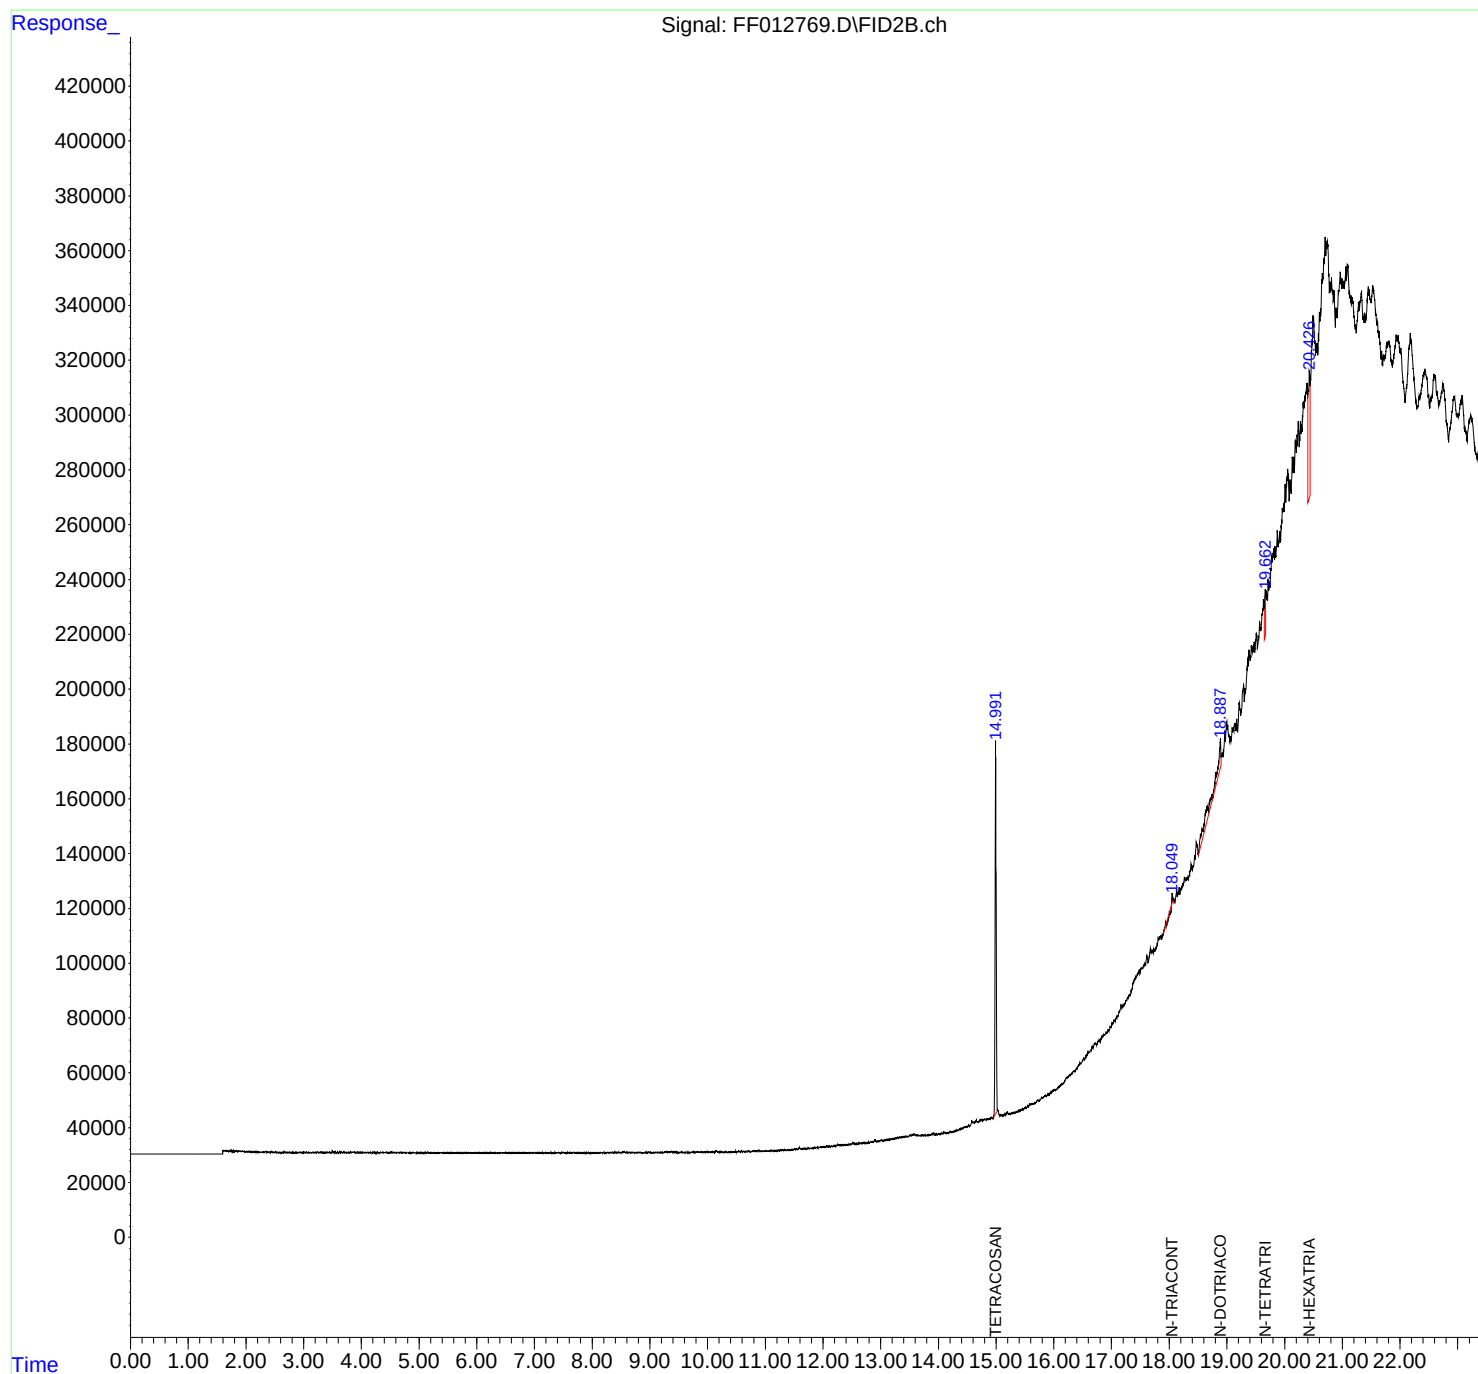


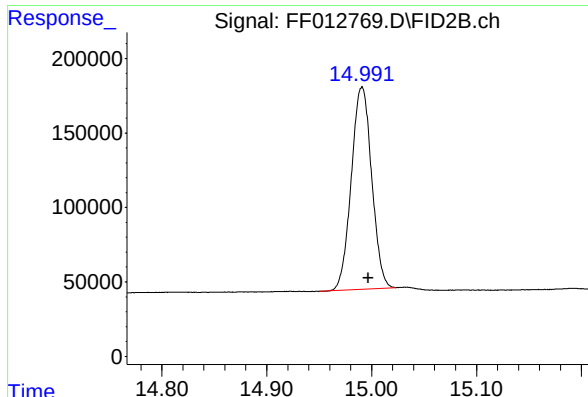

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.991 min
Delta R.T.: -0.006 min
Response: 1832580
Conc: 15.18 ug/ml

Instrument :
FID_F
ClientSampleId :

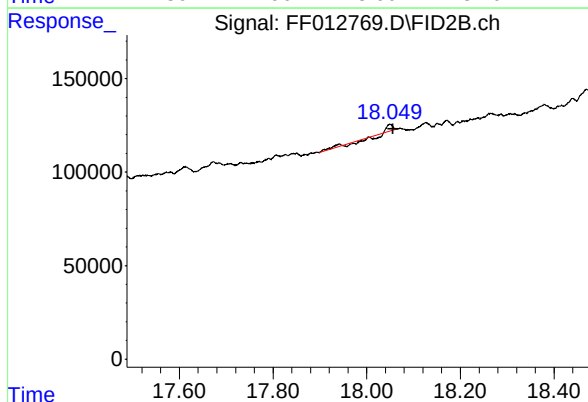


#13 N-TRIACONTANE

R.T.: 18.050 min
Delta R.T.: -0.007 min
Response: 1052
Conc: 0.01 ug/ml

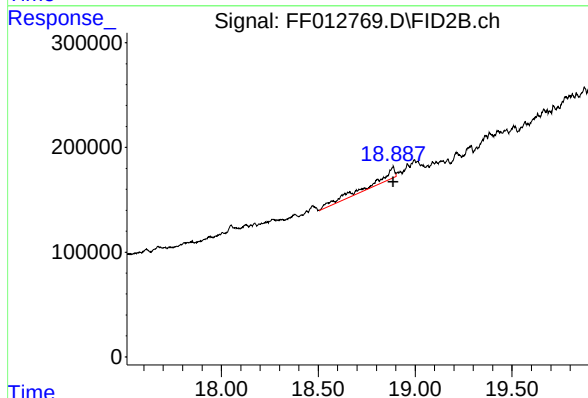


#14 N-DOTRIACONTANE

R.T.: 18.887 min
Delta R.T.: 0.000 min
Response: 816217
Conc: 6.83 ug/ml

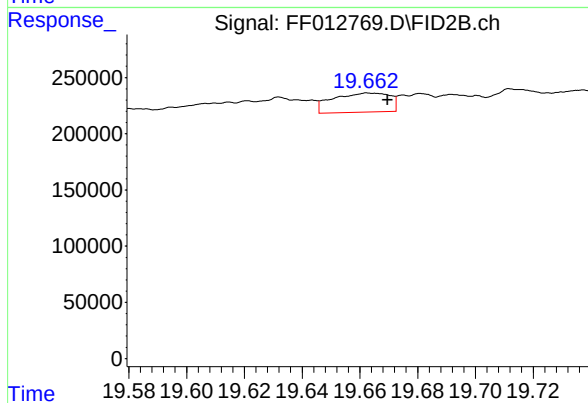

#15 N-TETRATRIACONTANE

R.T.: 19.663 min
Delta R.T.: -0.006 min
Response: 234541
Conc: 2.13 ug/ml

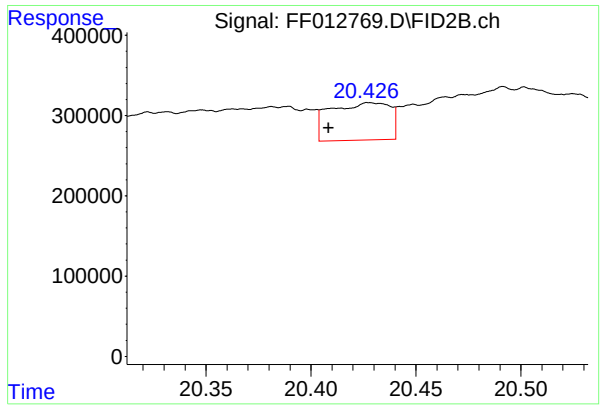

#16 N-HEXATRIACONTANE

R.T.: 20.428 min
Delta R.T.: 0.019 min
Response: 927621
Conc: 8.91 ug/ml

Instrument :

FID_F

ClientSampleId :